



Acrolein

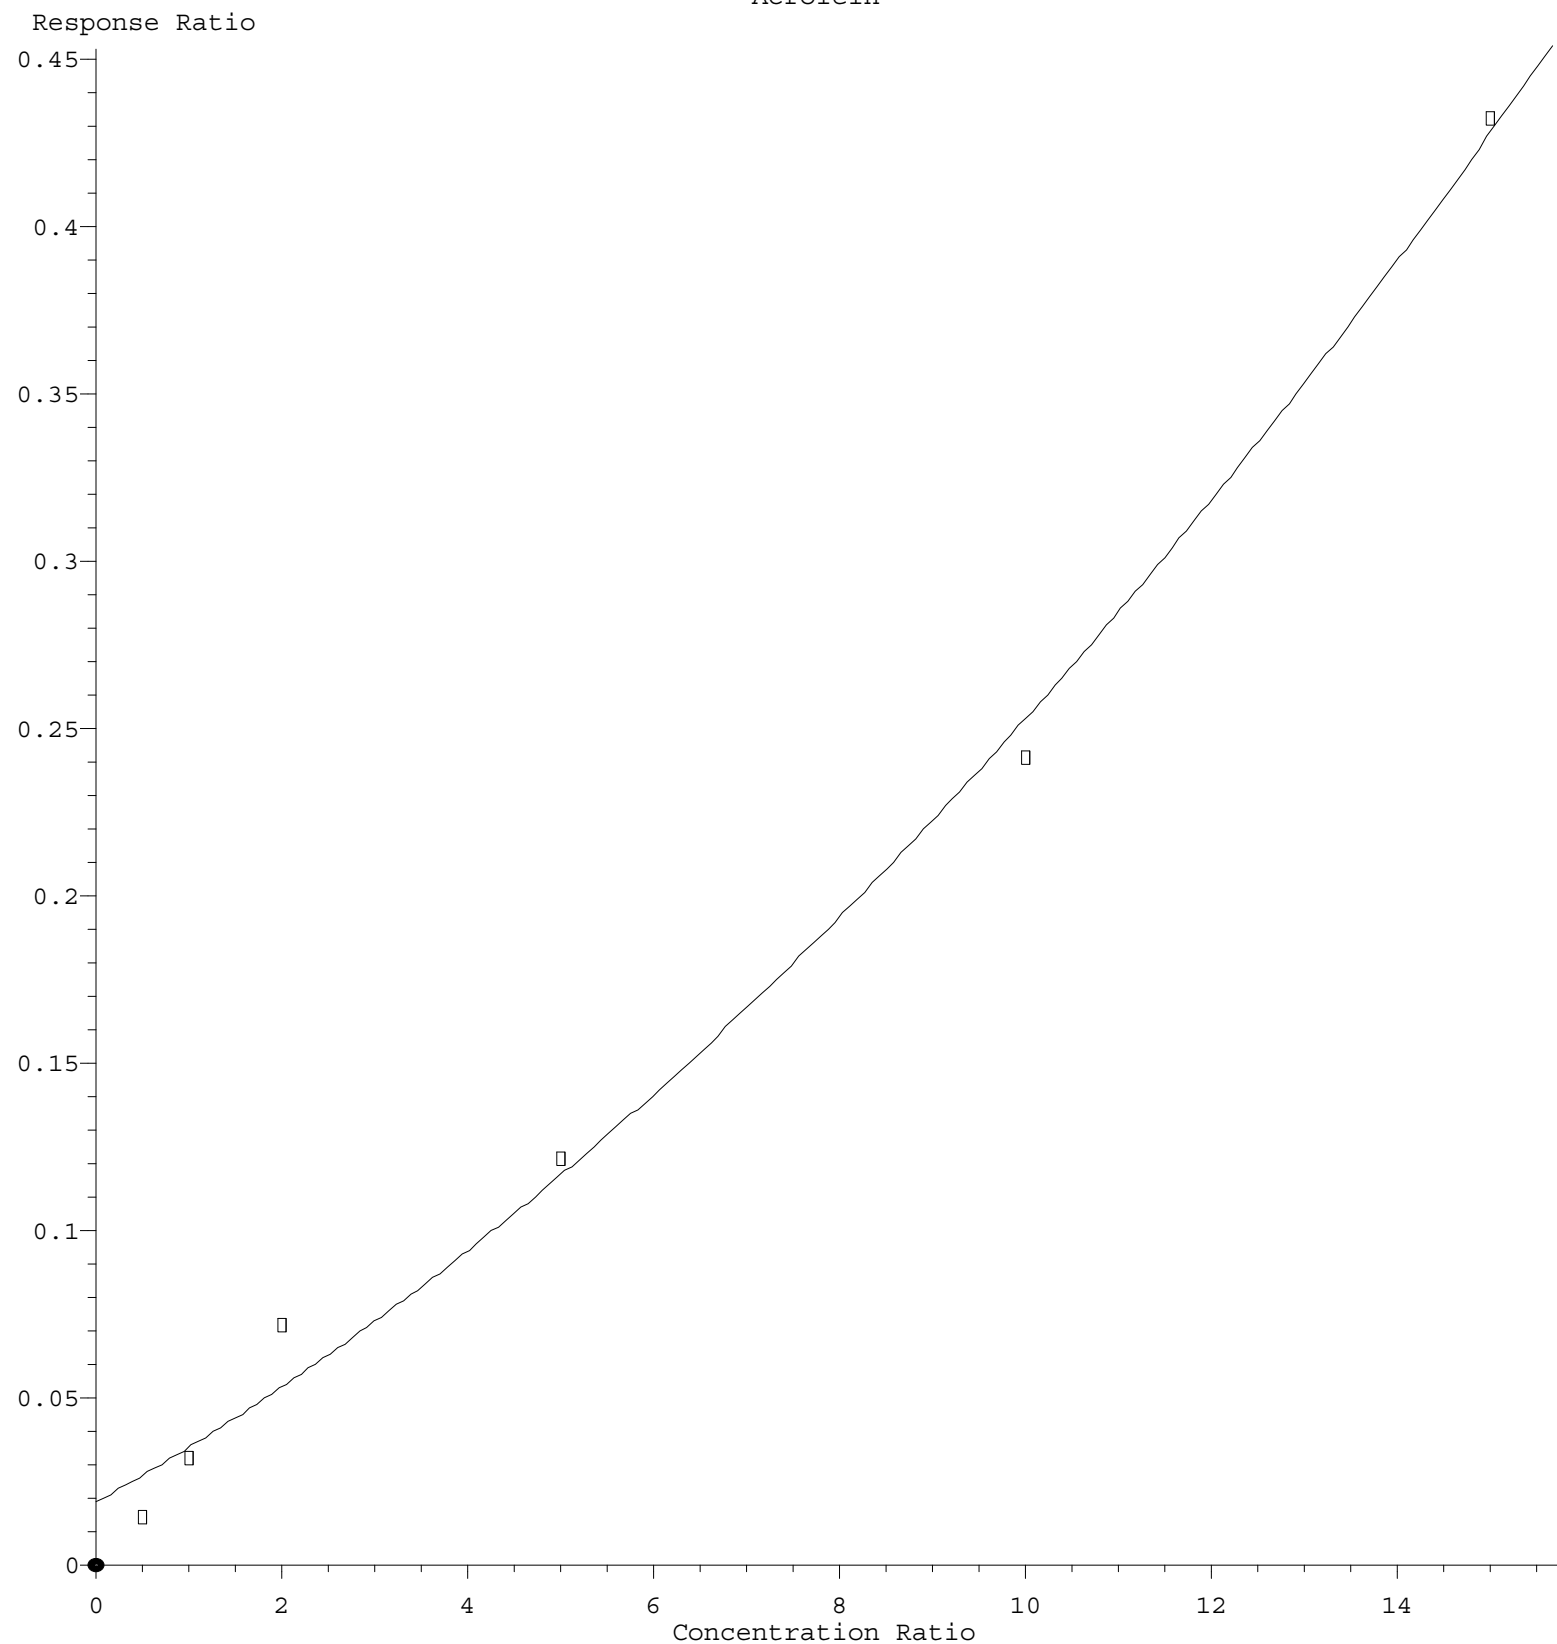

$R = 7.733e-004 A^2 + 1.567e-002 A + 1.889e-002$
 Coef of Det (r^2) = 0.994608 Curve Fit: Quadratic
 Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W010422S.M
 Calibration Table Last Updated: Tue Jan 04 06:15:33 2022


Dichlorodifluoromethane

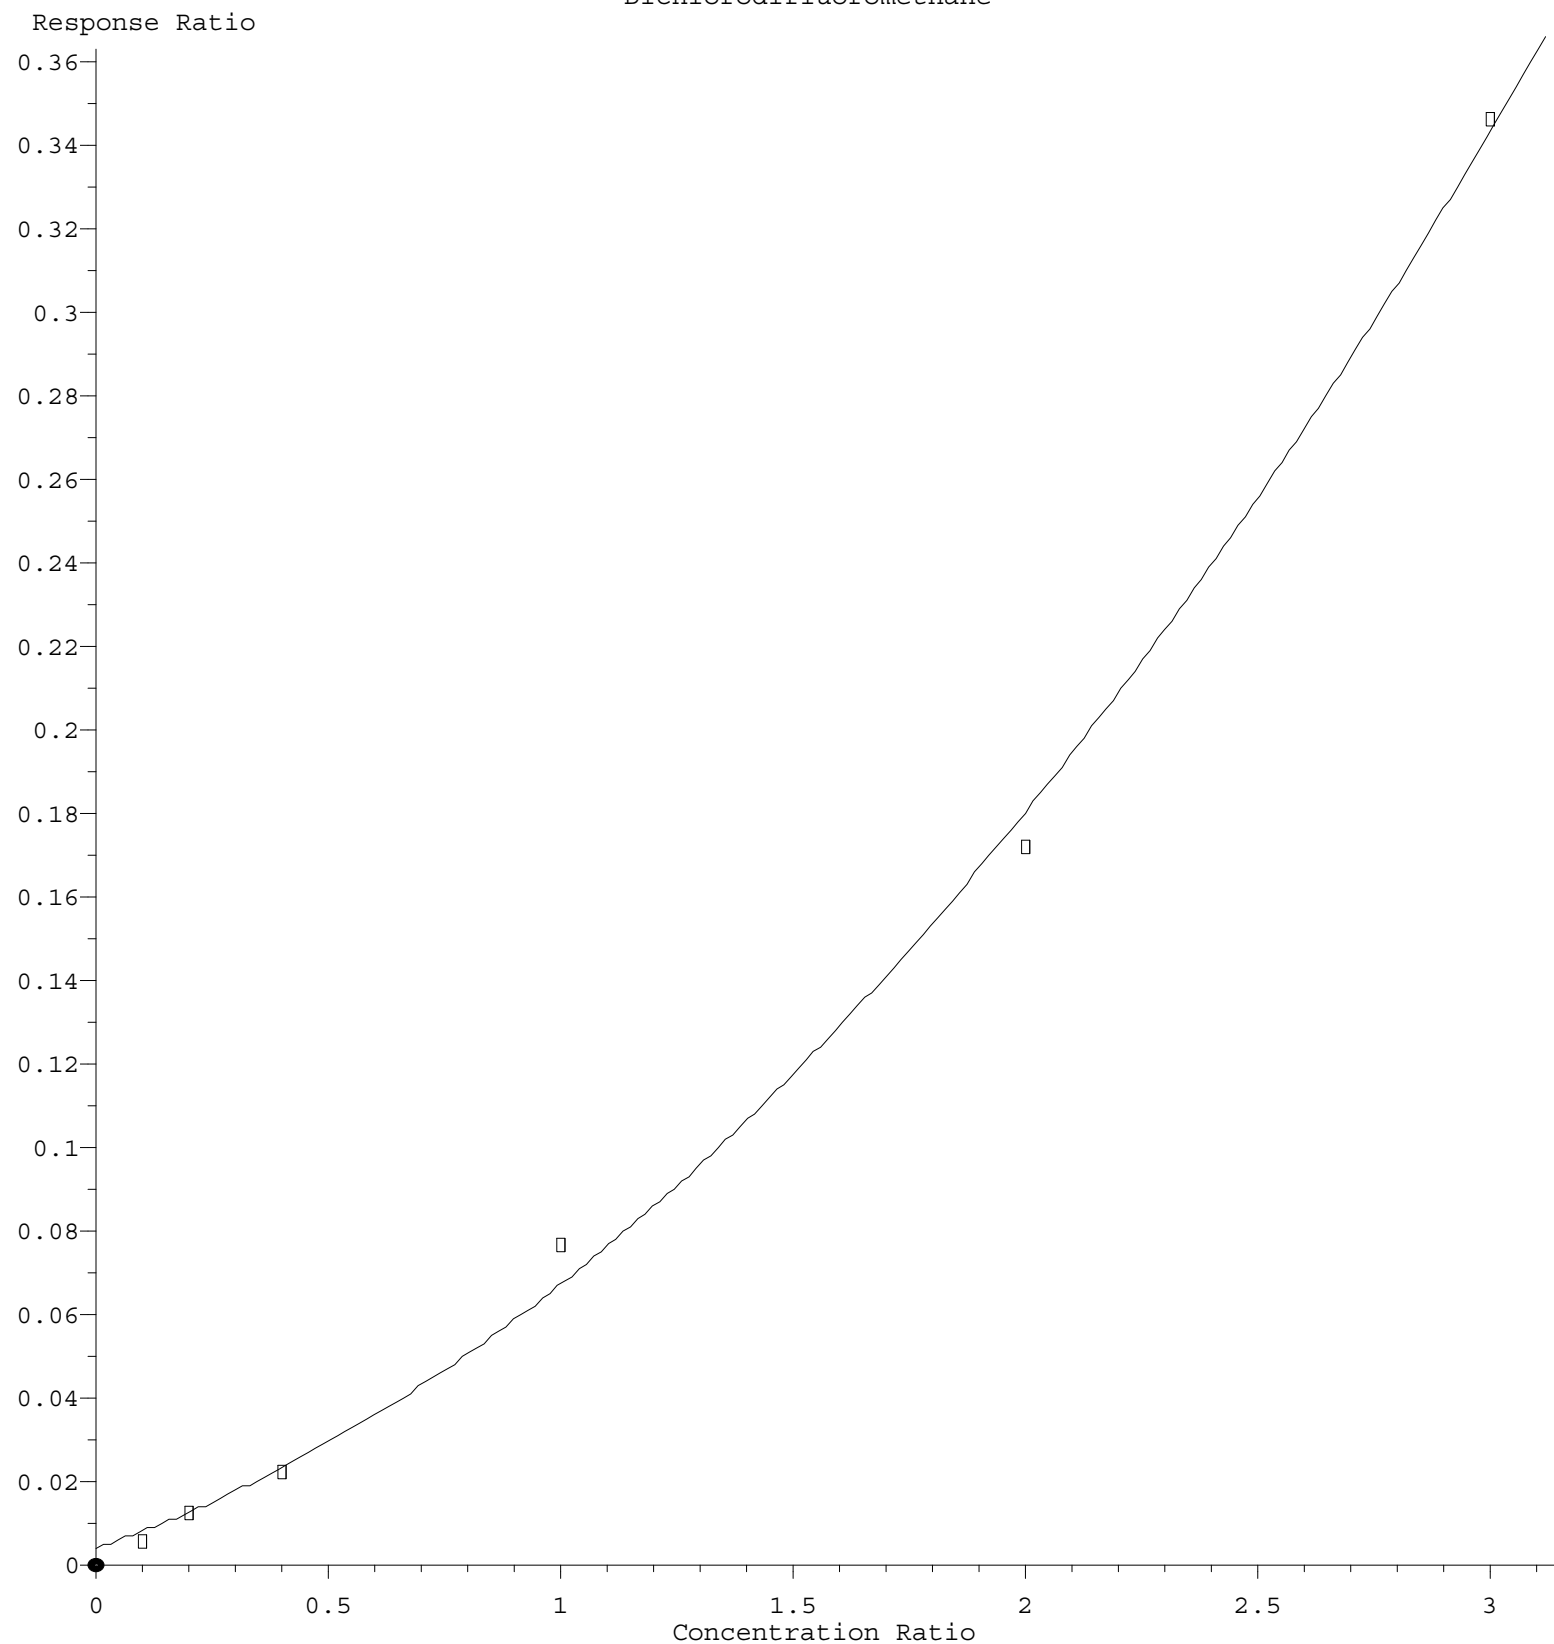

$R = 2.496e-002 A^2 + 3.828e-002 A + 4.030e-003$
 Coef of Det (r^2) = 0.998039 Curve Fit: Quadratic
 Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W010422S.M
 Calibration Table Last Updated: Tue Jan 04 06:15:33 2022

Methylene Chloride

Response Ratio

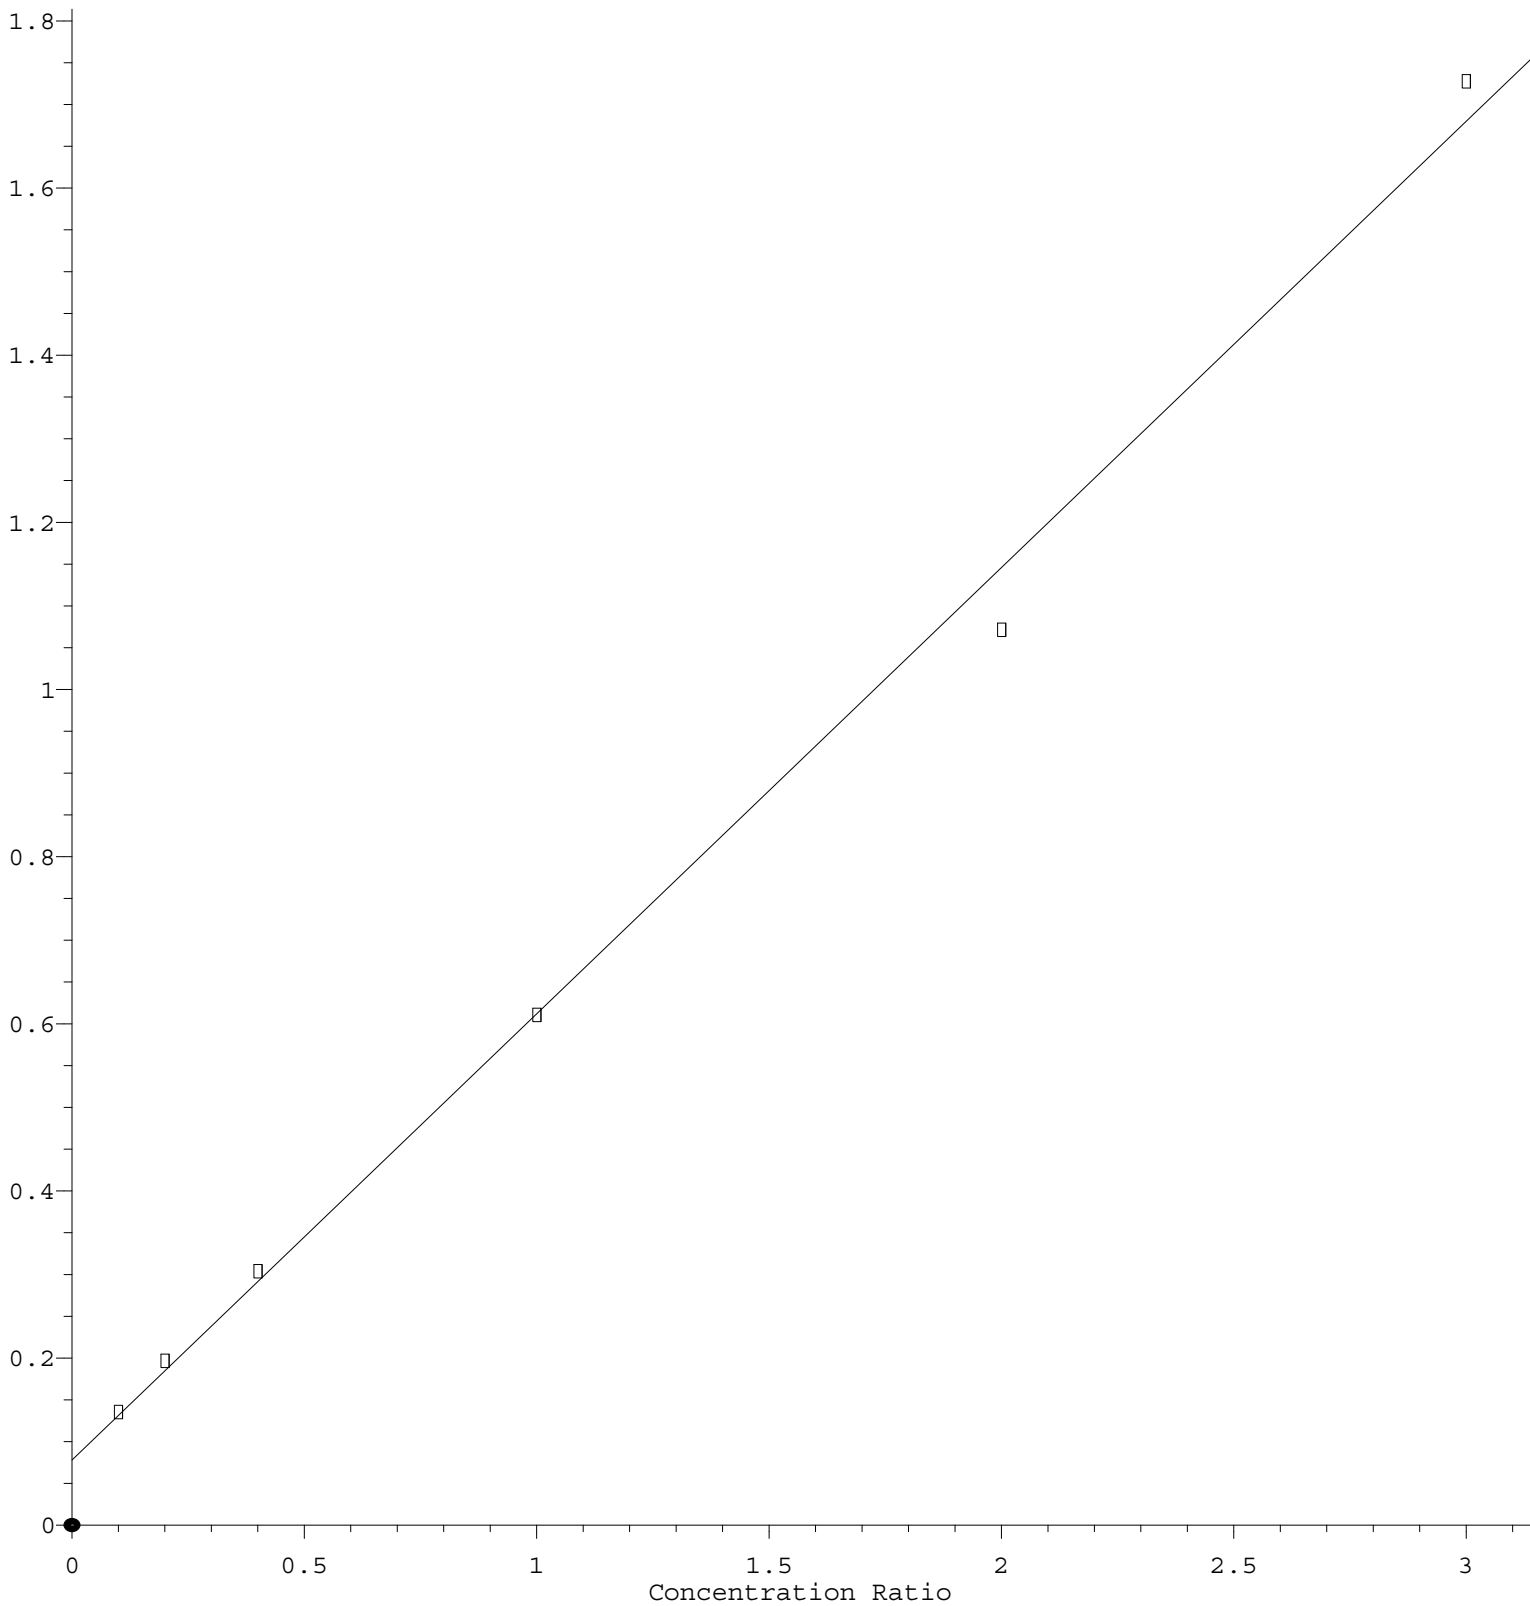

$$\text{Response} = 5.340\text{e-}001 * \text{Amt} + 7.787\text{e-}002$$


Coef of Det (r^2) = 0.995765 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W010422S.M

Calibration Table Last Updated: Tue Jan 04 06:15:33 2022

Trichlorofluoromethane

Response Ratio

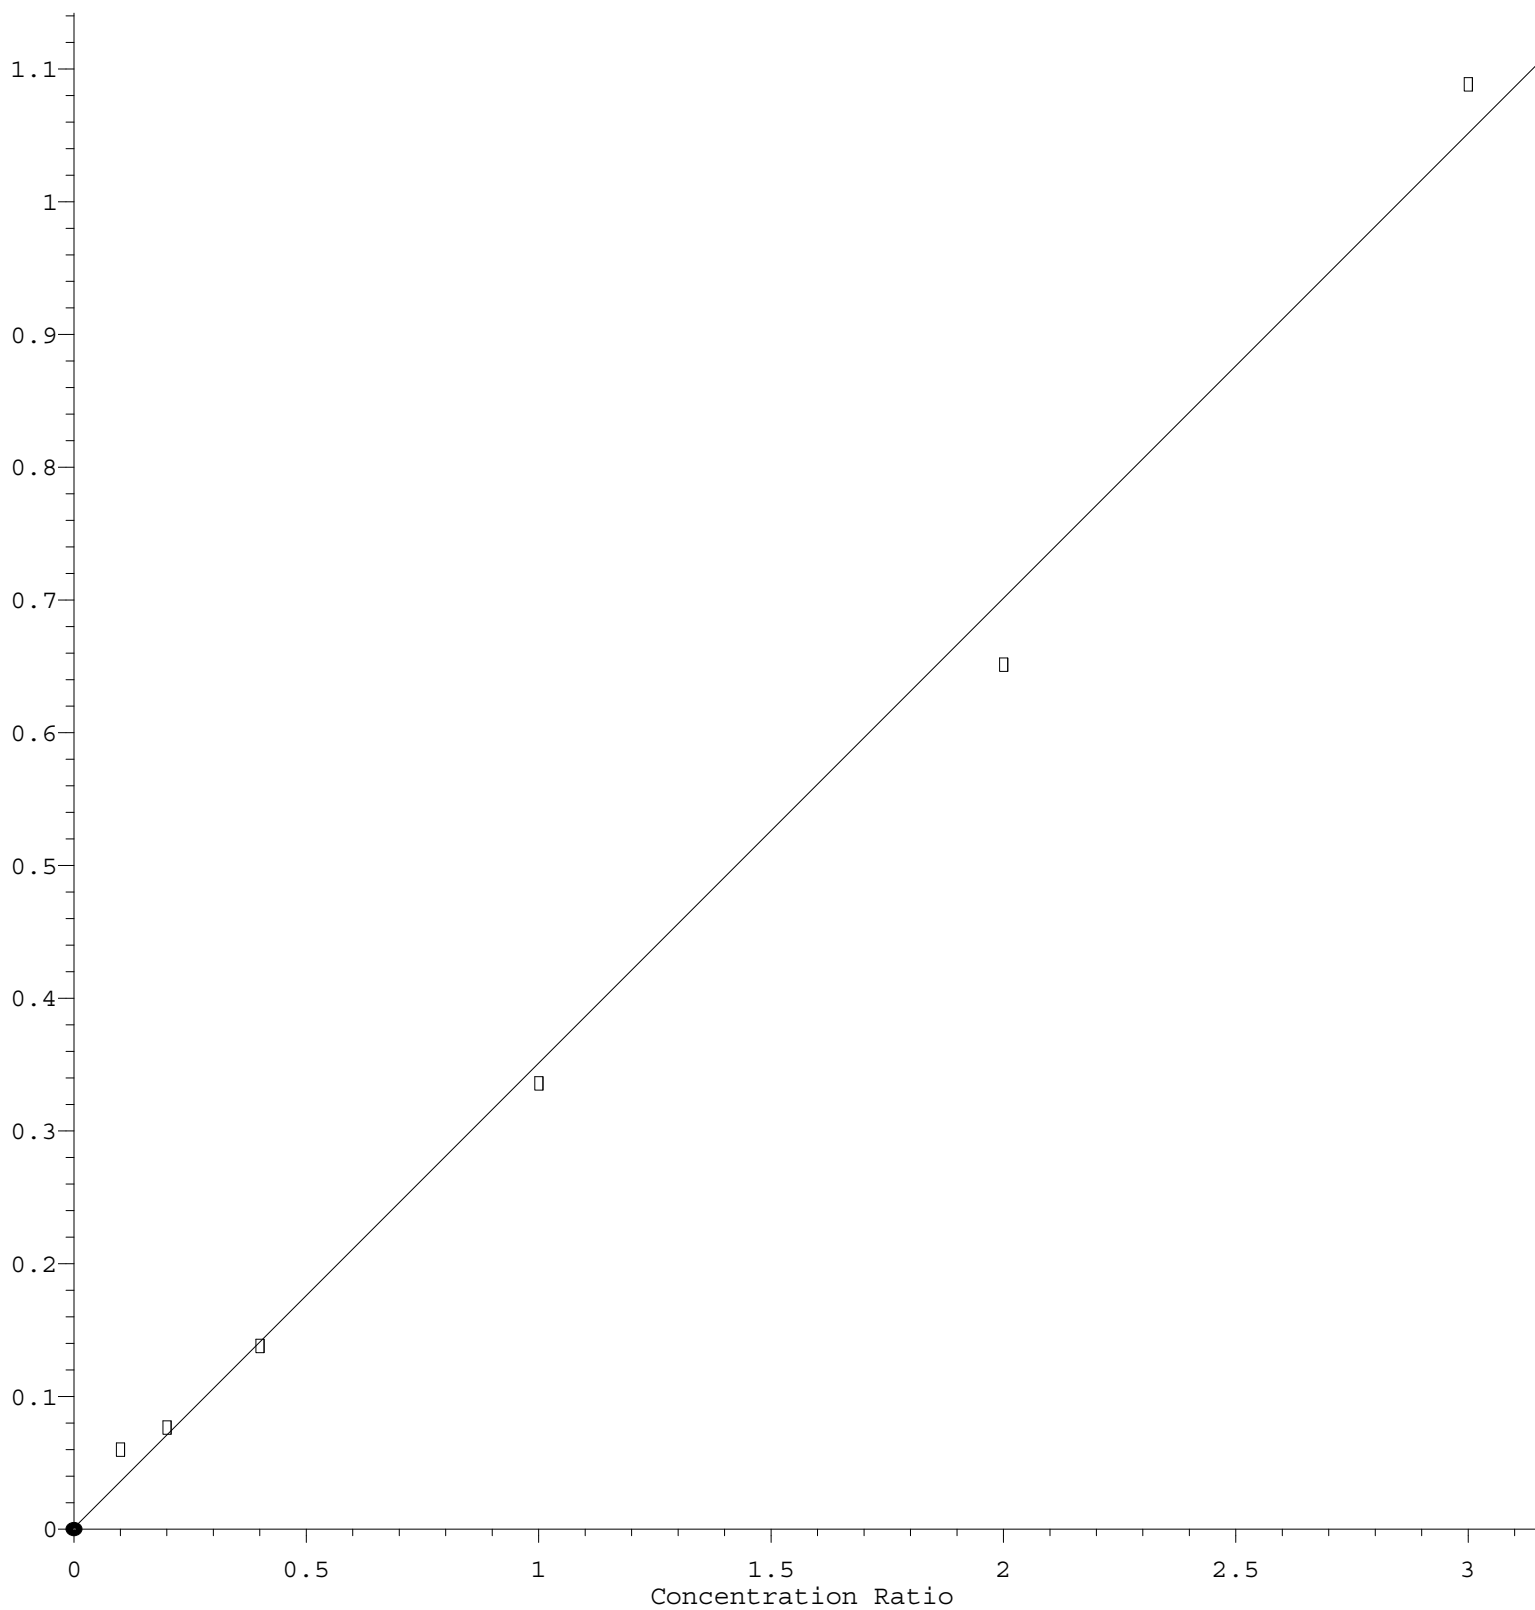


$$\text{Response} = 3.502\text{e-}001 * \text{Amt} + 6.250\text{e-}004$$

Coef of Det (r^2) = 0.994321 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W010422S.M


Calibration Table Last Updated: Tue Jan 04 06:15:33 2022

Bromoform

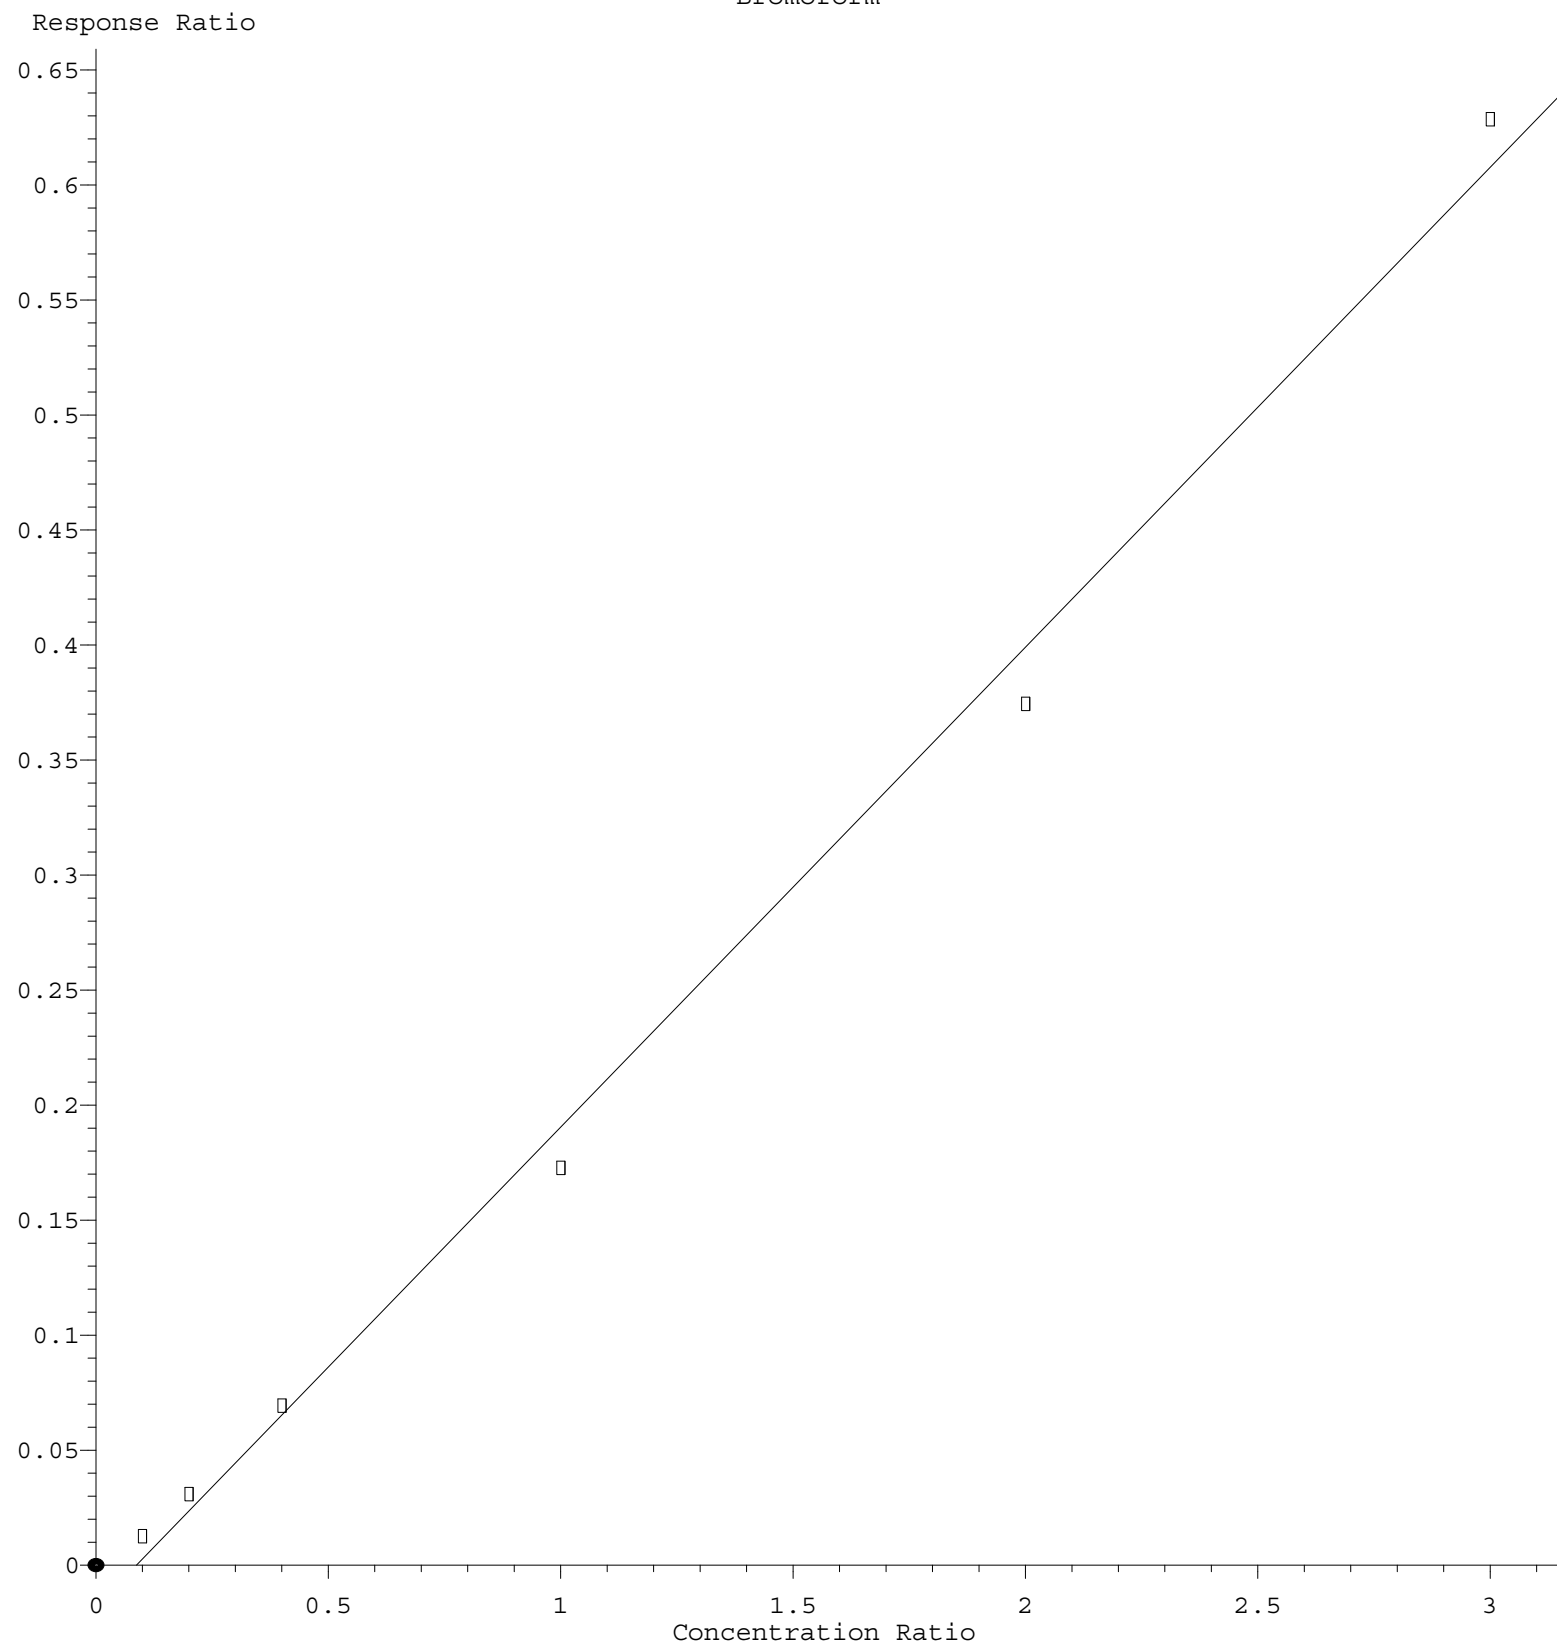

$\text{Response} = 2.086\text{e-}001 * \text{Amt} - 1.820\text{e-}002$
 Coef of Det (r^2) = 0.994822 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W010422S.M
 Calibration Table Last Updated: Tue Jan 04 06:15:33 2022

trans-1,4-Dichloro-2-butene

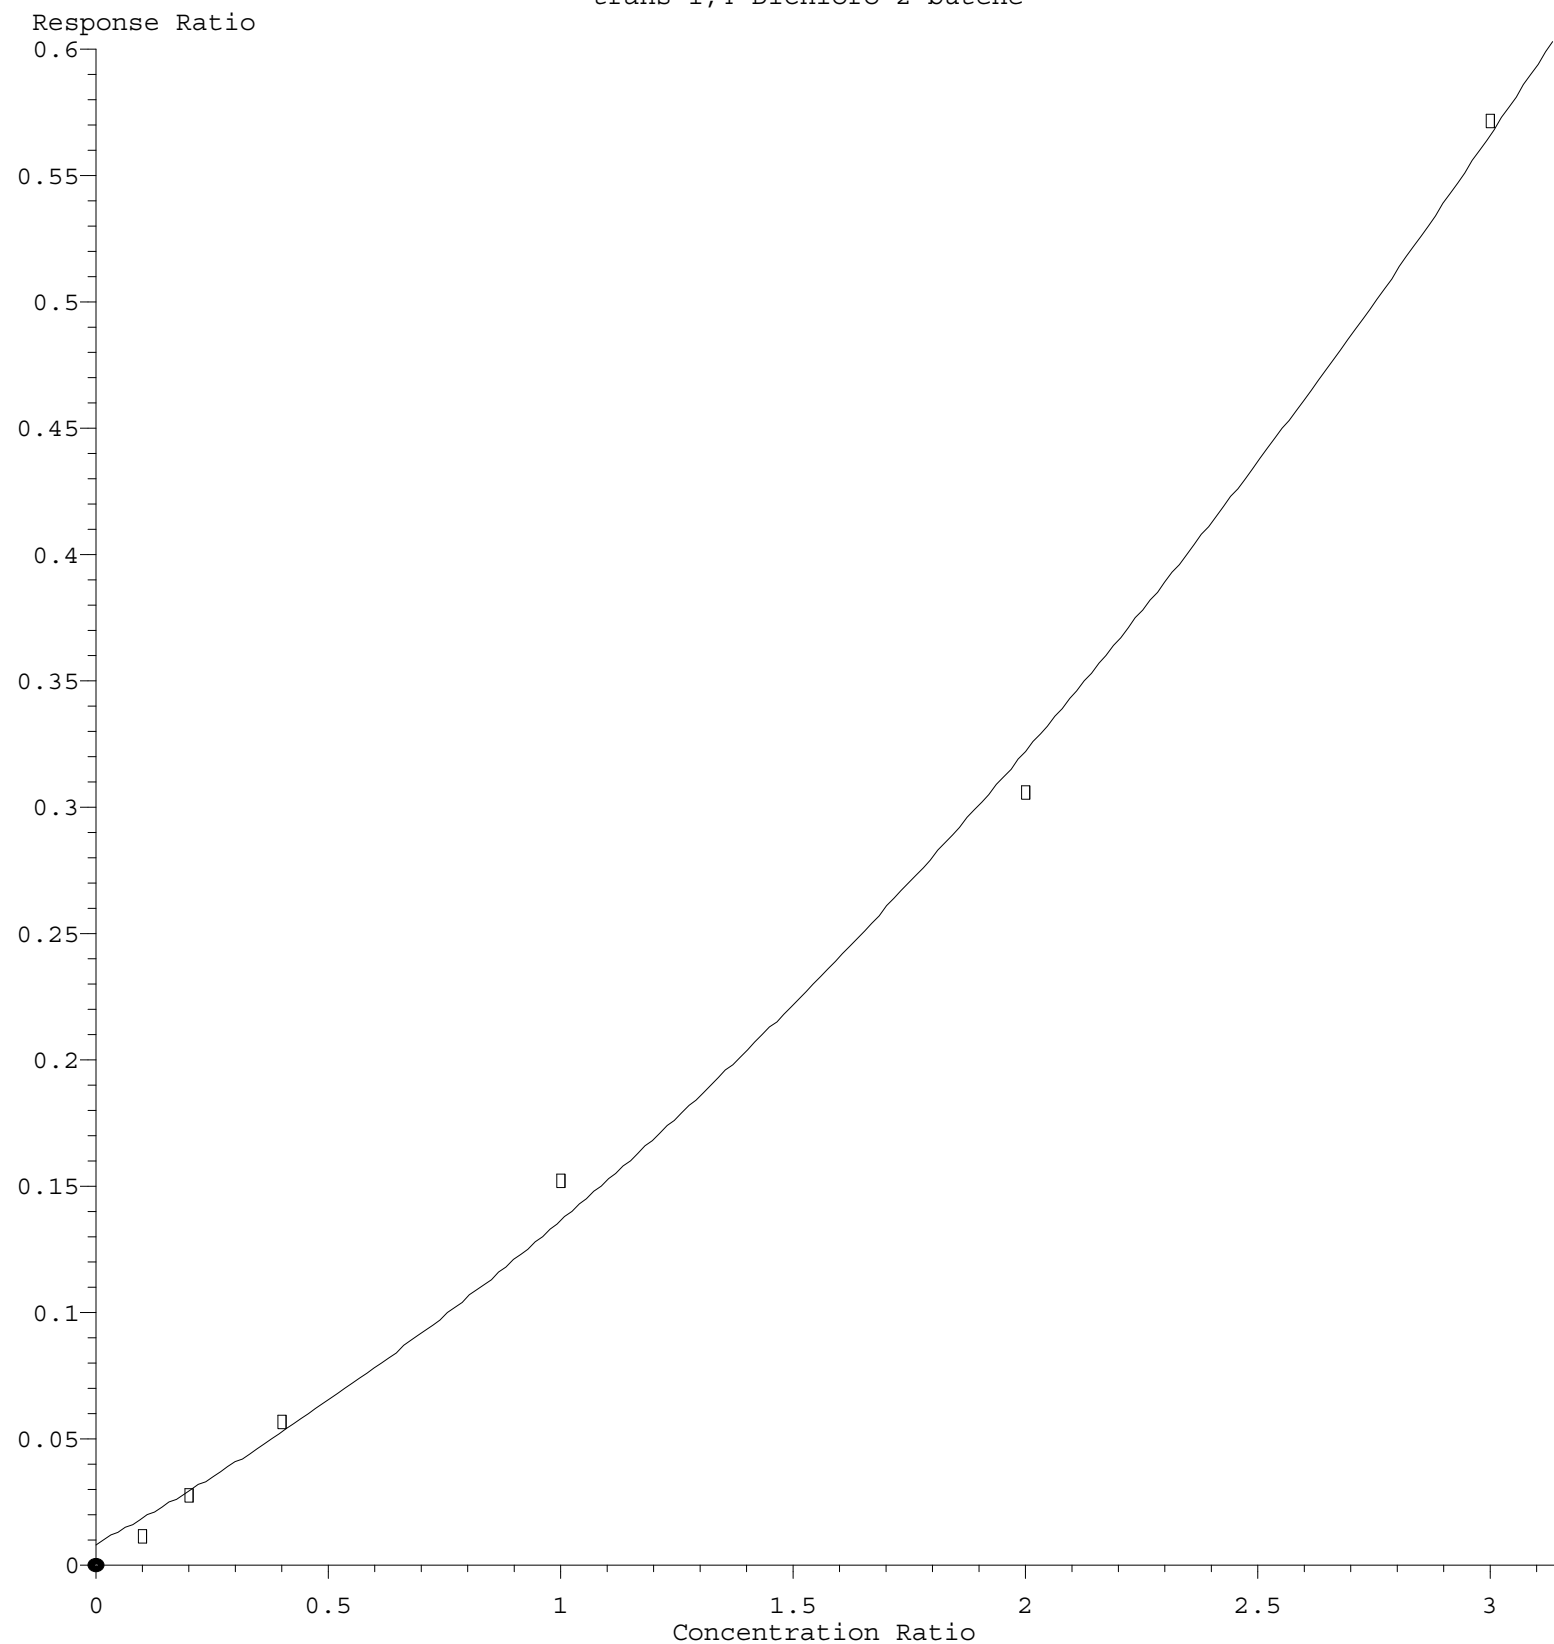

$R = 2.903e-002 A^2 + 9.880e-002 A + 8.452e-003$
Coef of Det (r^2) = 0.997381 Curve Fit: Quadratic
Method Name: Z:\voasrv\HPCHEM1\MSVOA W\Method\82W010422S.M
Calibration Table Last Updated: Tue Jan 04 06:15:33 2022