
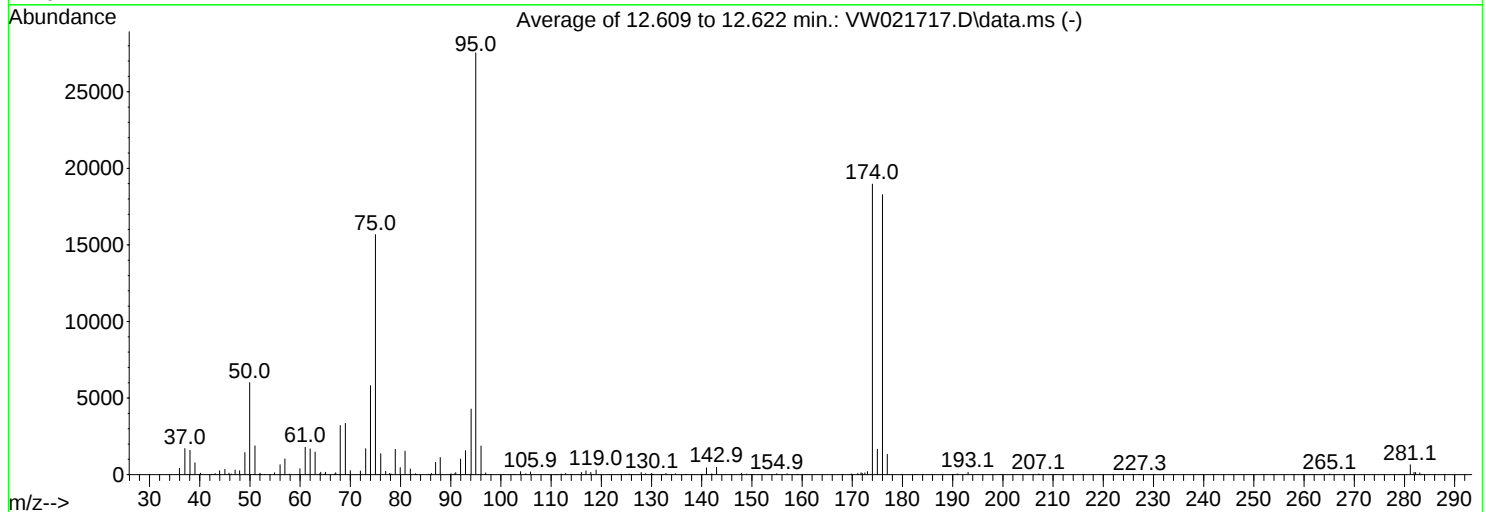


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW010422\
 Data File : VW021717.D
 Acq On : 03 Jan 2022 18:48
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00g/5.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W010422S.M
 Title : SW846 8260
 Last Update : Tue Jan 04 06:15:33 2022

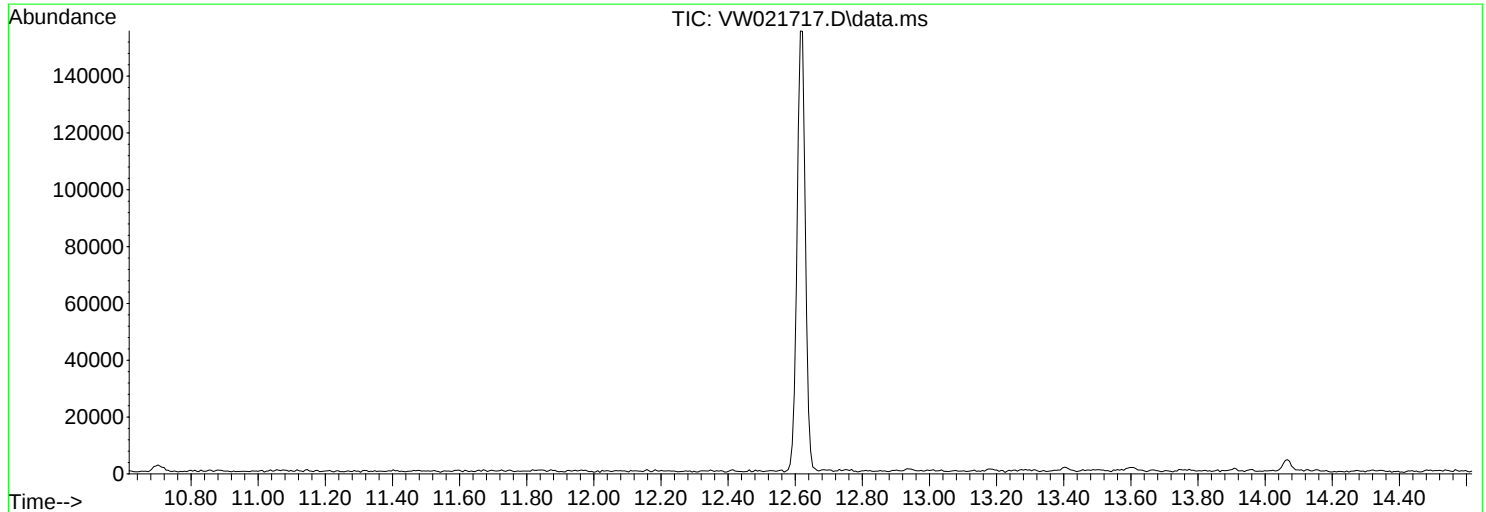

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.8	6010	PASS
75	95	30	60	56.9	15673	PASS
95	95	100	100	100.0	27539	PASS
96	95	5	9	6.8	1868	PASS
173	174	0.00	2	1.0	197	PASS
174	95	50	100	68.9	18973	PASS
175	174	5	9	8.8	1665	PASS
176	174	95	101	96.3	18278	PASS
177	176	5	9	7.3	1328	PASS