


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW010620\
 Data File : VW014516.D
 Acq On : 06 Jan 2020 09:34
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W010320S.M
 Title : SW846 8260
 Last Update : Fri Jan 03 16:07:20 2020

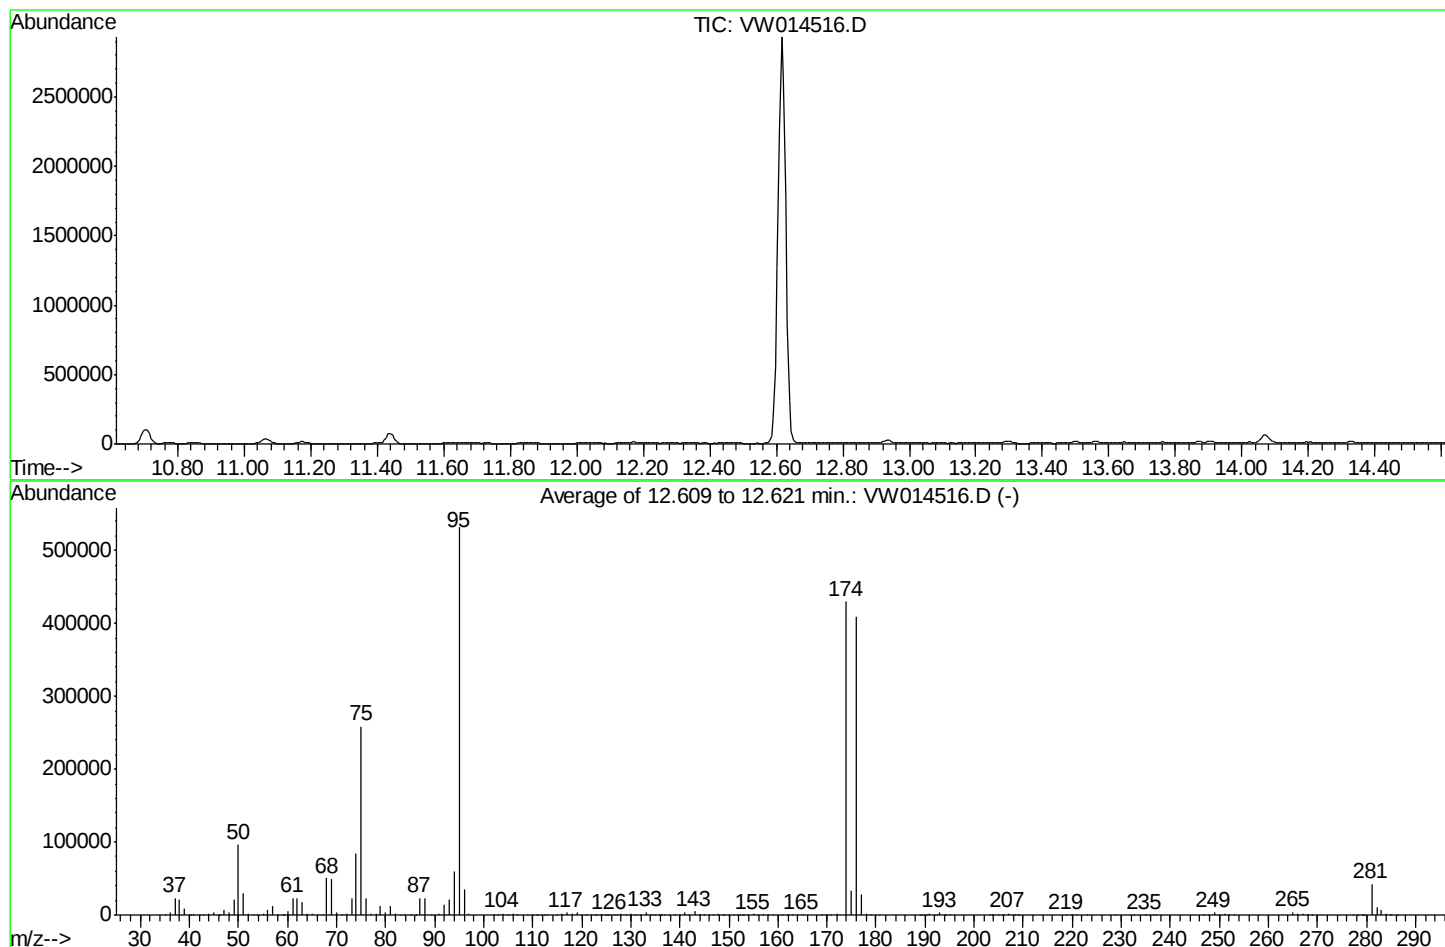

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1747

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	96042	PASS
75	95	30	60	48.6	258517	PASS
95	95	100	100	100.0	531776	PASS
96	95	5	9	6.7	35482	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	80.9	430016	PASS
175	174	5	9	7.9	33978	PASS
176	174	95	101	95.0	408618	PASS
177	176	5	9	7.0	28501	PASS