




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW010622\
 Data File : VW021761.D
 Acq On : 06 Jan 2022 16:44
 Operator : SY/VA
 Sample : N1025-01
 Misc : 5.87g/10mL/MSVOA_W/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLG5

Manual IntegrationsAPPROVED

Quant Time: Jan 07 00:22:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jan 04 00:22:49 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/11/2022
 Supervised By :Mahesh Dadoda 01/12/2022

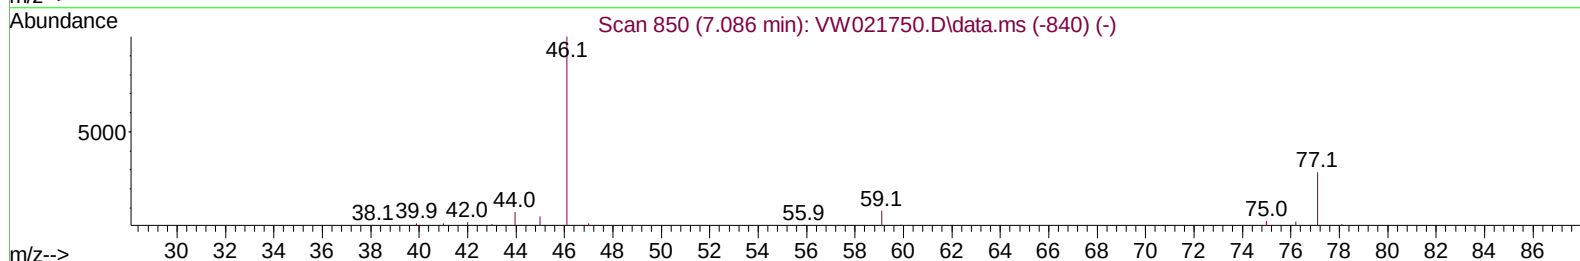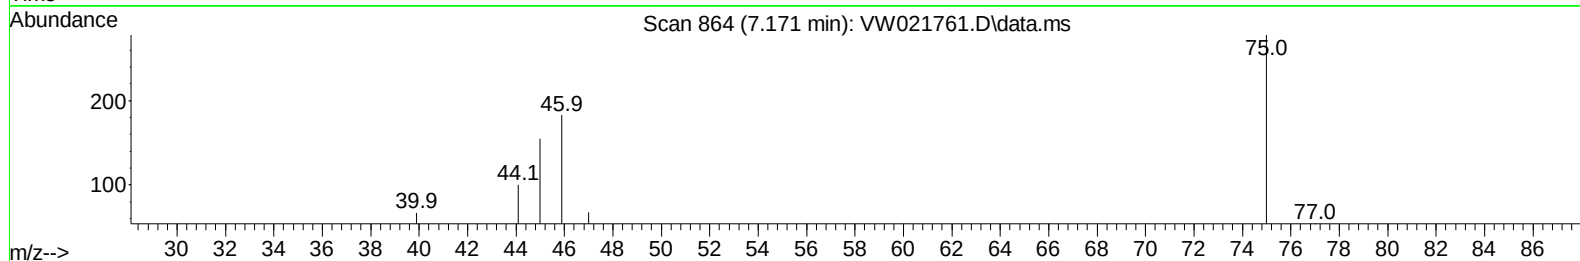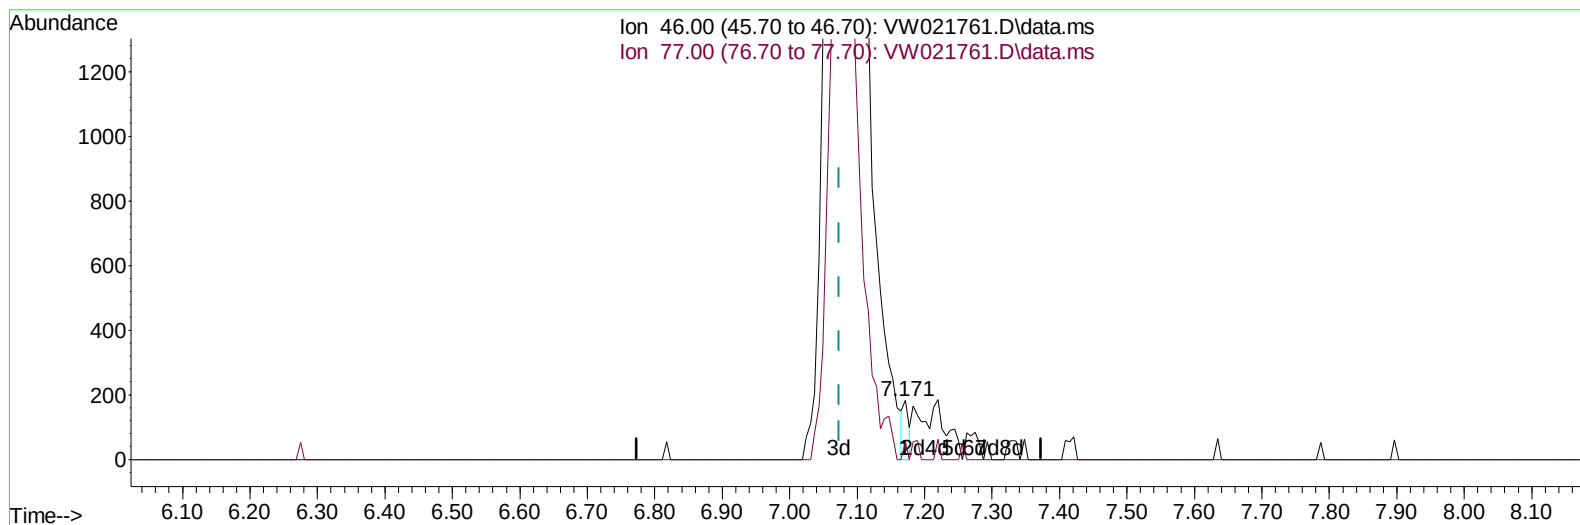

TIC: VW021761.D\data.ms

(21) 2-Butanone-d5 (S)

7.171min (+ 0.098) 0.20 ug/L

response 103

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	20.20	19.42
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW010622\
 Data File : VW021761.D
 Acq On : 06 Jan 2022 16:44
 Operator : SY/VA
 Sample : N1025-01
 Misc : 5.87g/10mL/MSVOA_W/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLG5

Manual IntegrationsAPPROVED

Quant Time: Jan 07 00:22:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jan 04 00:22:49 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/11/2022
 Supervised By :Mahesh Dadoda 01/12/2022

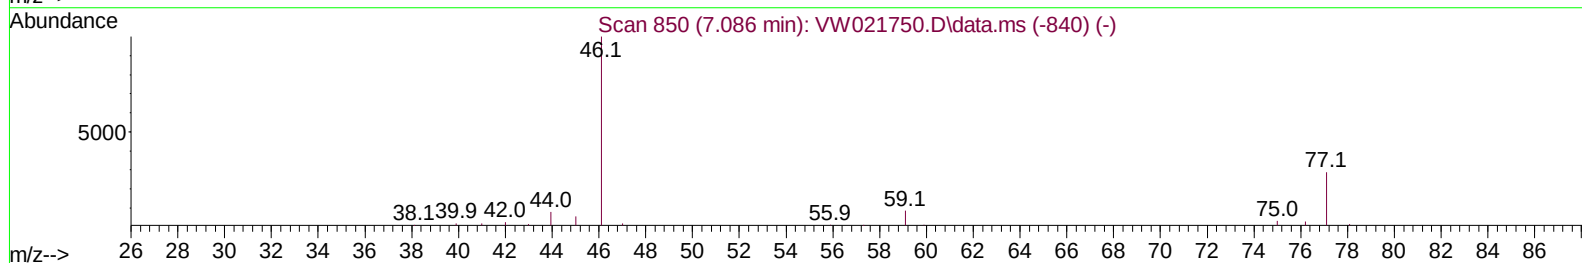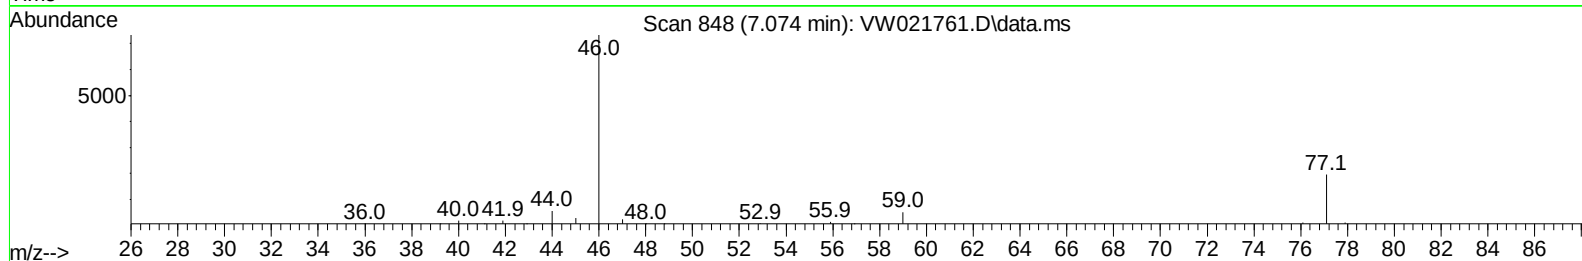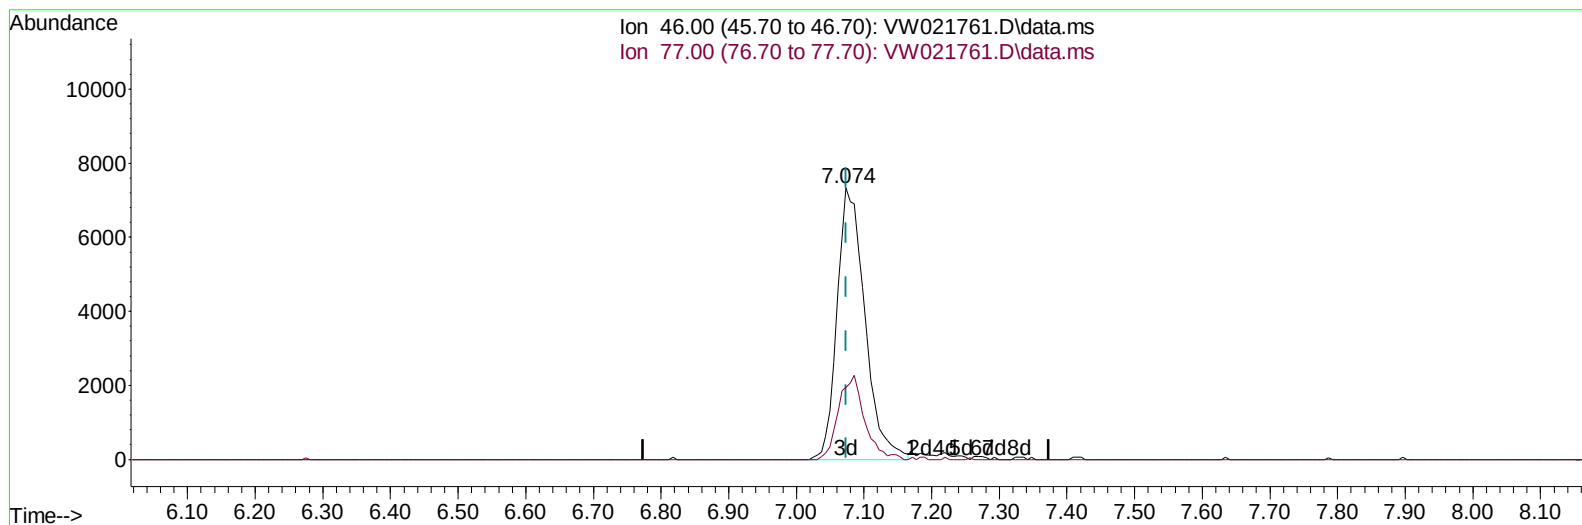

TIC: VW021761.D\data.ms

(21) 2-Butanone-d5 (S)

7.074min (-0.000) 39.70 ug/L m

response 20932

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	20.20	0.10#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW010622\
 Data File : VW021761.D
 Acq On : 06 Jan 2022 16:44
 Operator : SY/VA
 Sample : N1025-01
 Misc : 5.87g/10mL/MSVOA_W/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLG5

Manual IntegrationsAPPROVED

Quant Time: Jan 07 00:22:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jan 04 00:22:49 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/11/2022
 Supervised By :Mahesh Dadoda 01/12/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	182779	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117	171148	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	97265	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	57252	15.887	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	63.560%	
7) Chloroethane-d5	2.885	69	39925	16.449	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	65.800%	
11) 1,1-Dichloroethene-d2	4.013	63	69161	13.114	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	52.440%	
21) 2-Butanone-d5	7.074	46	20932m	39.701	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	79.400%	
24) Chloroform-d	7.653	84	110010	19.268	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	77.080%	
26) 1,2-Dichloroethane-d4	8.305	65	57078	18.932	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	75.720%	
32) Benzene-d6	8.275	84	221599	21.806	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	87.240%	
36) 1,2-Dichloropropane-d6	9.274	67	59950	21.746	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	87.000%	
41) Toluene-d8	10.323	98	222971	22.021	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	88.080%	
43) trans-1,3-Dichloroprop...	10.579	79	24040	17.921	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	71.680%	
47) 2-Hexanone-d5	10.920	63	18104	43.301	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	86.600%	
56) 1,1,2,2-Tetrachloroeth...	12.688	84	48058	21.145	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	84.560%	
66) 1,2-Dichlorobenzene-d4	13.853	152	83514	22.453	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	89.800%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW010622\
Data File : VW021761.D
Acq On : 06 Jan 2022 16:44
Operator : SY/VA
Sample : N1025-01
Misc : 5.87g/10mL/MSVOA_W/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLG5

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/11/2022
Supervised By :Mahesh Dadoda 01/12/2022

Quant Time: Jan 07 00:22:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jan 04 00:22:49 2022
Response via : Initial Calibration

