

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW010622\
 Data File : VW021757.D
 Acq On : 06 Jan 2022 15:08
 Operator : SY/VA
 Sample : N1009-05
 Misc : 6.42g/10mL/MSVOA_W/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLG1

Quant Time: Jan 06 16:31:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jan 04 00:22:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	56130	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117	56263	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	30669	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	16092	14.541	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	58.160%
7) Chloroethane-d5	2.891	69	12510	16.783	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	67.120%
11) 1,1-Dichloroethene-d2	4.019	63	21281	13.140	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	52.560%
21) 2-Butanone-d5	7.073	46	6869	42.424	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	84.840%
24) Chloroform-d	7.659	84	31732	18.098	ug/L	0.01
Spiked Amount	25.000	Range	40 - 150	Recovery	=	72.400%
26) 1,2-Dichloroethane-d4	8.311	65	17401	18.795	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	75.160%
32) Benzene-d6	8.274	84	64386	19.273	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	77.080%
36) 1,2-Dichloropropane-d6	9.274	67	17843	19.688	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	78.760%
41) Toluene-d8	10.323	98	61792	18.564	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	74.240%
43) trans-1,3-Dichloroprop...	10.579	79	6755	15.318	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	61.280%
47) 2-Hexanone-d5	10.926	63	5122	37.266	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	74.540%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	15742	21.069	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	84.280%
66) 1,2-Dichlorobenzene-d4	13.853	152	23280	19.850	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	79.400%
Target Compounds						Qvalue
16) Methylene chloride	4.921	84	5725	5.714	ug/L	77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW010622\
Data File : VW021757.D
Acq On : 06 Jan 2022 15:08
Operator : SY/VA
Sample : N1009-05
Misc : 6.42g/10mL/MSVOA_W/SOIL
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLG1

Quant Time: Jan 06 16:31:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jan 04 00:22:49 2022
Response via : Initial Calibration

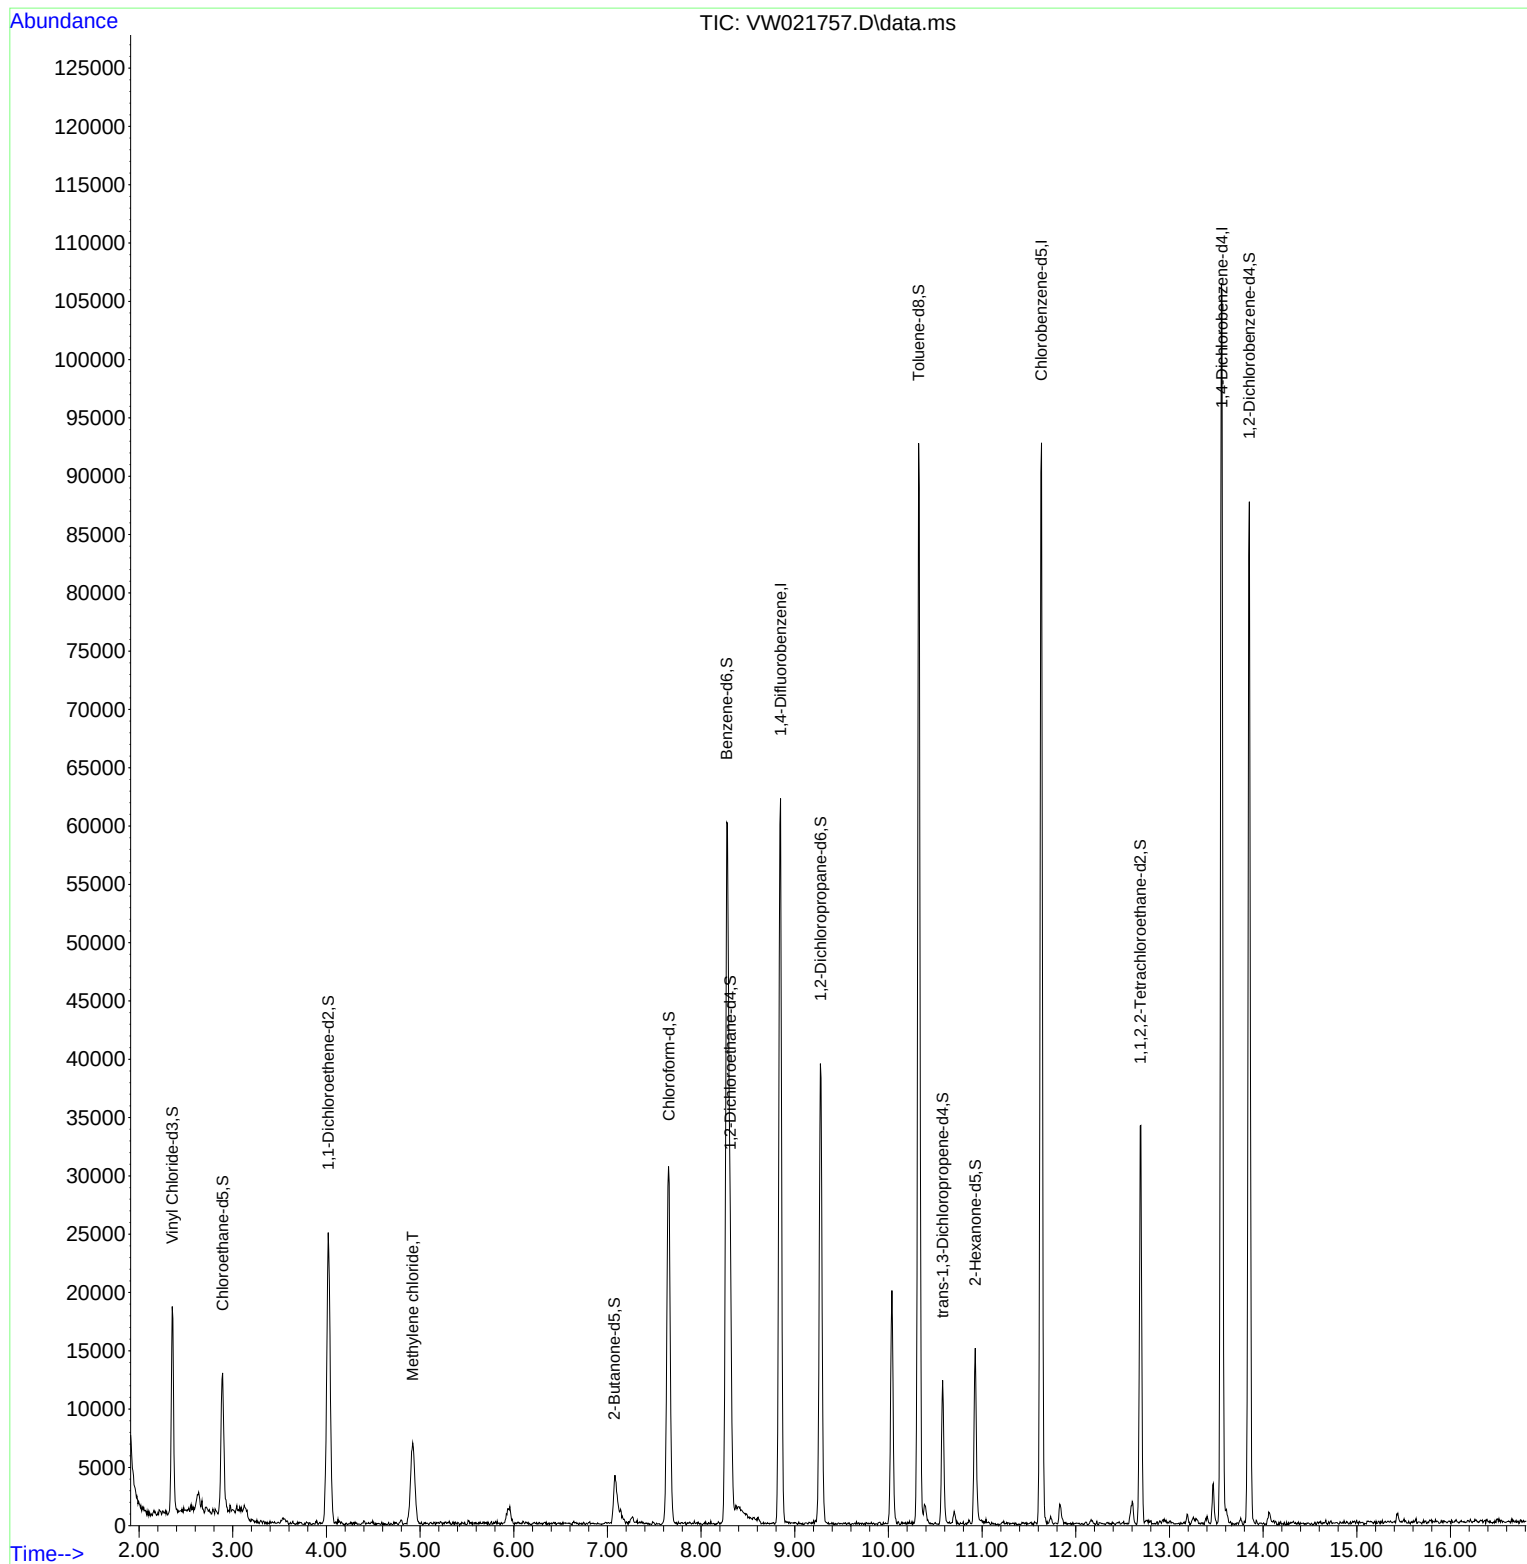

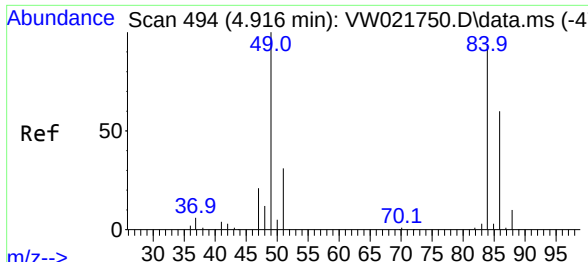

#16
Methylene chloride
Concen: 5.714 ug/L
RT: 4.921 min Scan# 49
Delta R.T. 0.012 min
Lab File: VW021757.D
Acq: 06 Jan 2022 15:08

Instrument :
MSVOA_W
ClientSampleId :
BGLG1

Tgt Ion: 84 Resp: 5725
Ion Ratio Lower Upper
84 100
86 57.4 45.5 84.5
49 107.0 100.5 186.7

