

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW010622\
 Data File : VW021758.D
 Acq On : 06 Jan 2022 15:32
 Operator : SY/VA
 Sample : N1009-06
 Misc : 7.68g/10mL/MSVOA_W/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLG2

Quant Time: Jan 06 16:31:20 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jan 04 00:22:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	145678	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117	144754	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	79666	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	41746	14.534	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	58.120%		
7) Chloroethane-d5	2.885	69	30674	15.856	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	63.440%		
11) 1,1-Dichloroethene-d2	4.019	63	51254	12.194	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	48.760%		
21) 2-Butanone-d5	7.092	46	18179	43.261	ug/L	0.02
Spiked Amount 50.000	Range 20 - 135		Recovery =	86.520%		
24) Chloroform-d	7.653	84	81870	17.991	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	71.960%		
26) 1,2-Dichloroethane-d4	8.305	65	44263	18.421	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	73.680%		
32) Benzene-d6	8.275	84	164149	19.098	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	76.400%		
36) 1,2-Dichloropropane-d6	9.275	67	44038	18.887	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	75.560%		
41) Toluene-d8	10.323	98	166850	19.483	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	77.920%		
43) trans-1,3-Dichloroprop...	10.579	79	18530	16.332	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	65.320%		
47) 2-Hexanone-d5	10.927	63	16281	46.041	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	92.080%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84	40888	21.270	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	85.080%		
66) 1,2-Dichlorobenzene-d4	13.853	152	62915	20.652	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	82.600%		
Target Compounds						Qvalue
16) Methylene chloride	4.916	84	12323	4.739	ug/L	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW010622\
Data File : VW021758.D
Acq On : 06 Jan 2022 15:32
Operator : SY/VA
Sample : N1009-06
Misc : 7.68g/10mL/MSVOA_W/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLG2


Quant Time: Jan 06 16:31:20 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM122821SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jan 04 00:22:49 2022
Response via : Initial Calibration

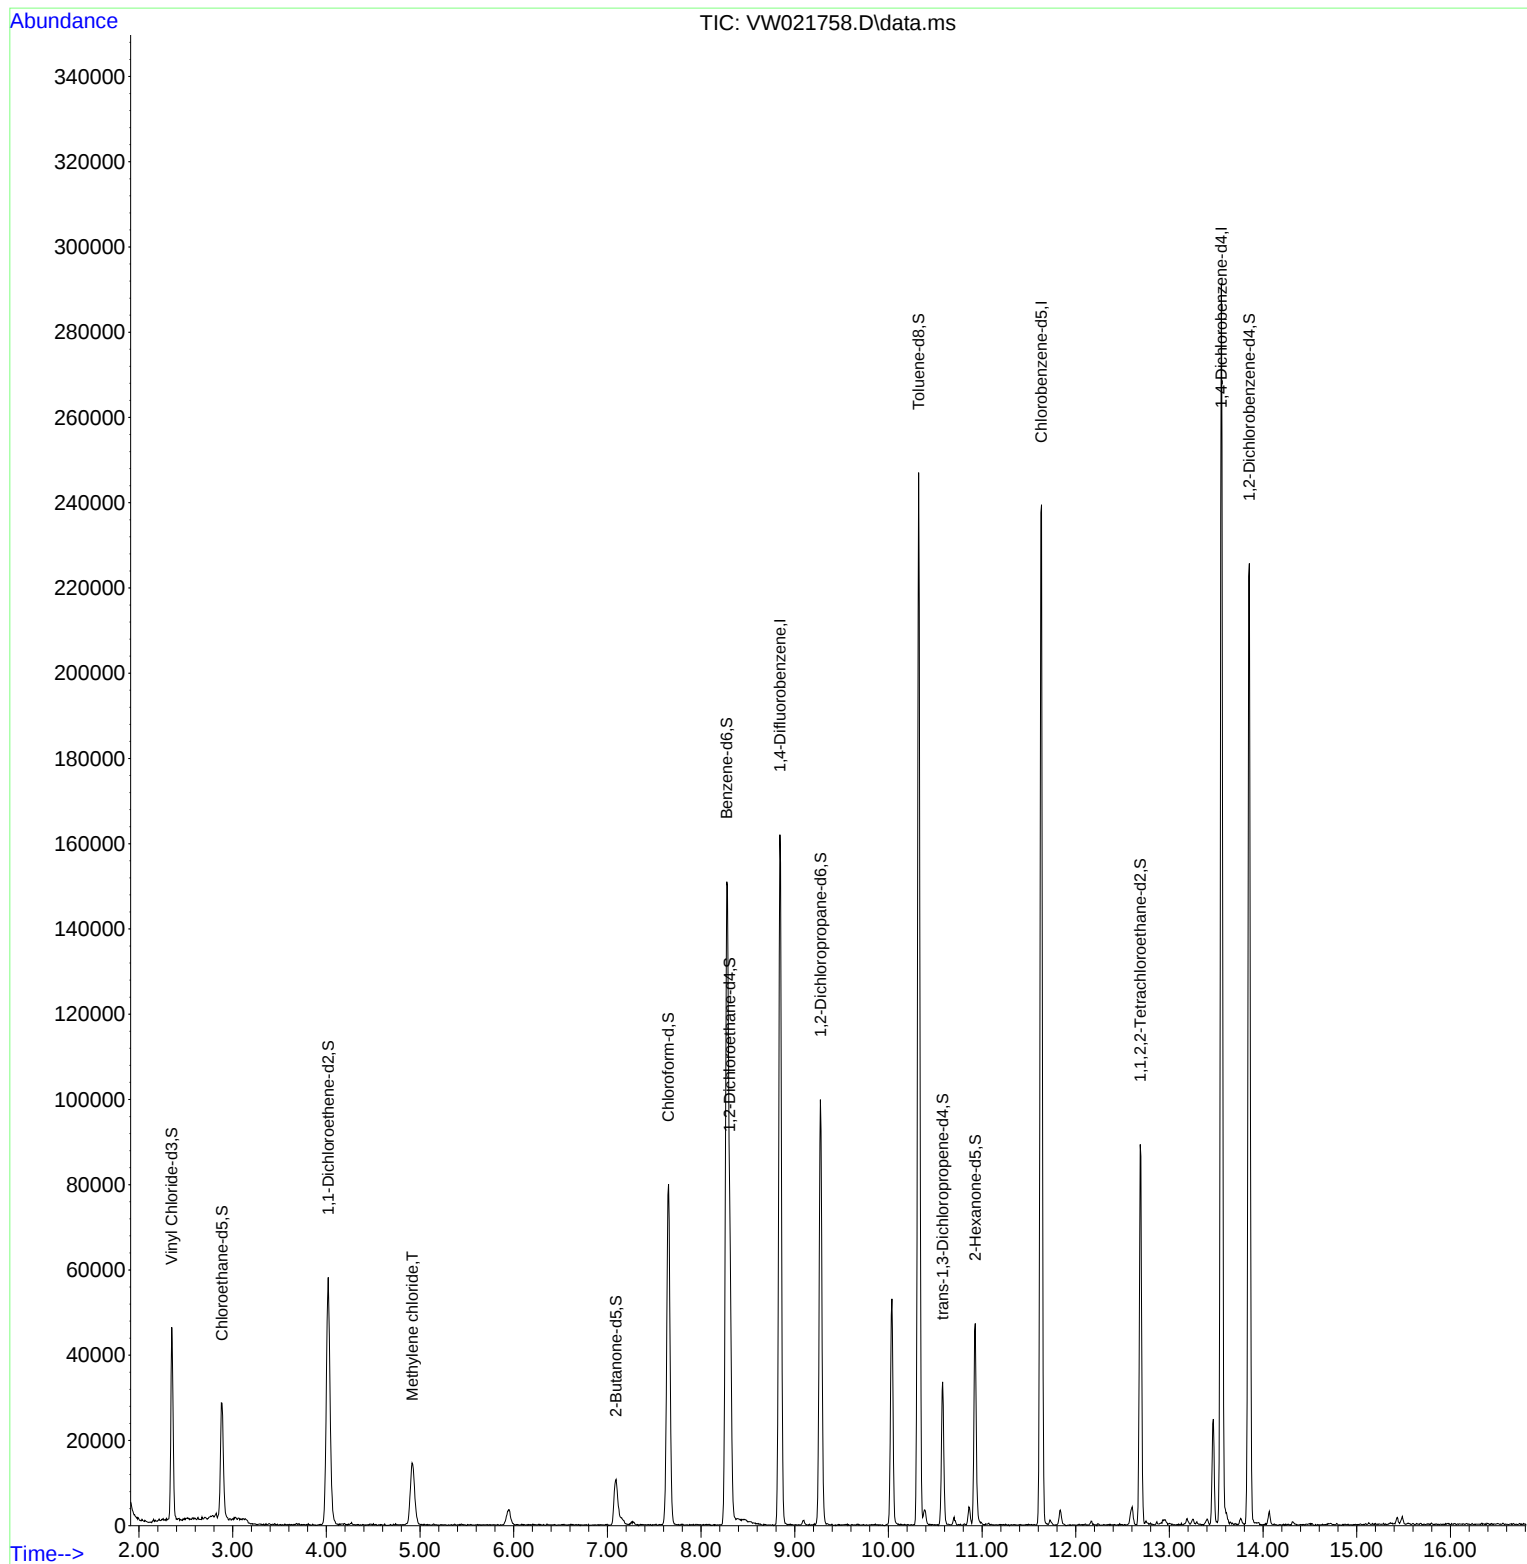

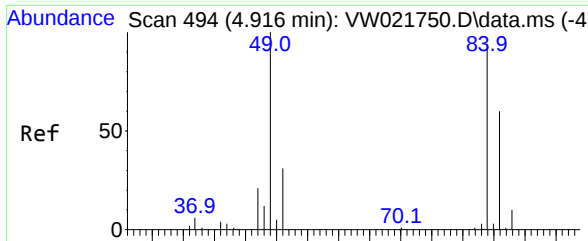

#16
Methylene chloride
Concen: 4.739 ug/L
RT: 4.916 min Scan# 49
Delta R.T. 0.006 min
Lab File: VW021758.D
Acq: 06 Jan 2022 15:32

Instrument :
MSVOA_W
ClientSampleId :
BGLG2

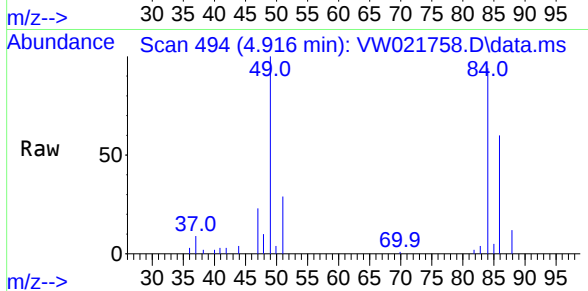

Tgt Ion:	84	Resp:	12323
Ion	Ratio	Lower	Upper
84	100		
86	64.3	45.5	84.5
49	106.9	100.5	186.7

