


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW010720\
 Data File : VW014539.D
 Acq On : 07 Jan 2020 09:32
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W010320S.M
 Title : SW846 8260
 Last Update : Fri Jan 03 16:07:20 2020

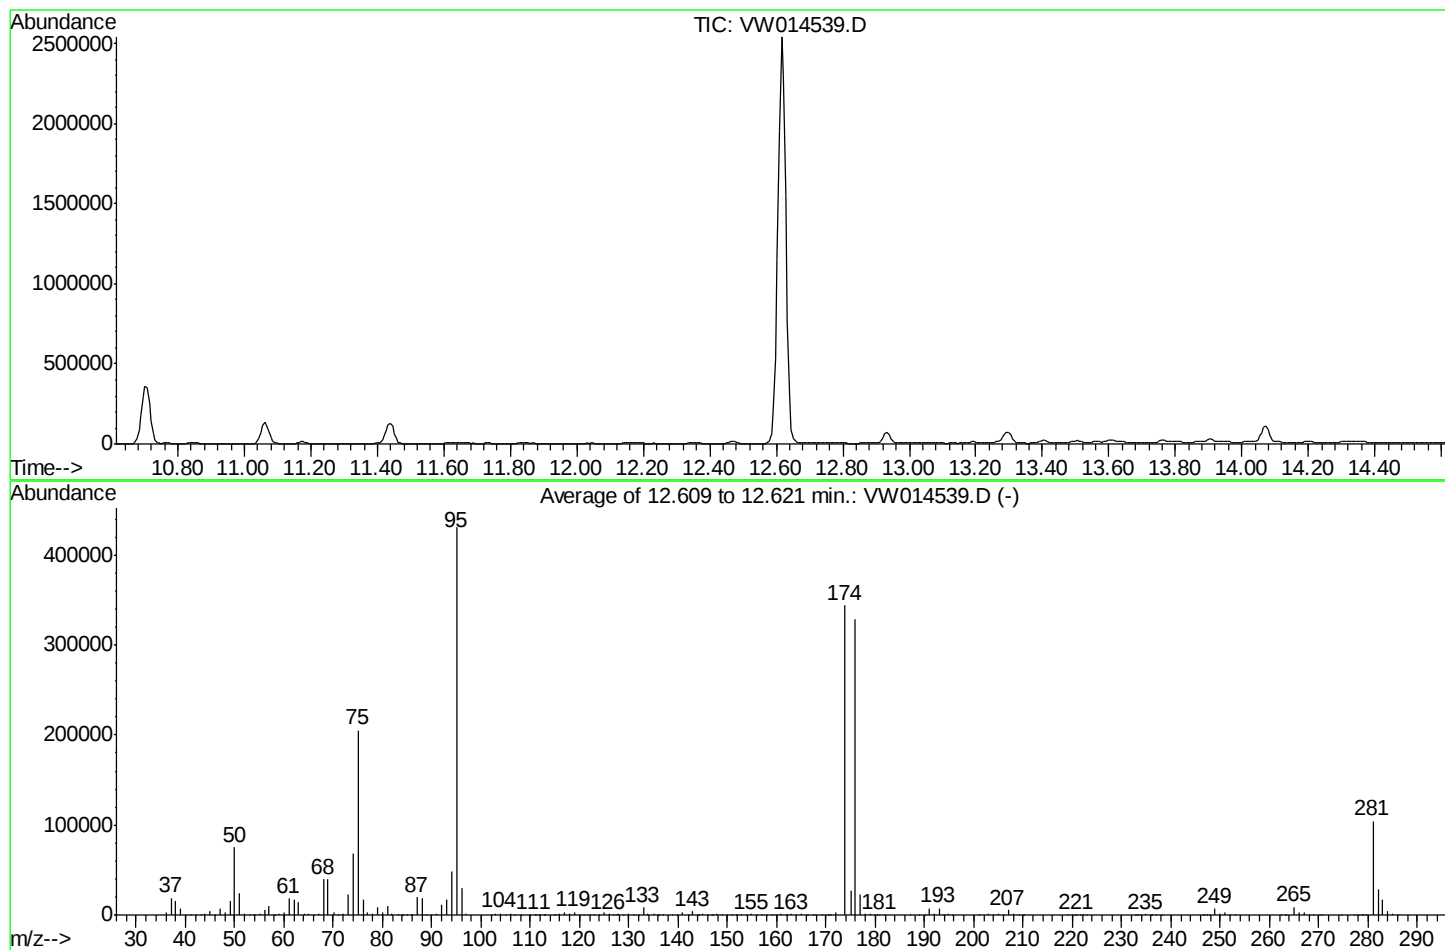

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1747

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	74976	PASS
75	95	30	60	47.7	205354	PASS
95	95	100	100	100.0	430634	PASS
96	95	5	9	6.8	29325	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	79.8	343722	PASS
175	174	5	9	8.1	27746	PASS
176	174	95	101	95.6	328704	PASS
177	176	5	9	7.1	23341	PASS