
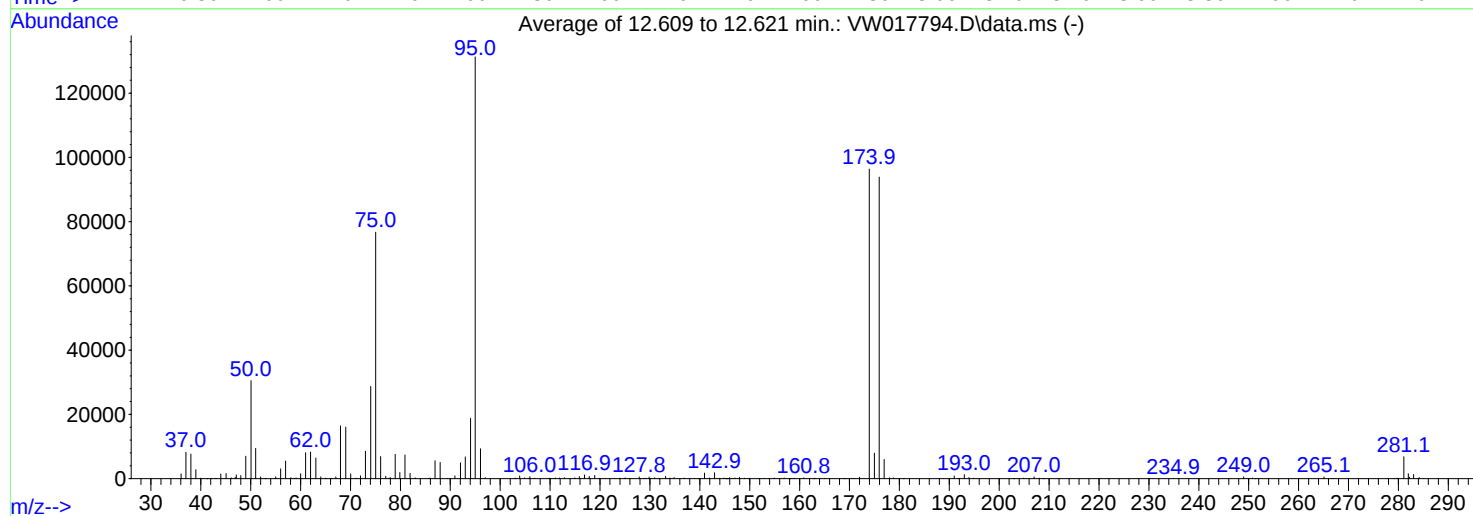


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW010721\
Data File : VW017794.D
Acq On : 07 Jan 2021 11:32
Operator : SY/VA
Sample : BFB
Misc : 5.00G/5ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W010721S.M
Title : SW846 8260
Last Update : Fri Jan 08 05:24:44 2021

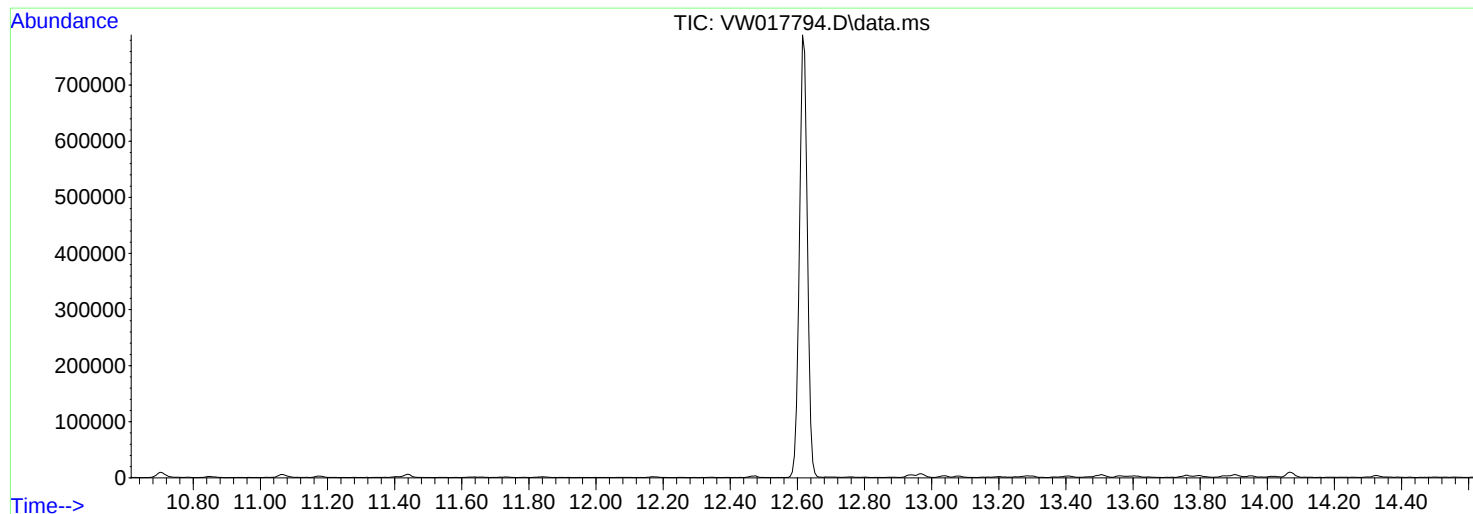

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.2	30515	PASS
75	95	30	60	58.4	76699	PASS
95	95	100	100	100.0	131304	PASS
96	95	5	9	7.1	9311	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	73.4	96355	PASS
175	174	5	9	8.2	7910	PASS
176	174	95	101	97.4	93864	PASS
177	176	5	9	6.4	5989	PASS