



Methylene Chloride

Response Ratio

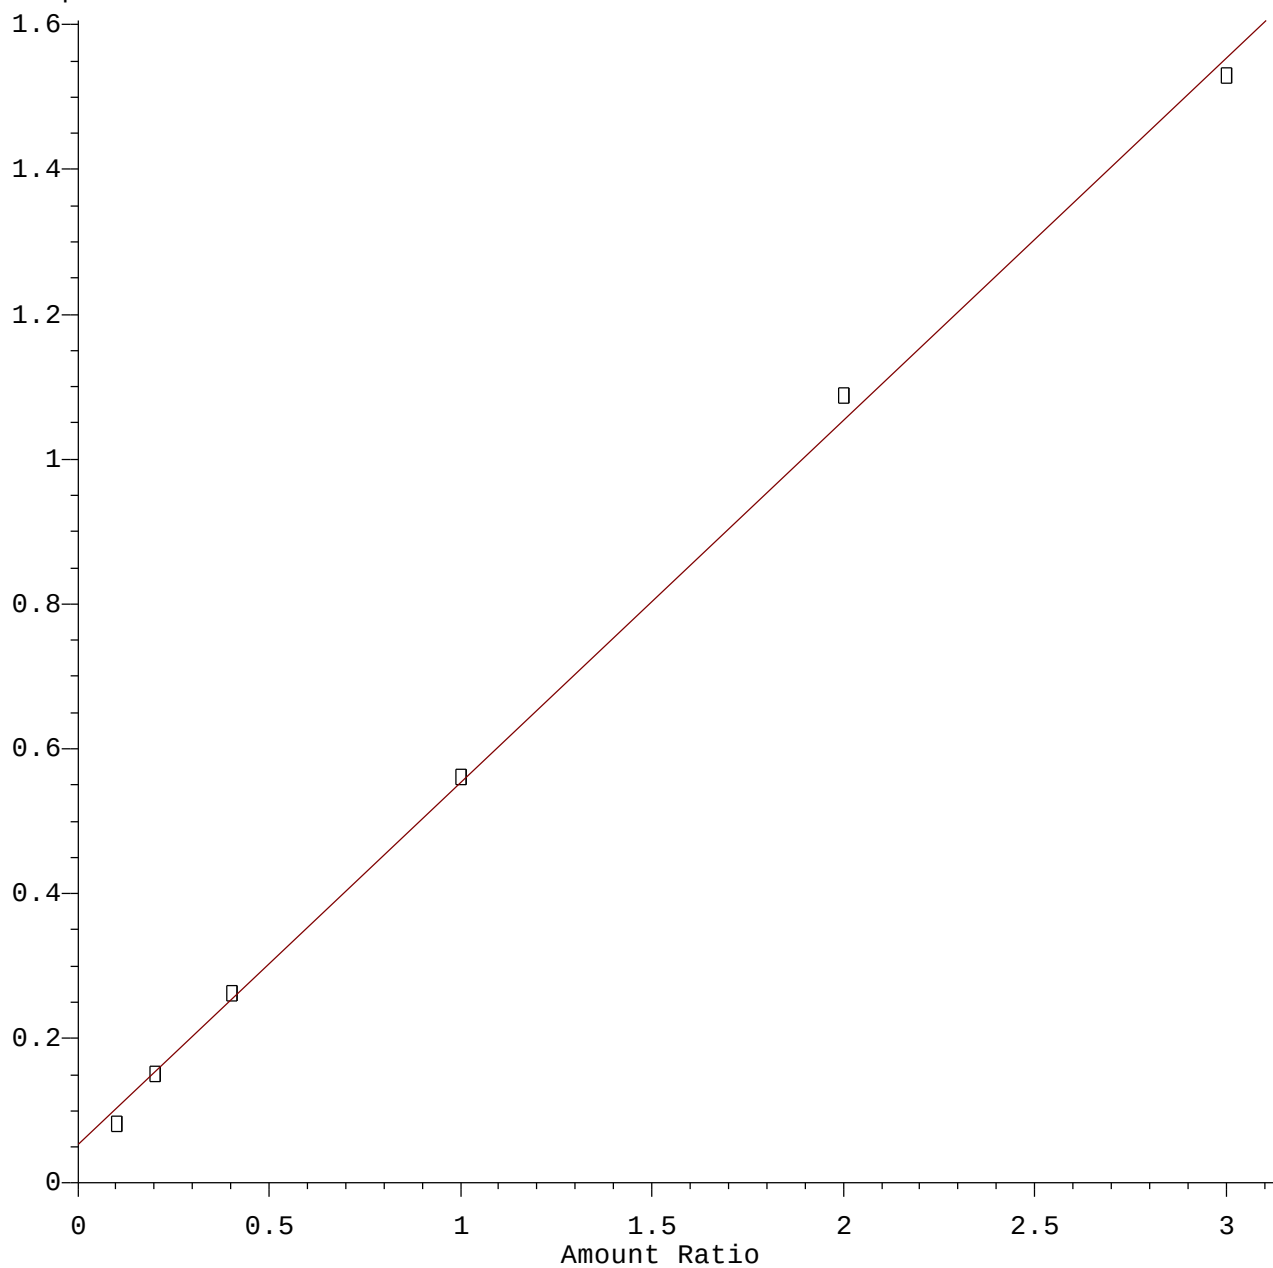


Resp Ratio = $5.00\text{e-}001 * \text{Amt} + 5.32\text{e-}002$
Coef of Det (r^2) = 0.999 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W010819S.M
Calibration Table Last Updated: Wed Jan 09 04:40:48 2019

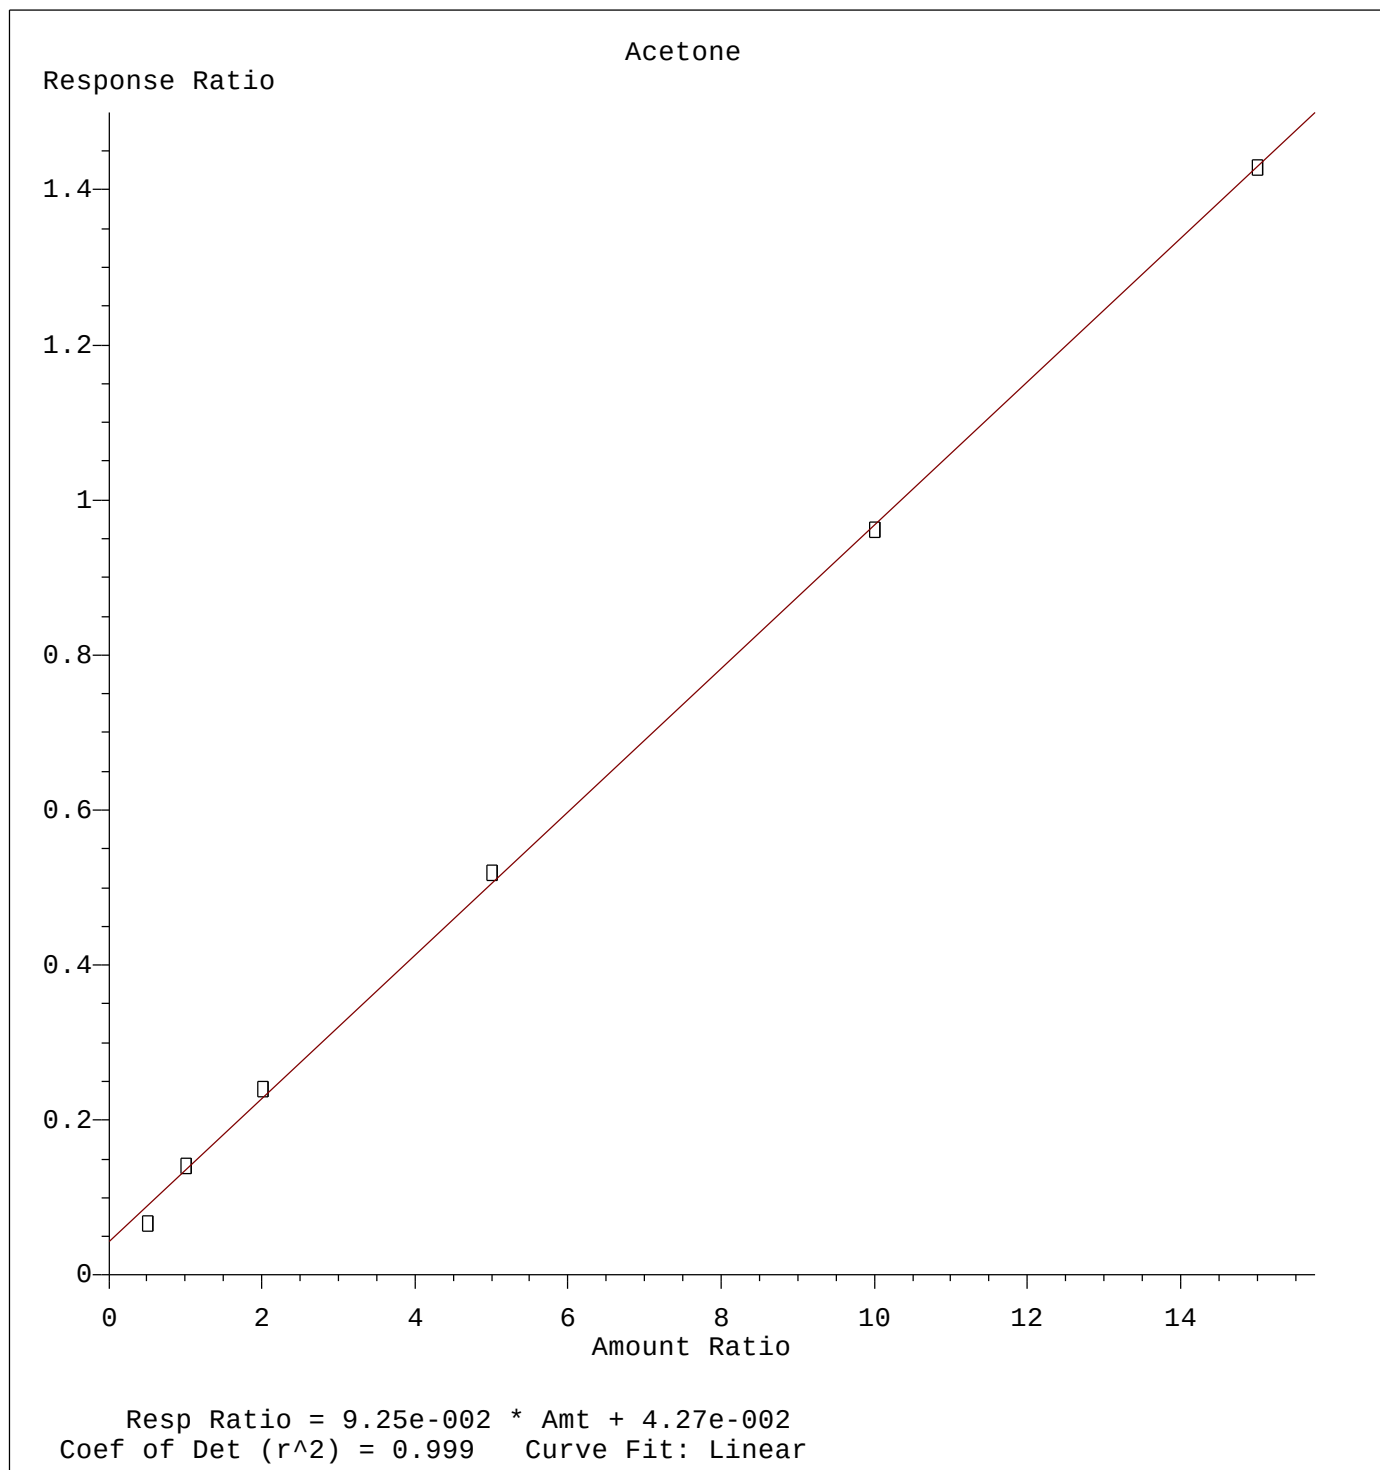

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W010819S.M
Calibration Table Last Updated: Wed Jan 09 04:40:48 2019

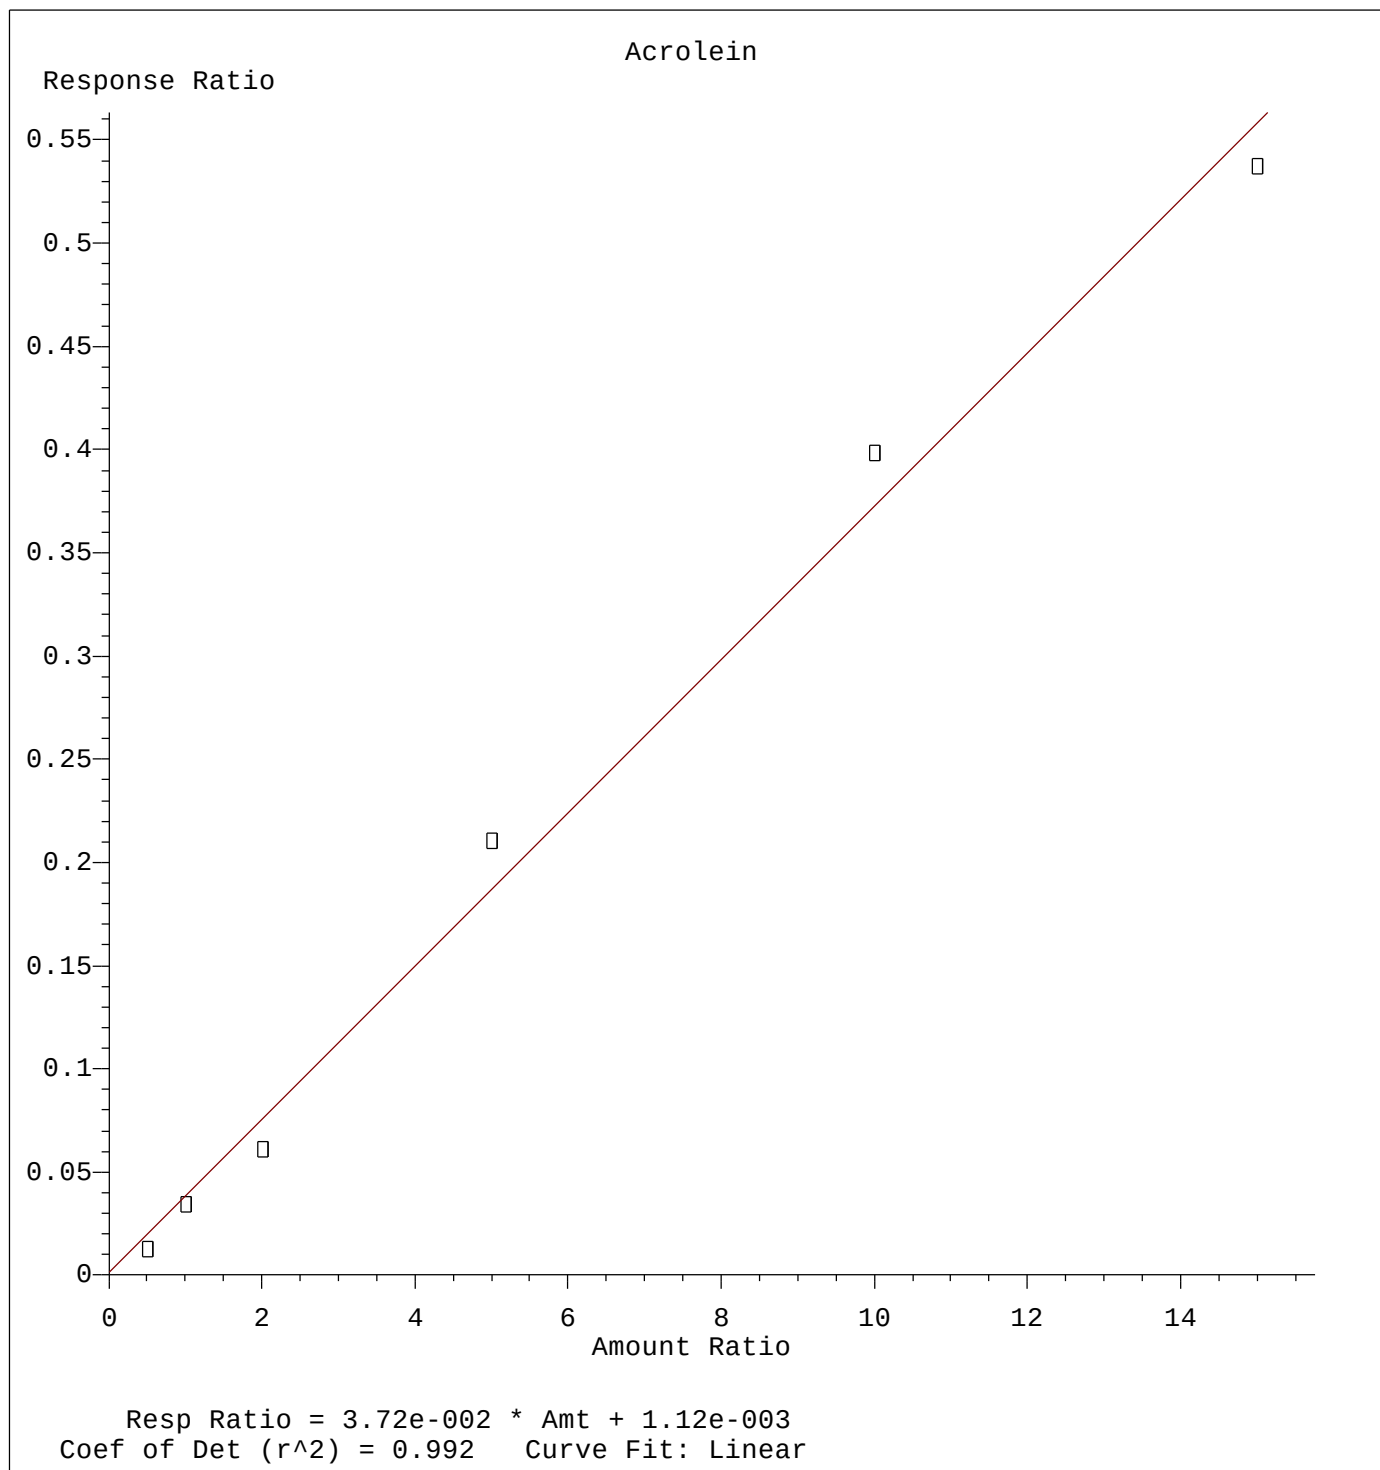

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W010819S.M
Calibration Table Last Updated: Wed Jan 09 04:40:48 2019

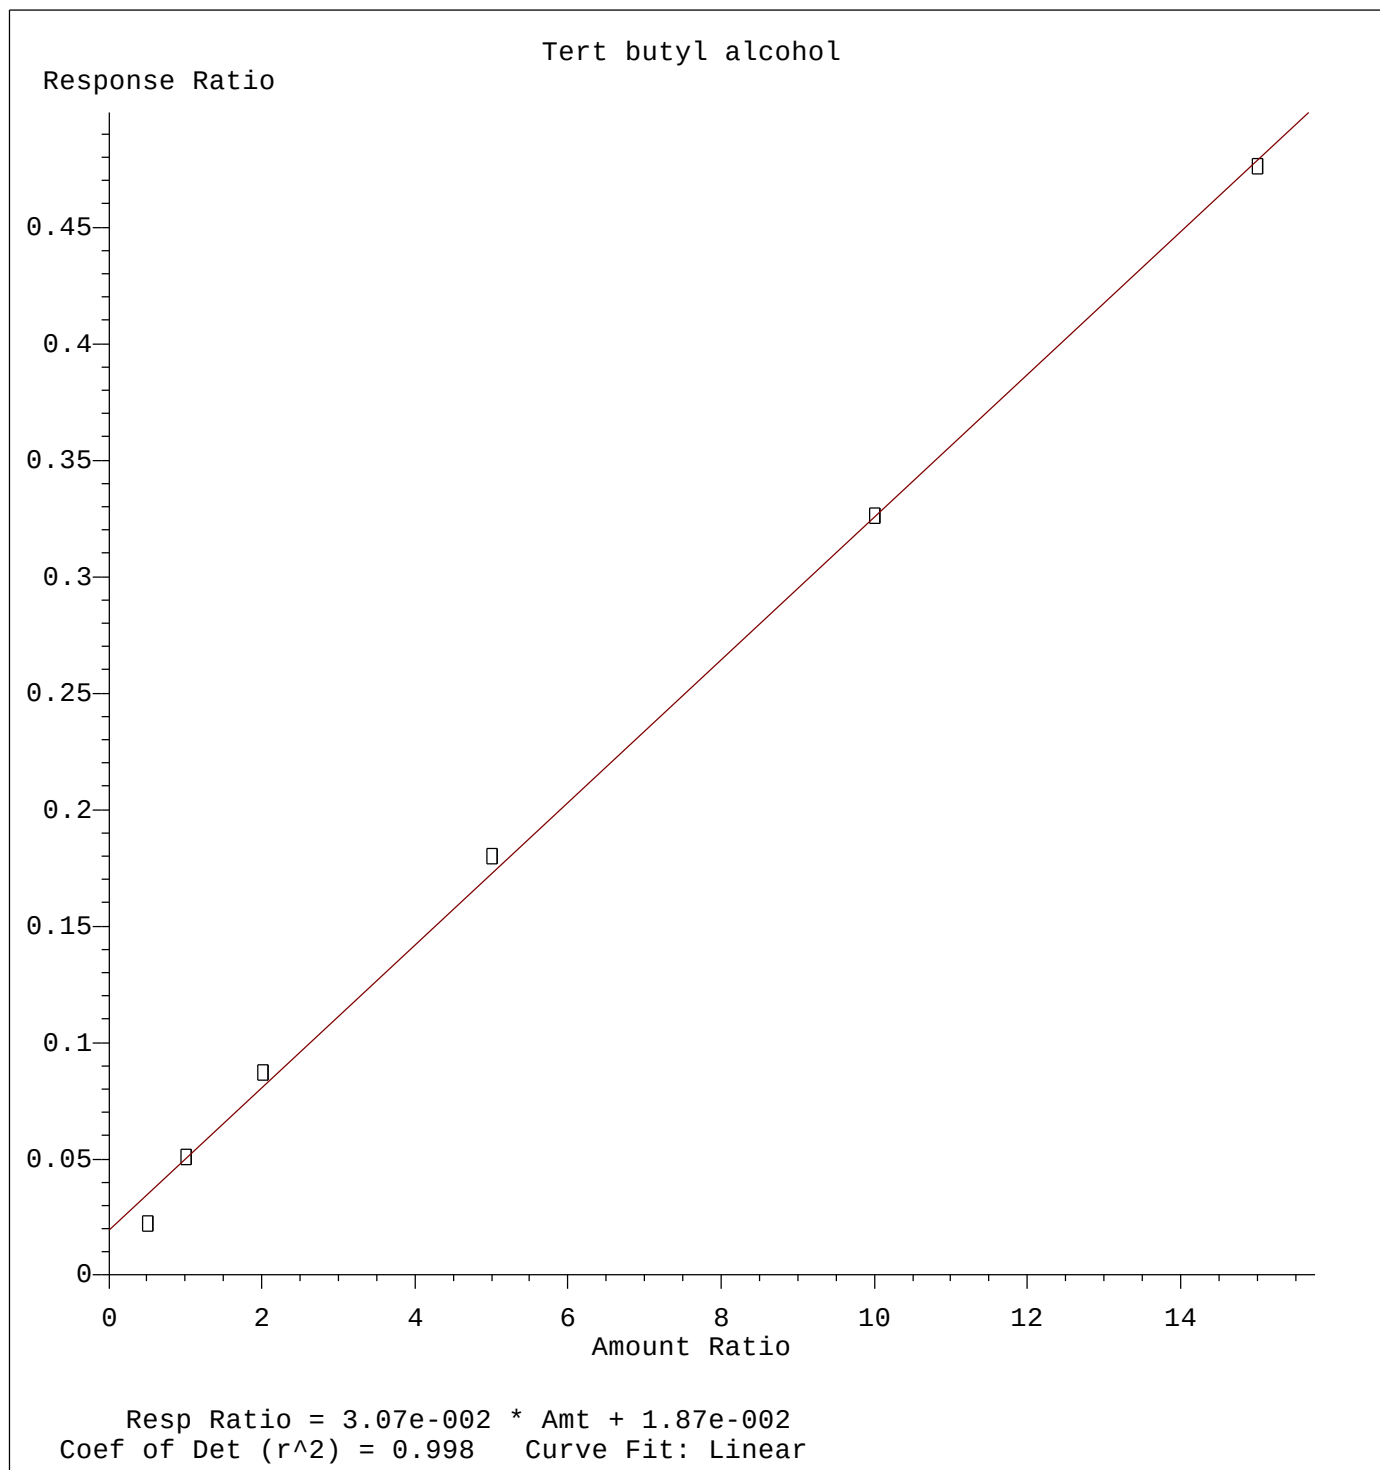

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W010819S.M
Calibration Table Last Updated: Wed Jan 09 04:40:48 2019