

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW010820\
 Data File : VW014566.D
 Acq On : 08 Jan 2020 18:07
 Operator : SY/VA
 Sample : L1056-07
 Misc : 7.27G/5ML/MSVOA_W/SOIL
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 WP022SB449_200107_36-38_FD

Quant Time: Jan 09 08:16:00 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W010320S.M
 Quant Title : SW846 8260
 QLast Update : Fri Jan 03 16:07:20 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	609310	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	938986	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	647264	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.55	152	200880	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.30	65	241841	45.40	ug/l	0.00
Spiked Amount 50.000			Recovery	=	90.80%	
35) Dibromofluoromethane	7.88	113	242490	45.19	ug/l	0.00
Spiked Amount 50.000			Recovery	=	90.38%	
50) Toluene-d8	10.32	98	922278	41.18	ug/l	0.00
Spiked Amount 50.000			Recovery	=	82.36%	
62) 4-Bromofluorobenzene	12.62	95	223926	29.48	ug/l	0.00
Spiked Amount 50.000			Recovery	=	58.96%	
Target Compounds						
16) Acetone	4.12	43	22703	15.093	ug/l	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW010820\
Data File : VW014566.D
Acq On : 08 Jan 2020 18:07
Operator : SY/VA
Sample : L1056-07
Misc : 7.27G/5ML/MSVOA_W/SOIL
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
WP022SB449_200107_36-38_FD

Quant Time: Jan 09 08:16:00 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W010320S.M
Quant Title : SW846 8260
QLast Update : Fri Jan 03 16:07:20 2020
Response via : Initial Calibration

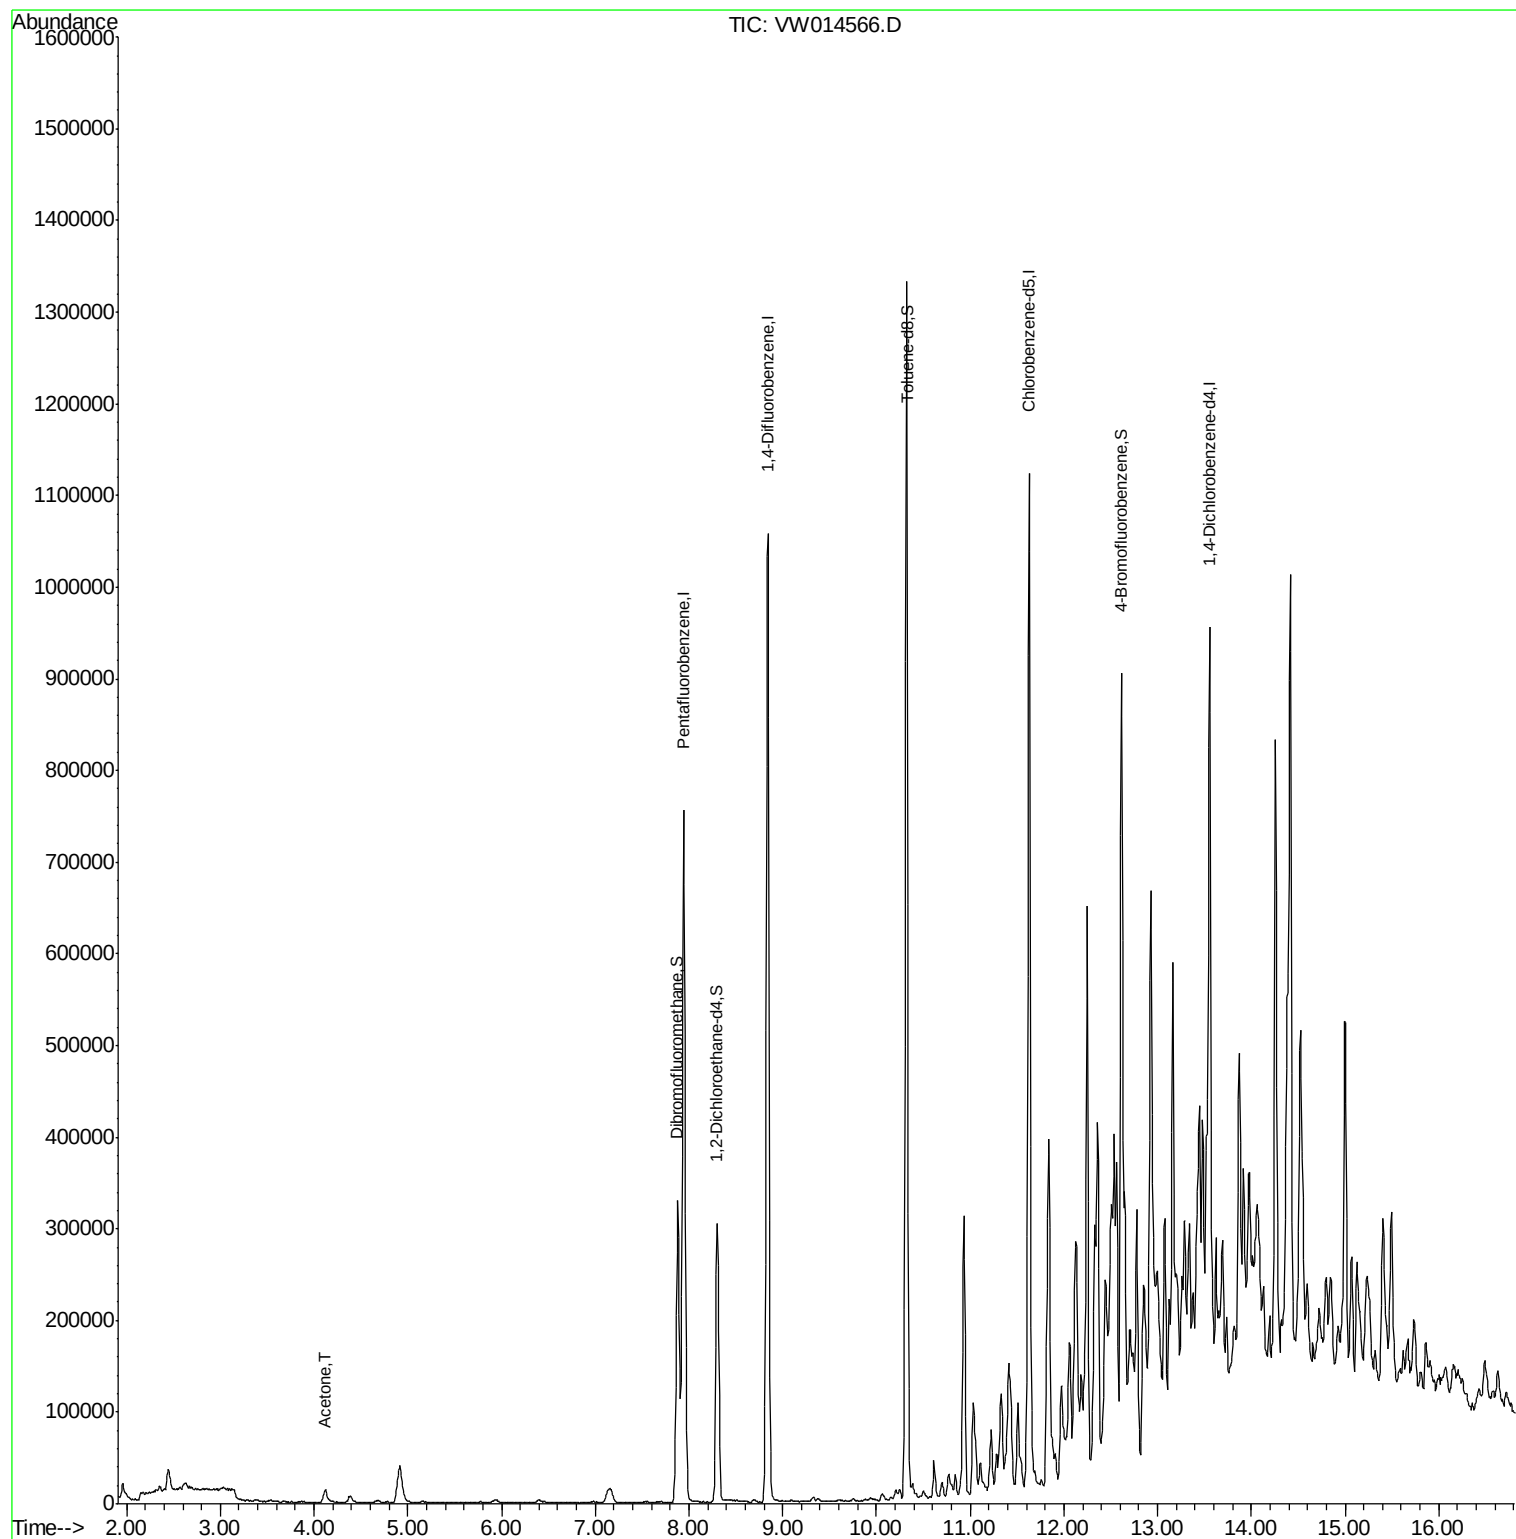

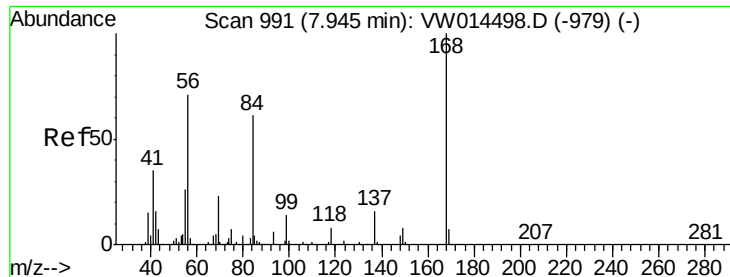

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 991

Delta R.T. -0.00 min

Lab File: VW014566.D

Acq: 08 Jan 2020 18:07

Instrument :

MSVOA_W

ClientSampleId :


WP022SB449_200107_36-38_FD

Tgt Ion:168 Resp: 609310

Ion Ratio Lower Upper

168 100

99 53.6 41.1 61.7

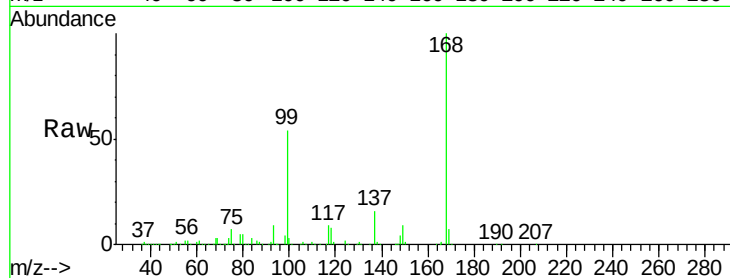

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

7.95

300000

250000

200000



150000

100000

50000

0

Time-->

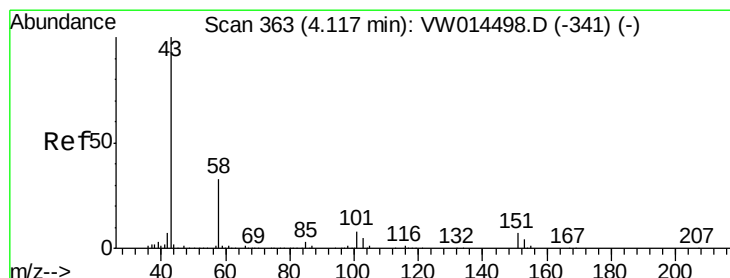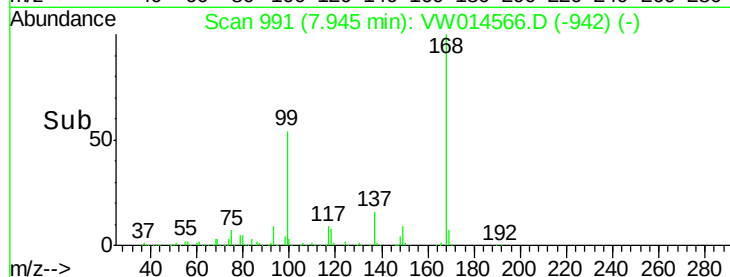

#16

Acetone

Concen: 15.093 ug/l

RT: 4.12 min Scan# 363

Delta R.T. -0.00 min

Lab File: VW014566.D


Acq: 08 Jan 2020 18:07

Tgt Ion: 43 Resp: 22703

Ion Ratio Lower Upper

43 100

58 33.2 26.6 39.8

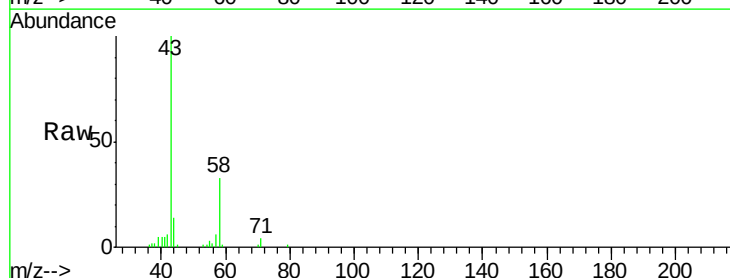

Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 58.00 (57.70 to 58.70): VW

4.12

8000


6000


4000

2000

0

Time-->




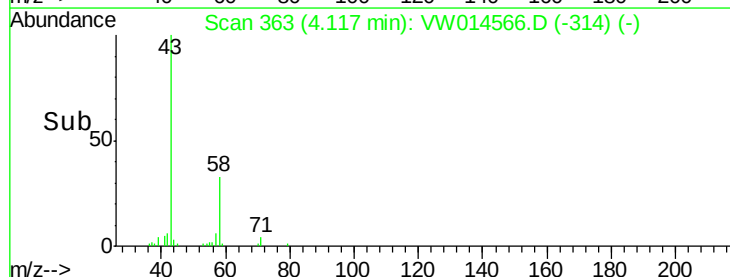


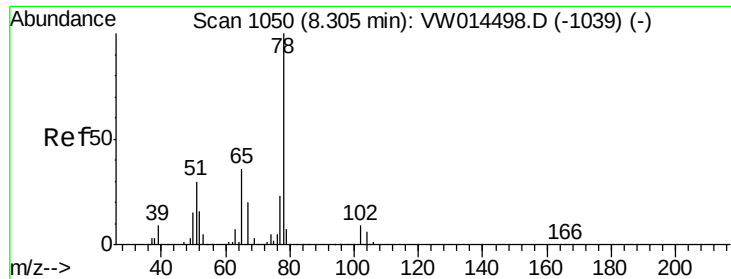

#33
 1,2-Dichloroethane-d4
 Concen: 45.397 ug/l
 RT: 8.30 min Scan# 1049
 Delta R.T. -0.01 min
 Lab File: VW014566.D
 Acq: 08 Jan 2020 18:07




Instrument :
 MSVOA_W
 ClientSampleId :
 WP022SB449_200107_36-38_FD


Tgt Ion: 65 Resp: 241841
 Ion Ratio Lower Upper
 65 100
 67 53.8 0.0 108.4

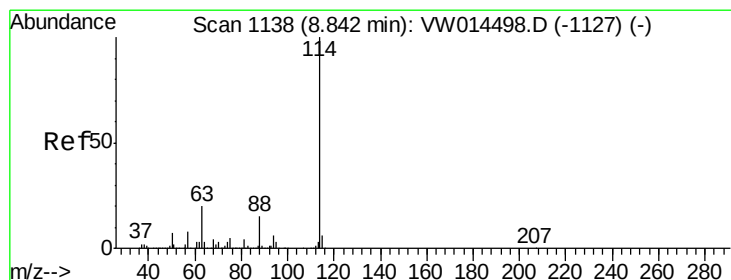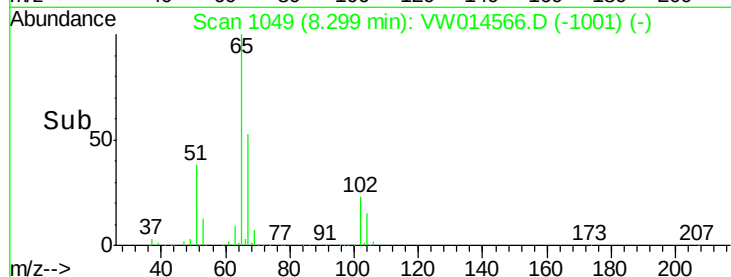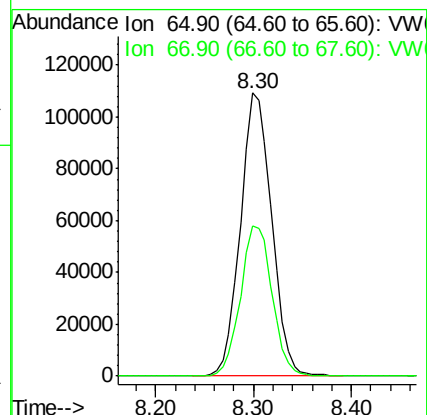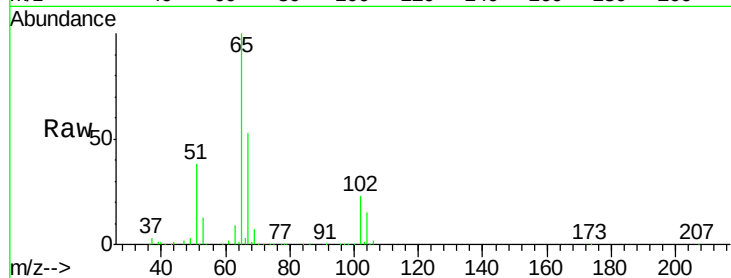

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.84 min Scan# 1138
 Delta R.T. -0.00 min
 Lab File: VW014566.D
 Acq: 08 Jan 2020 18:07

Tgt Ion: 114 Resp: 938986
 Ion Ratio Lower Upper
 114 100
 63 19.7 0.0 40.4
 88 15.7 0.0 30.6

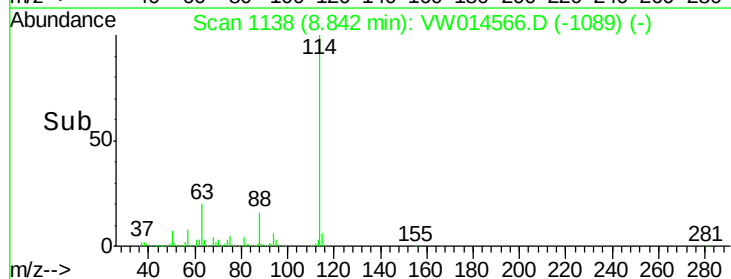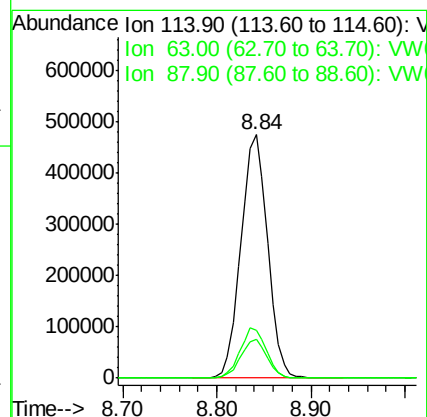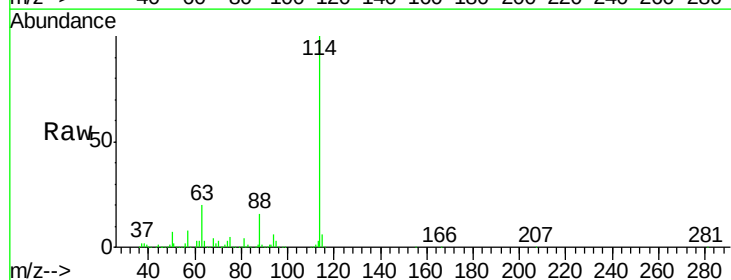

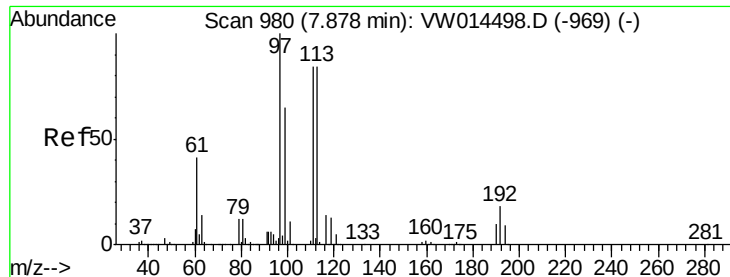

#35

Dibromofluoromethane

Concen: 45.186 ug/l

RT: 7.88 min Scan# 981

Delta R.T. 0.01 min

Lab File: VW014566.D

Acq: 08 Jan 2020 18:07

Instrument :

MSVOA_W

ClientSampleId :

WP022SB449_200107_36-38_FD


Tgt Ion:113 Resp: 242490

Ion Ratio Lower Upper

113 100

111 103.3 81.4 122.2




192 22.3 17.8 26.8

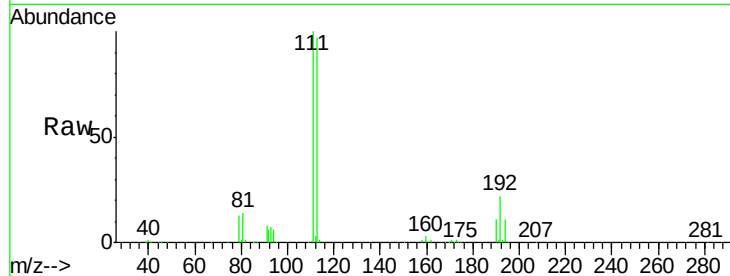

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

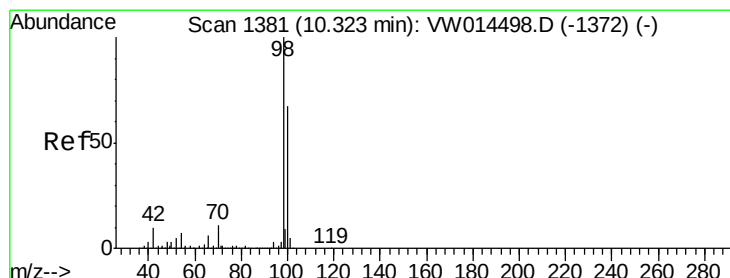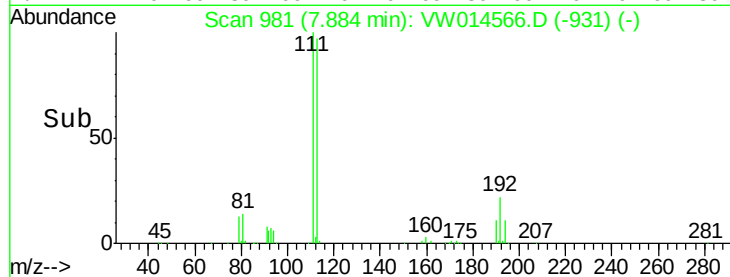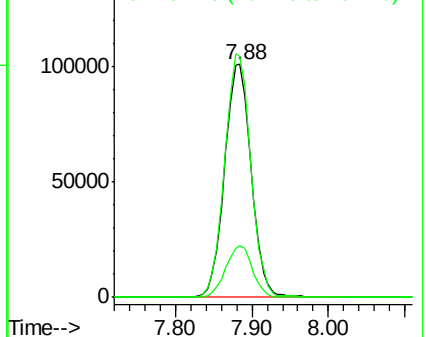

#50

Toluene-d8

Concen: 41.181 ug/l

RT: 10.32 min Scan# 1381

Delta R.T. -0.00 min

Lab File: VW014566.D


Acq: 08 Jan 2020 18:07

Tgt Ion: 98 Resp: 922278

Ion Ratio Lower Upper



98 100


100 65.7 53.8 80.6

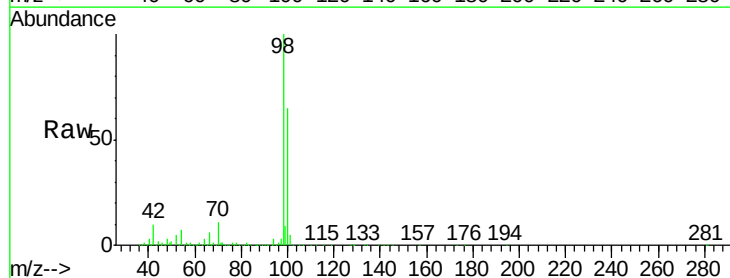

Abundance Ion 98.00 (97.70 to 98.70): VW

Ion 100.00 (99.70 to 100.70): VW



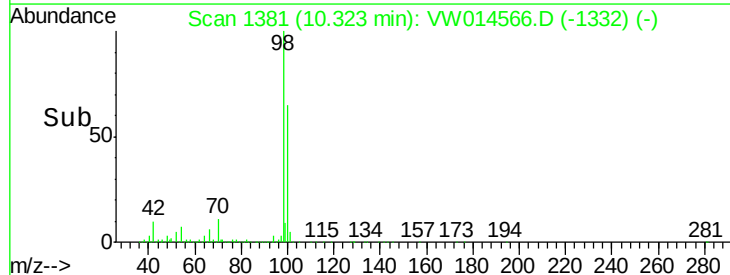
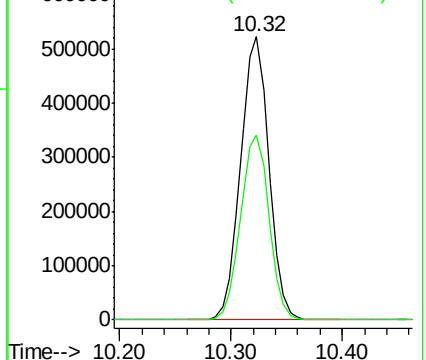


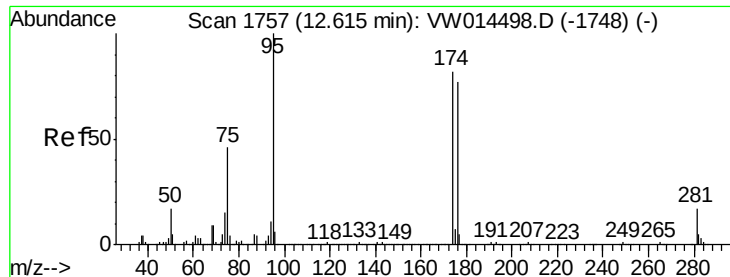

#62
4-Bromofluorobenzene
Concen: 29.478 ug/l
RT: 12.62 min Scan# 1757
Delta R.T. -0.00 min
Lab File: VW014566.D
Acq: 08 Jan 2020 18:07




Instrument :
MSVOA_W
ClientSampleId :
WP022SB449_200107_36-38_FD


Tgt Ion: 95 Resp: 223926
Ion Ratio Lower Upper
95 100
174 81.8 0.0 168.6
176 81.3 0.0 162.0

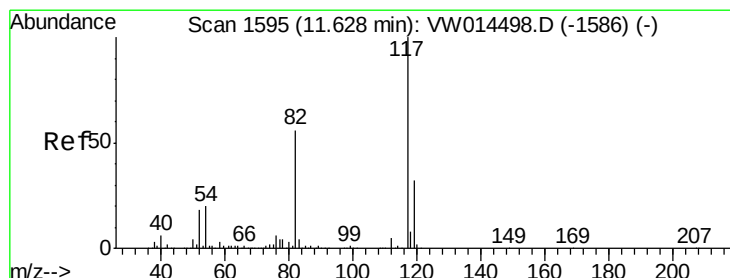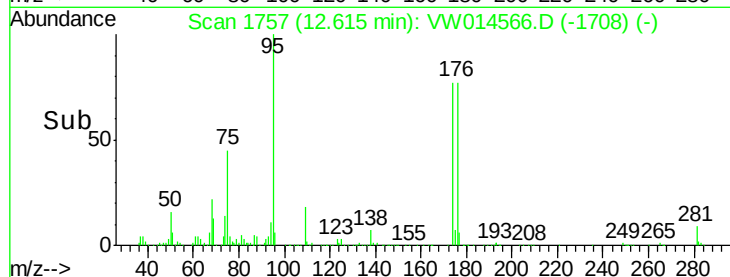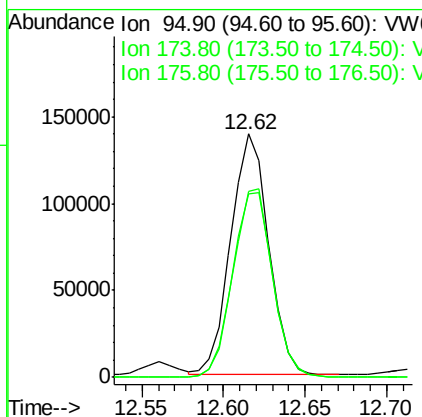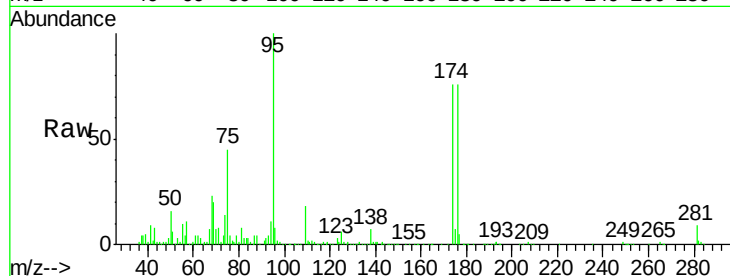

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.63 min Scan# 1595
Delta R.T. -0.00 min
Lab File: VW014566.D
Acq: 08 Jan 2020 18:07

Tgt Ion: 117 Resp: 647264
Ion Ratio Lower Upper
117 100
82 53.6 44.6 67.0
119 30.8 25.7 38.5

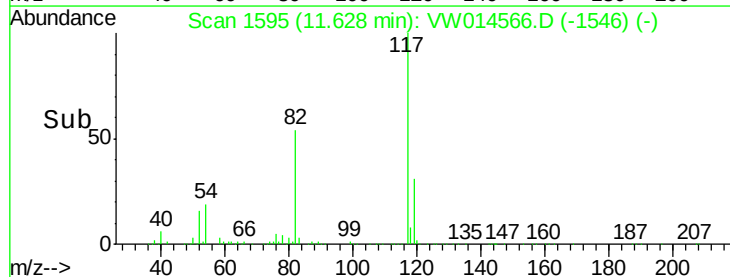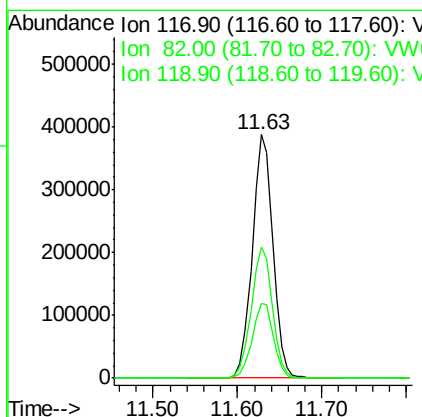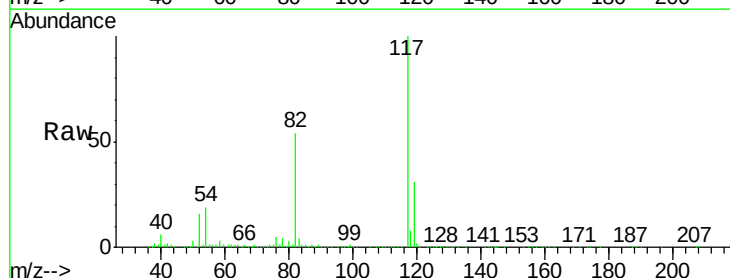

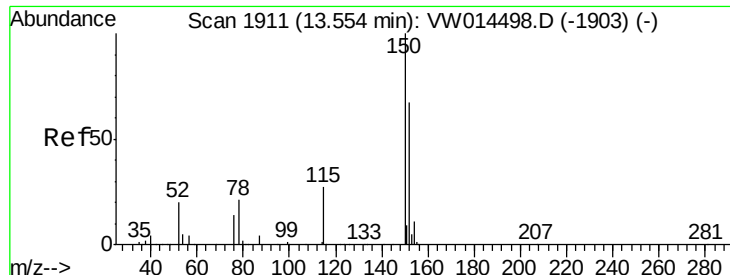

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.55 min Scan# 1911

Delta R.T. -0.00 min

Lab File: VW014566.D


Acq: 08 Jan 2020 18:07

Instrument :

MSVOA_W

ClientSampleId :

WP022SB449_200107_36-38_FD

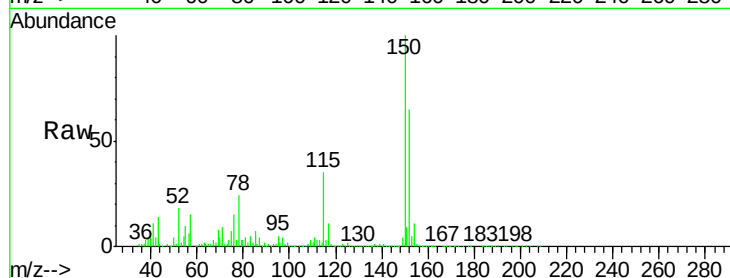


Tgt Ion:152 Resp: 200880

Ion Ratio Lower Upper

152 100

115 51.5 27.7 83.1

150 145.5 0.0 343.4

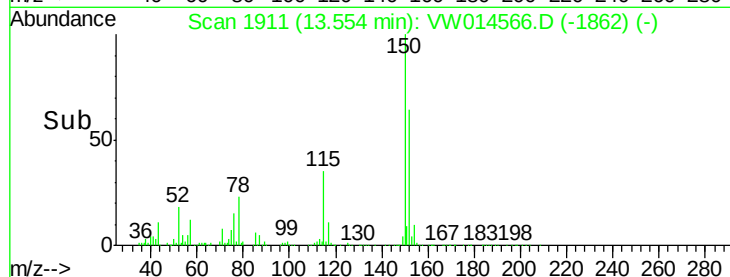

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

