


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW010820\
 Data File : VW014550.D
 Acq On : 08 Jan 2020 09:11
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W010320S.M
 Title : SW846 8260
 Last Update : Fri Jan 03 16:07:20 2020

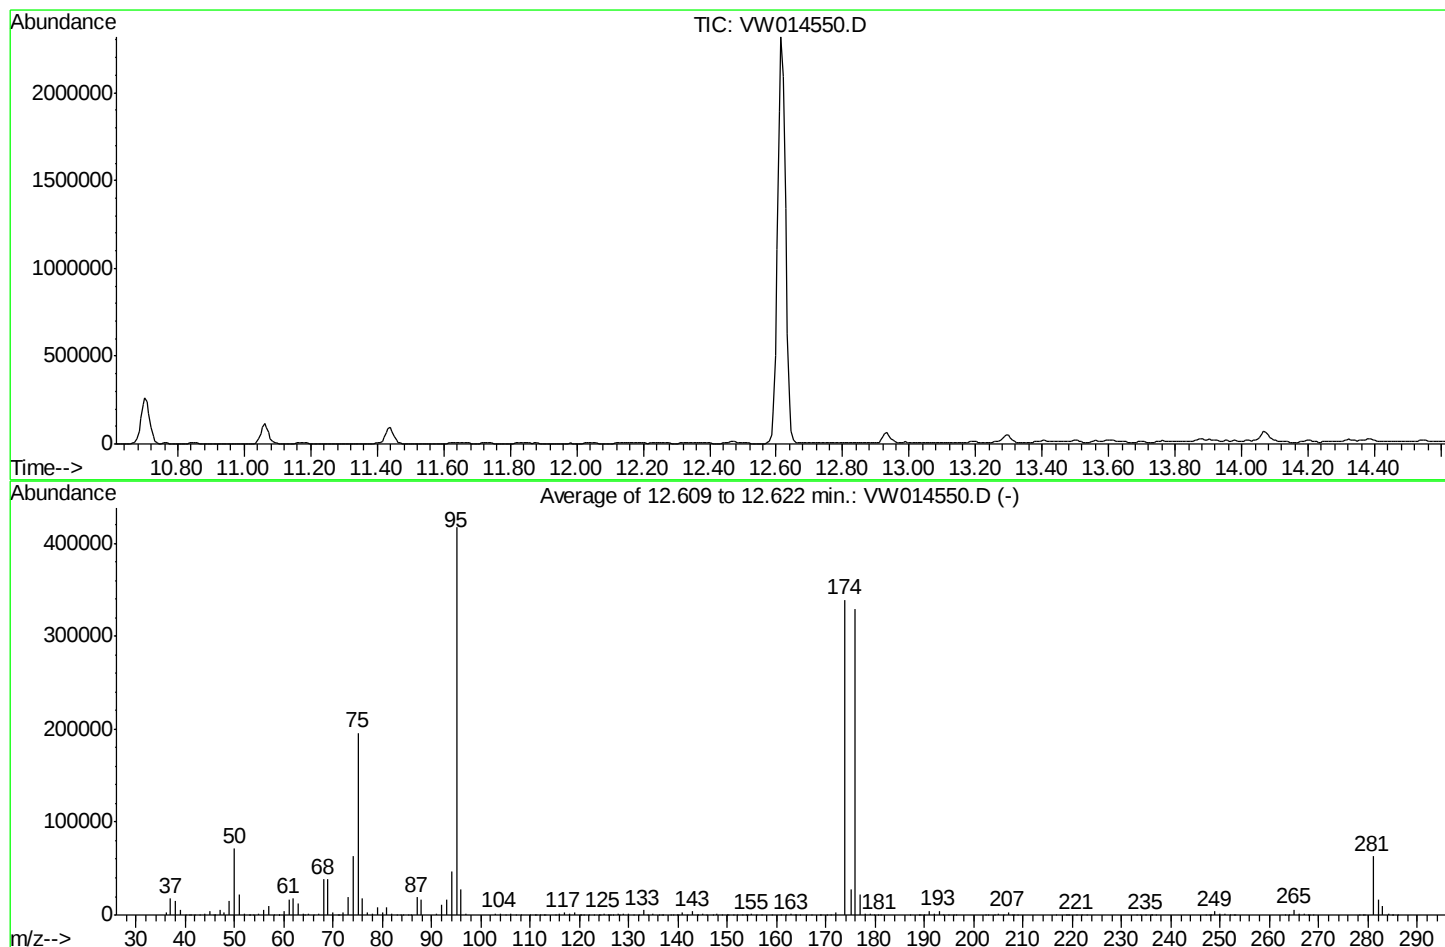

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1747

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	71250	PASS
75	95	30	60	47.1	196309	PASS
95	95	100	100	100.0	417216	PASS
96	95	5	9	6.7	27810	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	81.2	338944	PASS
175	174	5	9	8.0	27098	PASS
176	174	95	101	97.1	329024	PASS
177	176	5	9	6.9	22616	PASS