


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW010919\
 Data File : VW008118.D
 Acq On : 09 Jan 2019 22:48
 Operator : SY/AP
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W010819S.M
 Title : SW846 8260
 Last Update : Wed Jan 09 04:40:48 2019

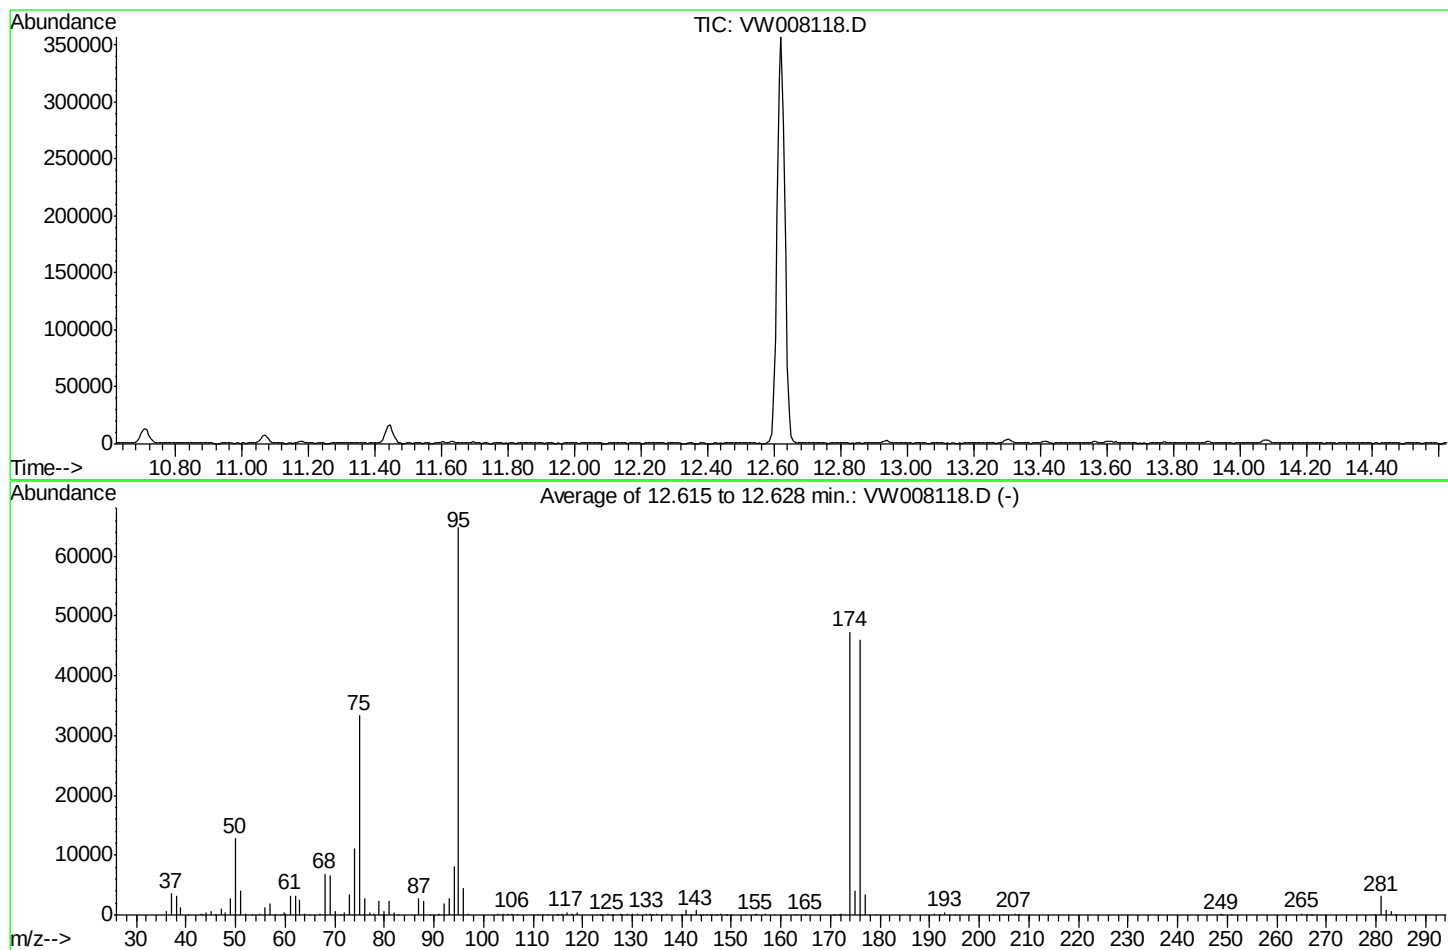

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	12797	PASS
75	95	30	60	51.5	33368	PASS
95	95	100	100	100.0	64832	PASS
96	95	5	9	6.9	4490	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	73.1	47386	PASS
175	174	5	9	8.5	4040	PASS
176	174	95	101	97.2	46080	PASS
177	176	5	9	7.3	3363	PASS