


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW010920\
 Data File : VW014571.D
 Acq On : 09 Jan 2020 09:09
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W010320S.M
 Title : SW846 8260
 Last Update : Fri Jan 03 16:07:20 2020

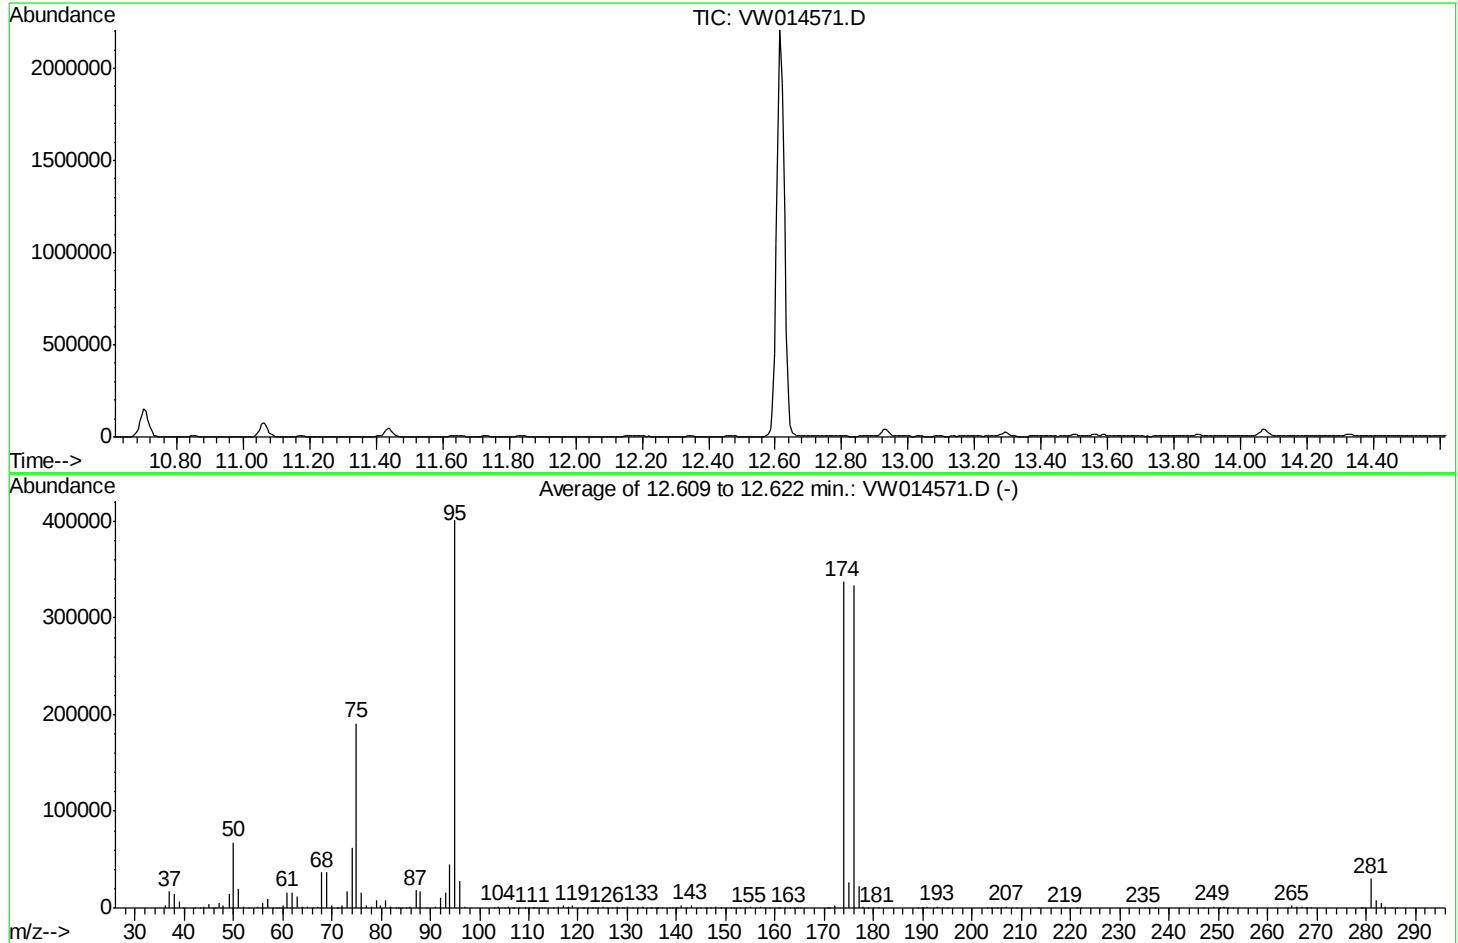

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1747

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	68016	PASS
75	95	30	60	47.6	190976	PASS
95	95	100	100	100.0	400960	PASS
96	95	5	9	6.8	27224	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	84.2	337408	PASS
175	174	5	9	7.7	25912	PASS
176	174	95	101	98.7	333162	PASS
177	176	5	9	6.7	22192	PASS