

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW011019\
 Data File : VW008143.D
 Acq On : 10 Jan 2019 12:15
 Operator : SY/AP
 Sample : VW0110SBL01
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VW0110SBL01

Quant Time: Jan 11 05:50:30 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W010819S.M
 Quant Title : SW846 8260
 QLast Update : Wed Jan 09 04:40:48 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	64024	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	120028	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	108676	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	47229	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	39867	55.40	ug/l	0.00
Spiked Amount	50.000		Recovery	=	110.80%	
35) Dibromofluoromethane	7.88	113	37808	54.01	ug/l	0.00
Spiked Amount	50.000		Recovery	=	108.02%	
50) Toluene-d8	10.32	98	156654	53.33	ug/l	0.00
Spiked Amount	50.000		Recovery	=	106.66%	
62) 4-Bromofluorobenzene	12.62	95	50879	48.31	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.62%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW011019\
Data File : VW008143.D
Acq On : 10 Jan 2019 12:15
Operator : SY/AP
Sample : VW0110SBL01
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VW0110SBL01

Quant Time: Jan 11 05:50:30 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W010819S.M
Quant Title : SW846 8260
QLast Update : Wed Jan 09 04:40:48 2019
Response via : Initial Calibration

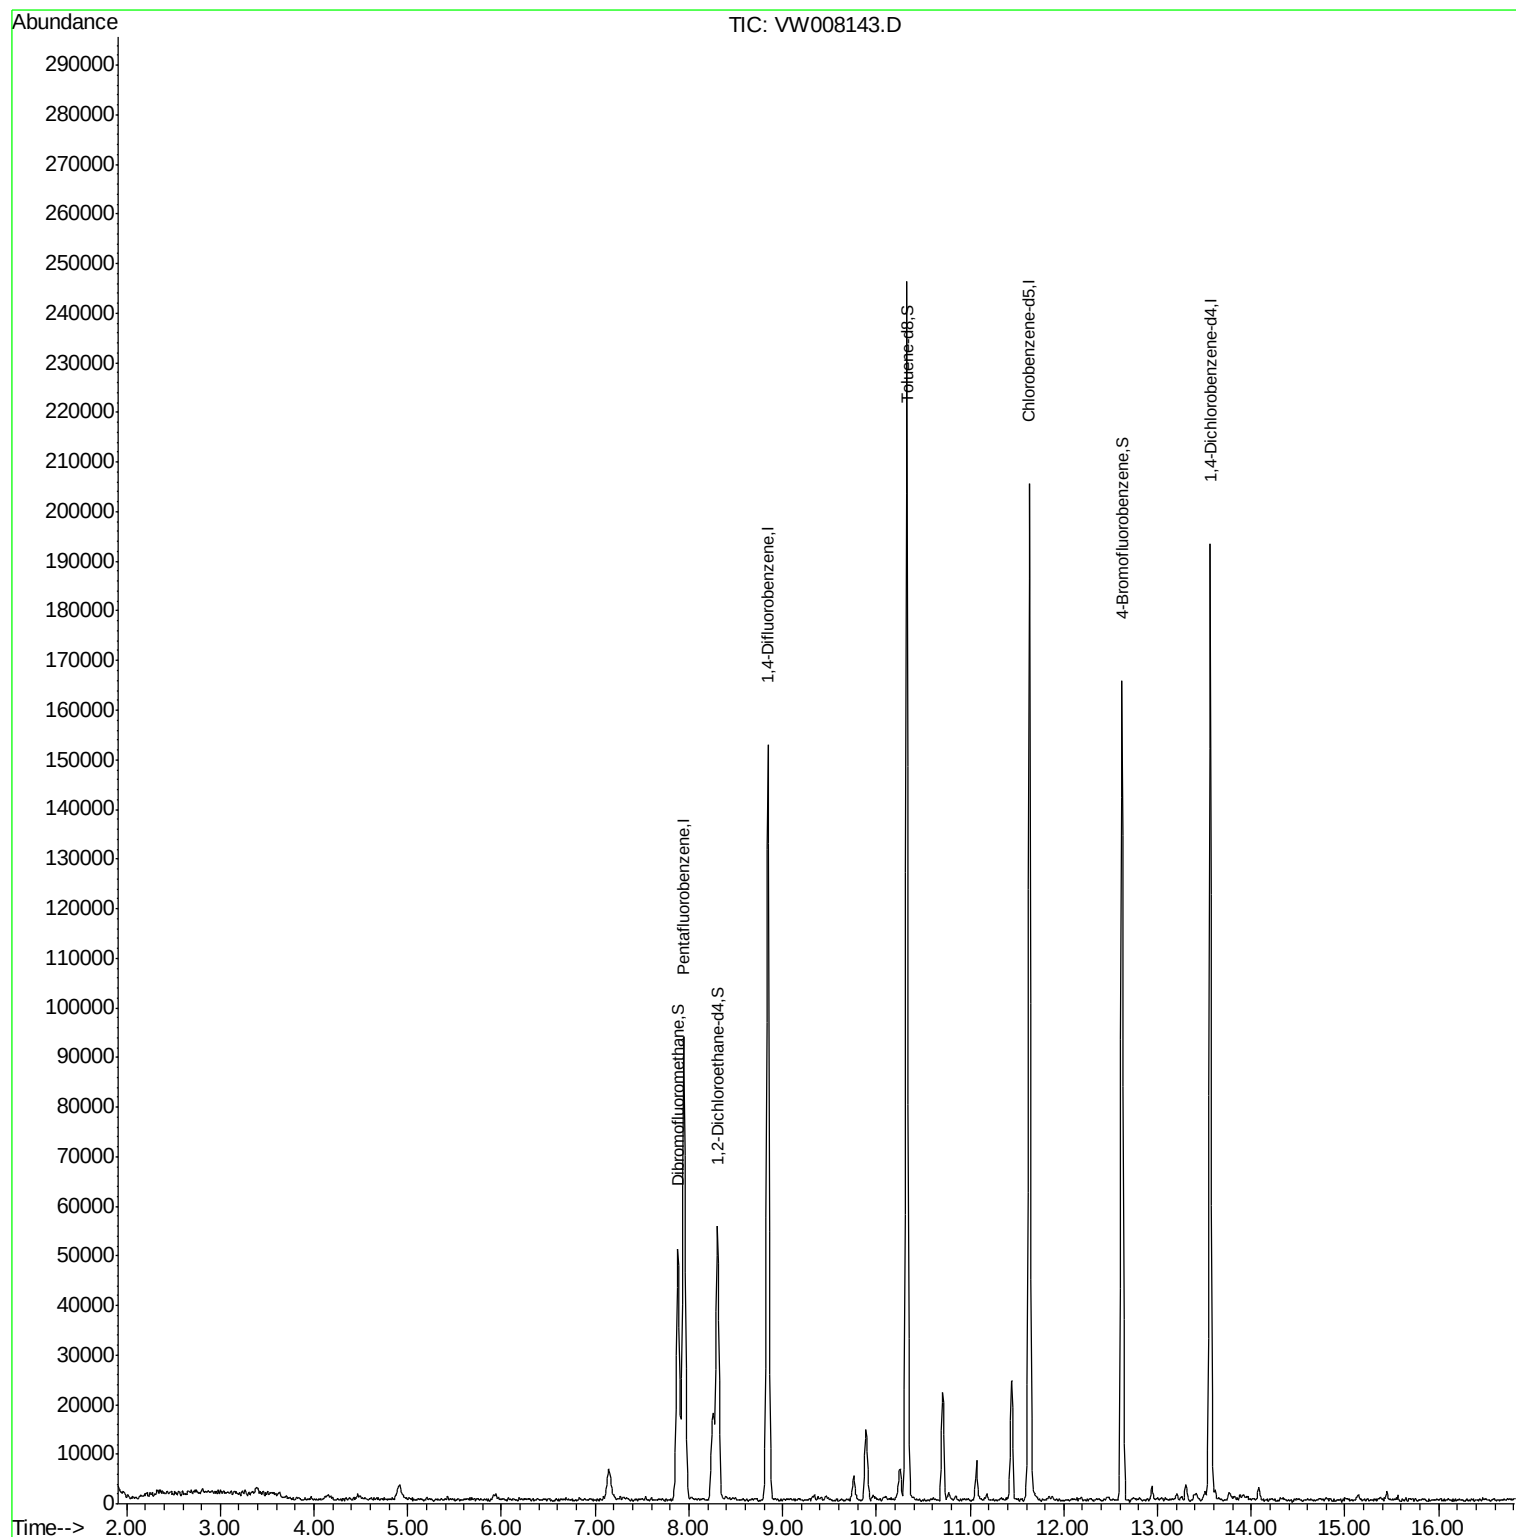

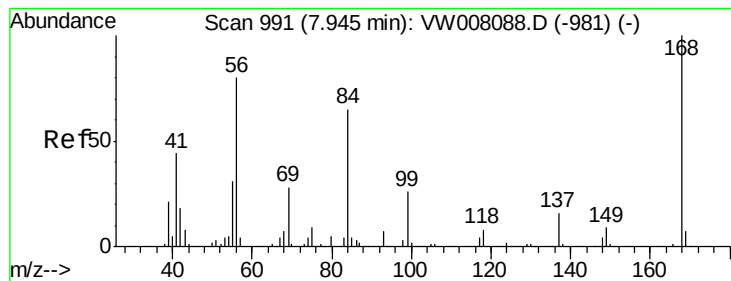

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 991

Delta R.T. -0.00 min

Lab File: VW008143.D

Acq: 10 Jan 2019 12:15

Instrument :

MSVOA_W

ClientSampleId :


VW0110SBL01

Tot Ion:168 Resp: 64024

Ion Ratio Lower Upper

168 100

99 63.7 52.6 78.8

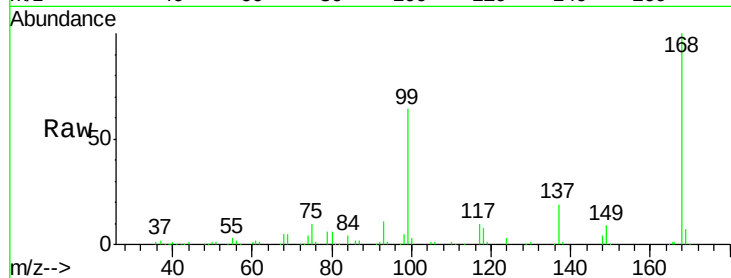

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

7.95

30000



20000

10000

0

7.85 7.90 7.95 8.00 8.05

Time-->

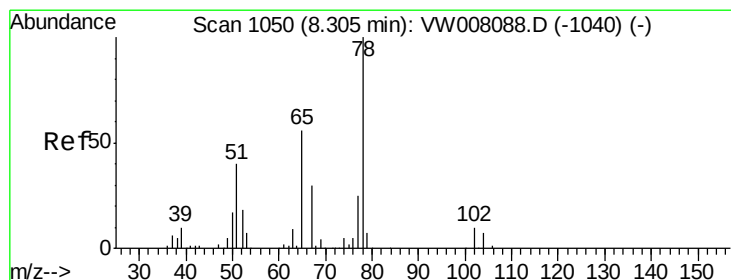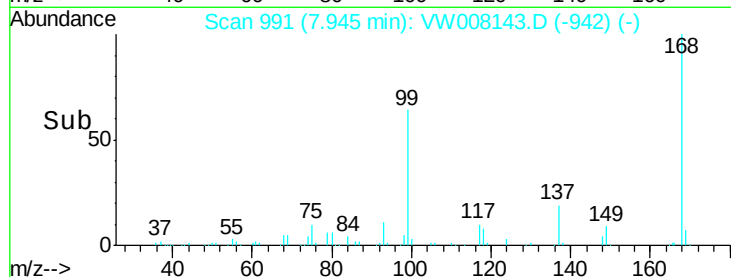

#33

1,2-Dichloroethane-d4

Concen: 55.404 ug/l

RT: 8.31 min Scan# 1050

Delta R.T. -0.00 min

Lab File: VW008143.D


Acq: 10 Jan 2019 12:15

Tgt Ion: 65 Resp: 39867

Ion Ratio Lower Upper

65 100

67 52.2 0.0 106.8

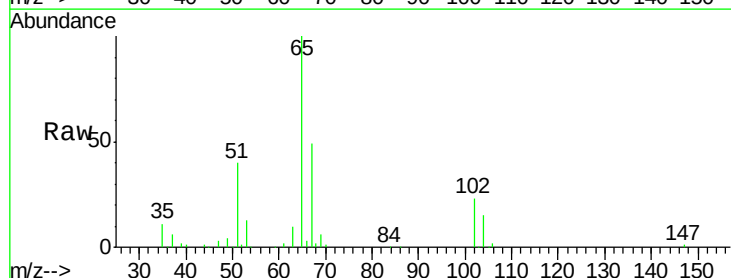

Abundance Ion 64.90 (64.60 to 65.60): VW

Ion 66.90 (66.60 to 67.60): VW

8.31

20000

15000


10000


5000

0

8.20 8.25 8.30 8.35 8.40

Time-->

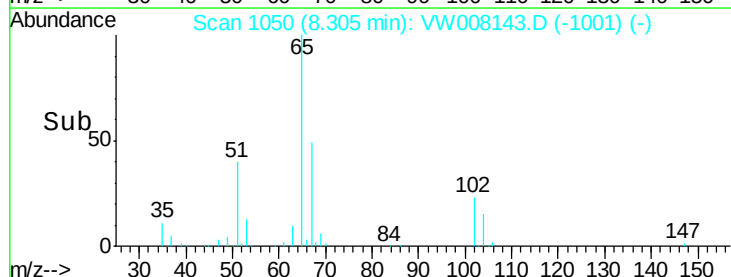


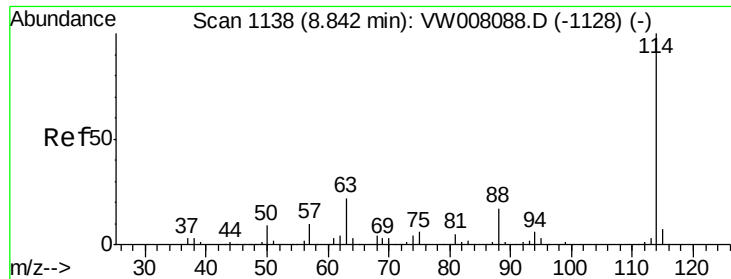




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.84 min Scan# 1138
 Delta R.T. -0.00 min
 Lab File: VW008143.D
 Acq: 10 Jan 2019 12:15

Instrument :
 MSVOA_W
 ClientSampleId :
 VW0110SBL01

Tot Ion:114 Resp: 120028
 Ion Ratio Lower Upper
 114 100
 63 20.6 0.0 43.4
 88 15.7 0.0 33.4

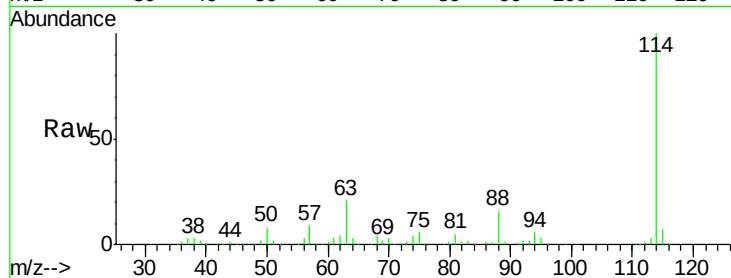


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VW
 Ion 87.90 (87.60 to 88.60): VW

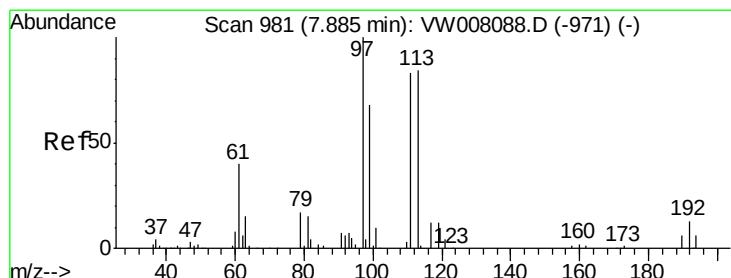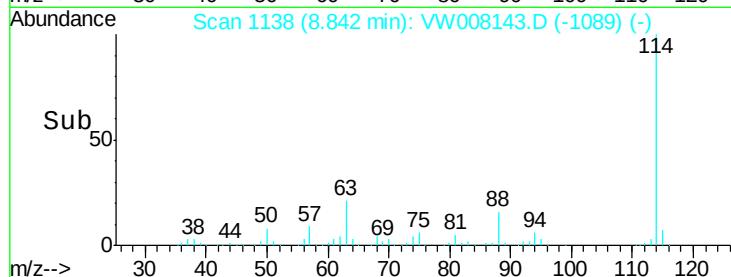
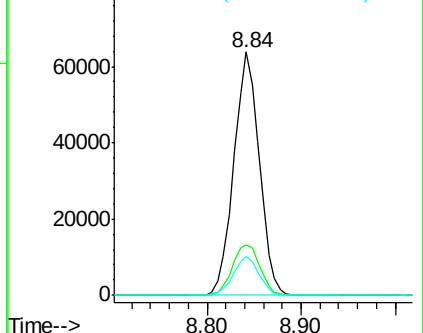



#35
 Dibromofluoromethane
 Concen: 54.008 ug/l
 RT: 7.88 min Scan# 980
 Delta R.T. -0.01 min
 Lab File: VW008143.D
 Acq: 10 Jan 2019 12:15

Tgt Ion:113 Resp: 37808
 Ion Ratio Lower Upper
 113 100
 111 99.7 81.8 122.8
 192 17.1 12.8 19.2

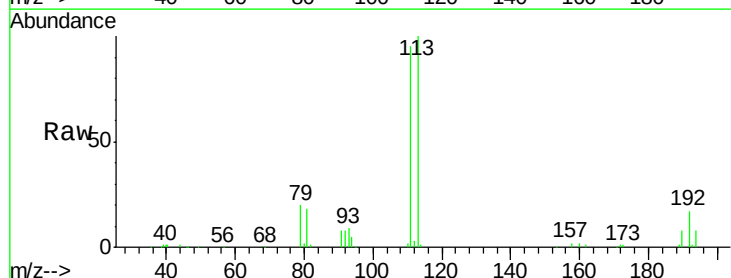

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V



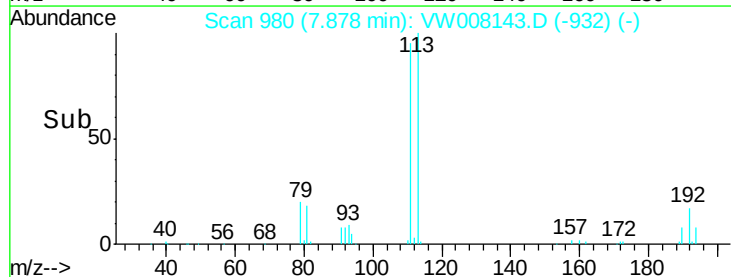
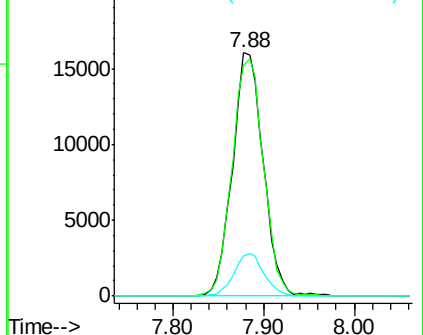


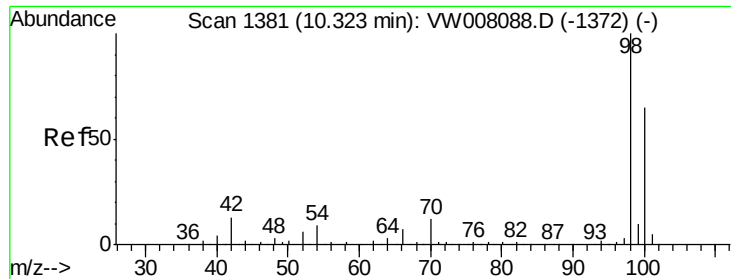

#50
Toluene-d8
Concen: 53.326 ug/l
RT: 10.32 min Scan# 1381
Delta R.T. -0.00 min
Lab File: VW008143.D
Acq: 10 Jan 2019 12:15




Instrument :
MSVOA_W
ClientSampleId :
VW0110SBL01


Tot Ion: 98 Resp: 156654
Ion Ratio Lower Upper
98 100
100 63.6 51.7 77.5

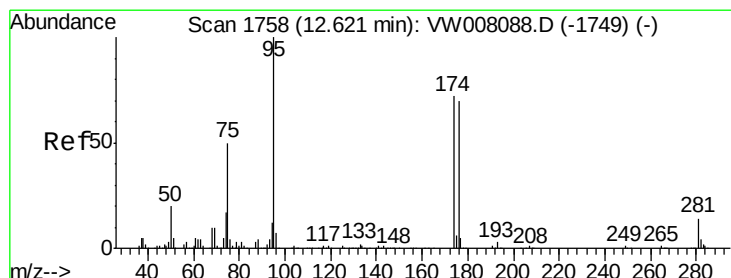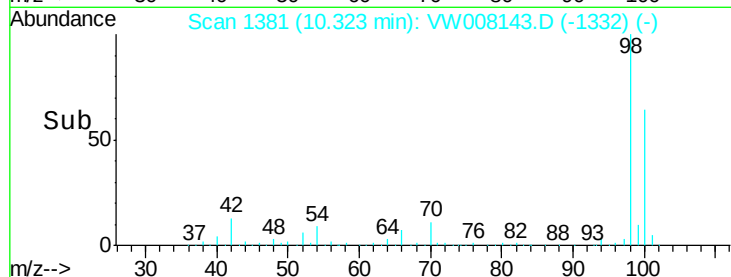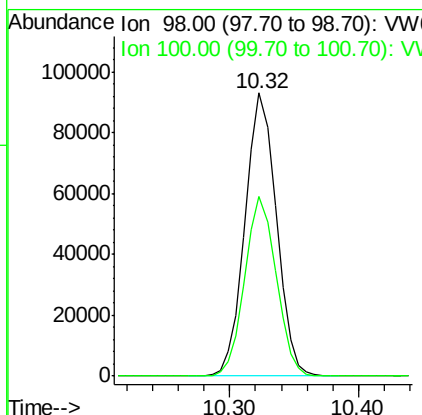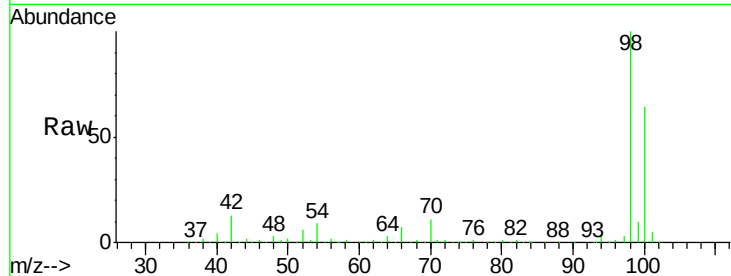

#62
4-Bromofluorobenzene
Concen: 48.311 ug/l
RT: 12.62 min Scan# 1758
Delta R.T. -0.00 min
Lab File: VW008143.D
Acq: 10 Jan 2019 12:15

Tgt Ion: 95 Resp: 50879
Ion Ratio Lower Upper
95 100
174 72.3 0.0 143.0
176 68.9 0.0 140.2


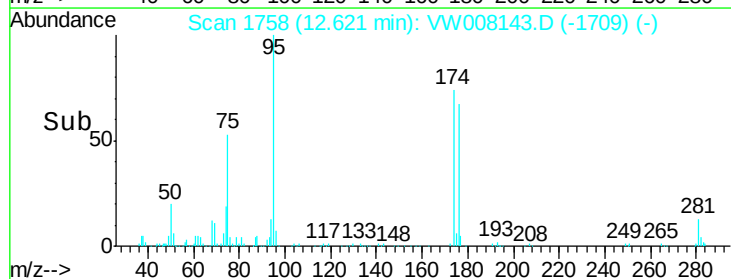
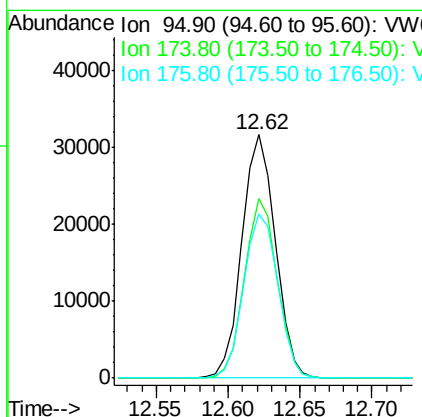
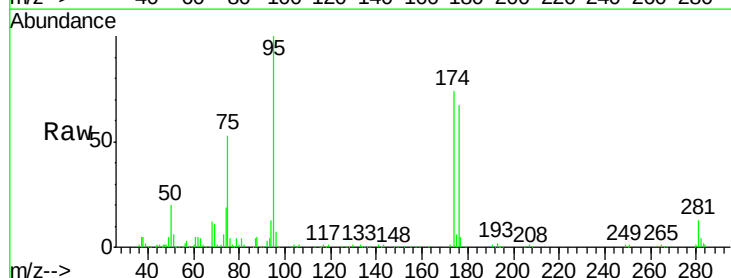


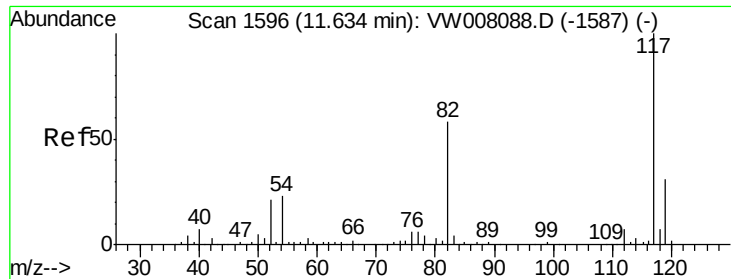

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.63 min Scan# 1596
Delta R.T. -0.00 min
Lab File: VW008143.D
Acq: 10 Jan 2019 12:15

Instrument :
MSVOA_W
ClientSampleId :
VW0110SBL01

Tot Ion:117 Resp: 108676
Ion Ratio Lower Upper
117 100
82 59.1 46.4 69.6
119 30.9 24.7 37.1

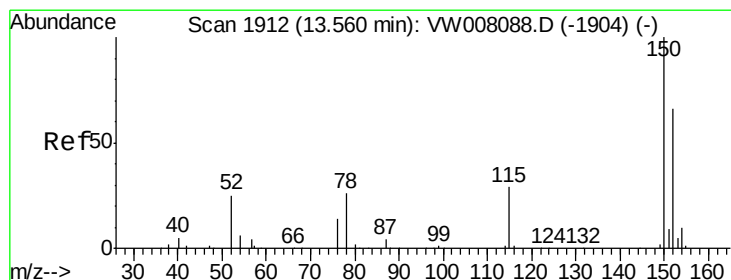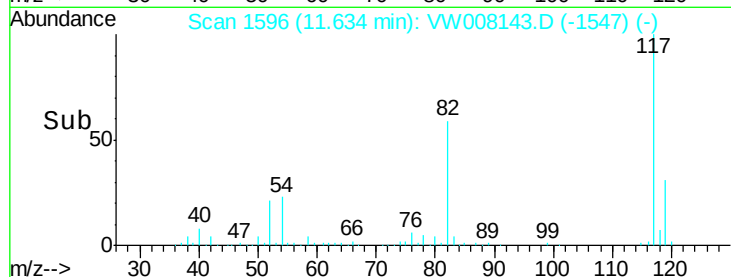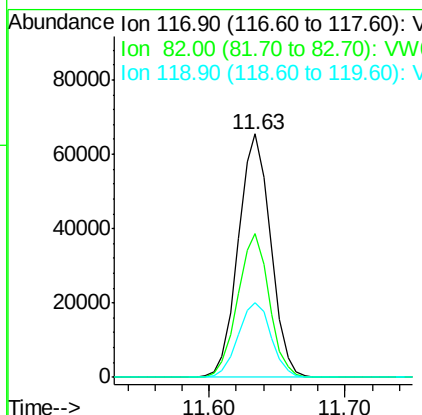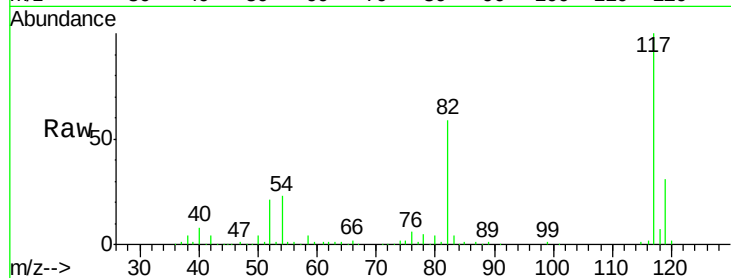

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.56 min Scan# 1912
Delta R.T. -0.00 min
Lab File: VW008143.D
Acq: 10 Jan 2019 12:15

Tgt Ion:152 Resp: 47229
Ion Ratio Lower Upper
152 100
115 61.2 30.8 92.4
150 159.7 0.0 350.2

