

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW011019\
 Data File : VW008164.D
 Acq On : 10 Jan 2019 22:06
 Operator : SY/AP
 Sample : K1088-11MSD
 Misc : 5.04G/5ML/MSVOA W/SOIL
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 CPSB-06(15-20)MSD

Quant Time: Jan 11 07:01:27 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W010819S.M
 Quant Title : SW846 8260
 QLast Update : Wed Jan 09 04:40:48 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	101991	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	183044	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	170109	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	79452	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.31	65	58299	50.86	ug/l	0.00
Spiked Amount 50.000			Recovery	=	101.72%	
35) Dibromofluoromethane	7.88	113	56579	53.00	ug/l	0.00
Spiked Amount 50.000			Recovery	=	106.00%	
50) Toluene-d8	10.32	98	235992	52.68	ug/l	0.00
Spiked Amount 50.000			Recovery	=	105.36%	
62) 4-Bromofluorobenzene	12.62	95	83770	52.16	ug/l	0.00
Spiked Amount 50.000			Recovery	=	104.32%	
Target Compounds						
16) Acetone	4.14	43	8214	20.445	ug/l	Qvalue 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW011019\
Data File : VW008164.D
Acq On : 10 Jan 2019 22:06
Operator : SY/AP
Sample : K1088-11MSD
Misc : 5.04G/5ML/MSVOA W/SOIL
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
CPSB-06(15-20)MSD

Quant Time: Jan 11 07:01:27 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W010819S.M
Quant Title : SW846 8260
QLast Update : Wed Jan 09 04:40:48 2019
Response via : Initial Calibration

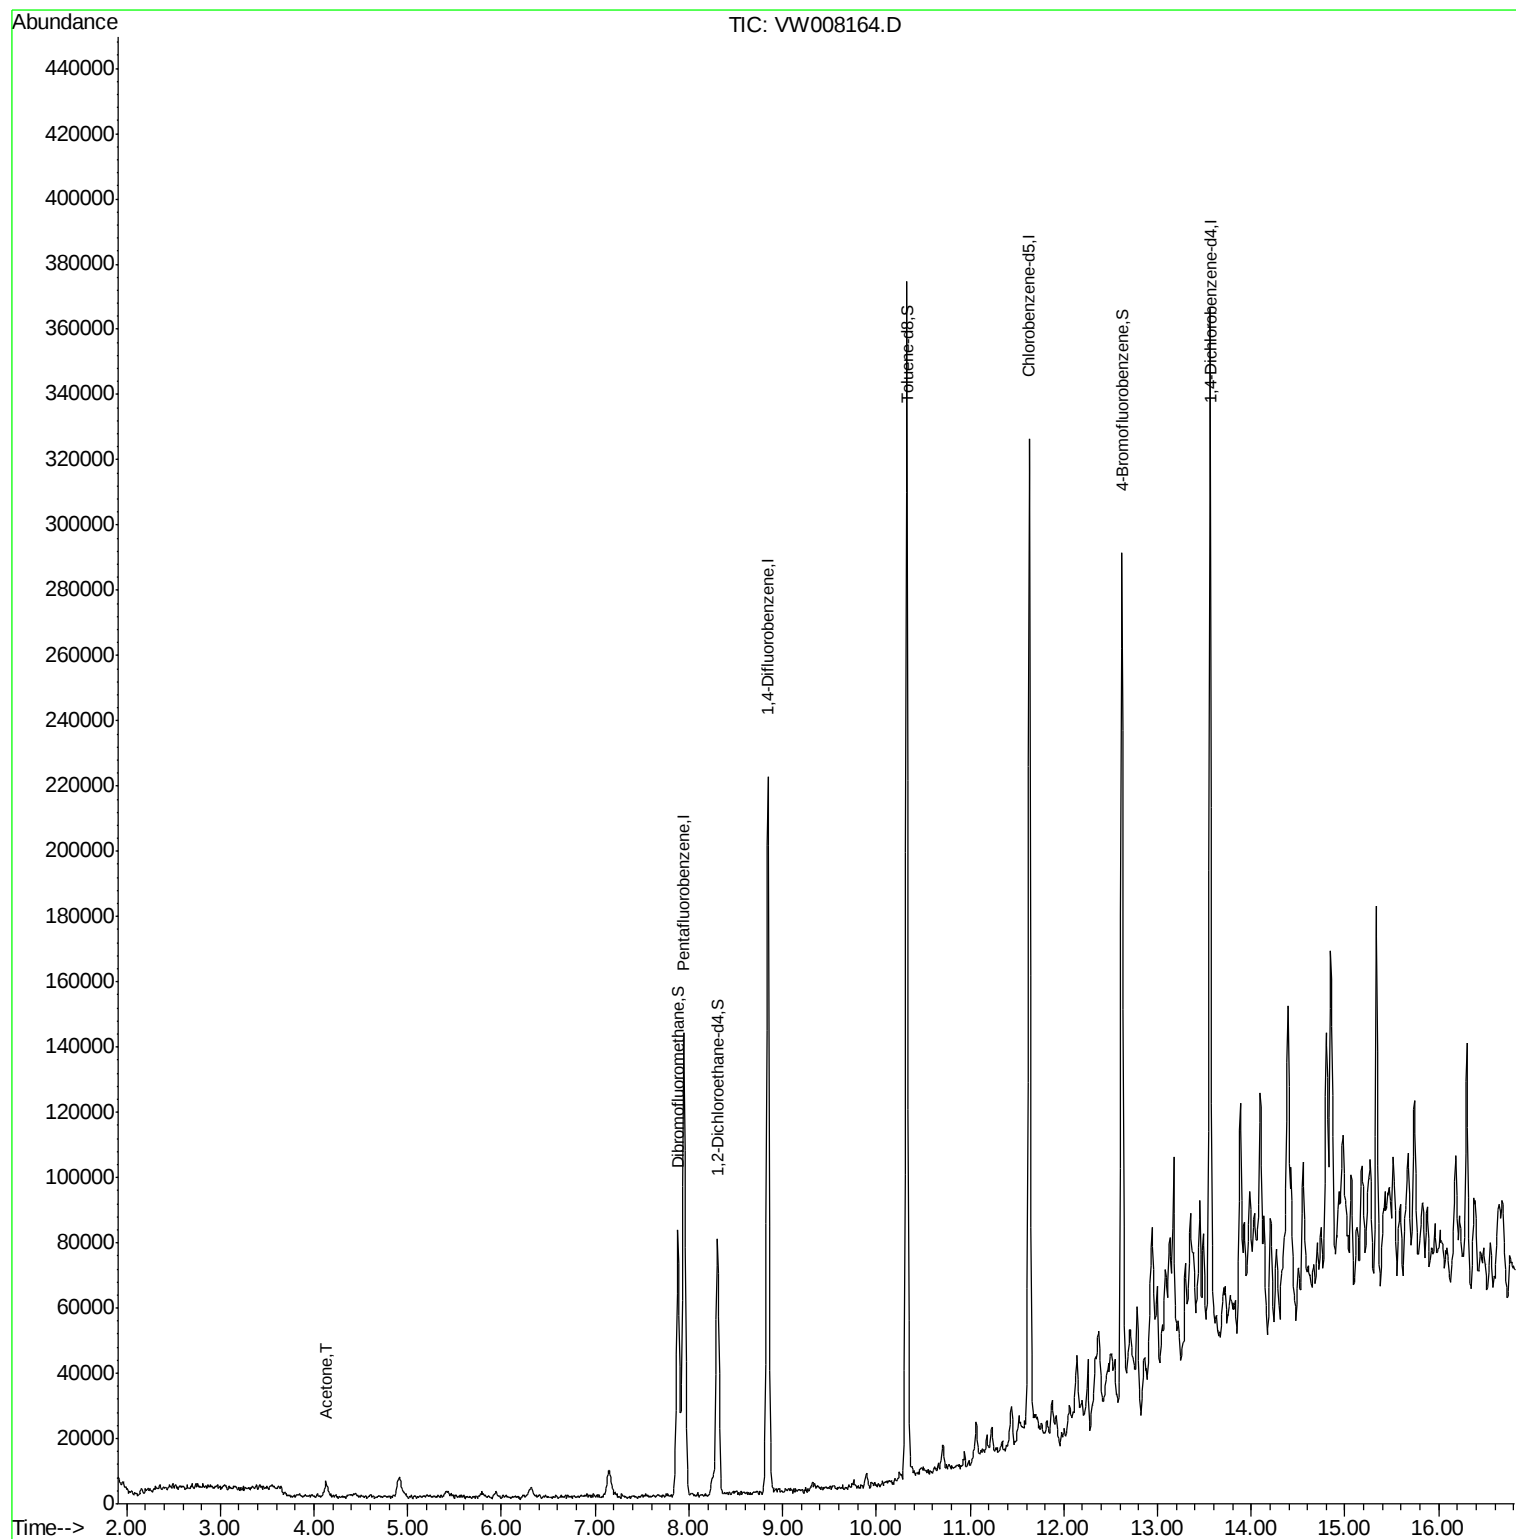

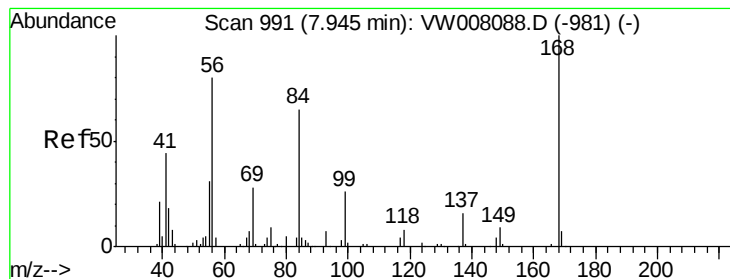

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 991

Delta R.T. -0.00 min

Lab File: VW008164.D

Acq: 10 Jan 2019 22:06

Instrument :

MSVOA_W

ClientSampleId :


CPSB-06(15-20)MSD

Tot Ion:168 Resp: 101991

Ion Ratio Lower Upper

168 100

99 61.2 52.6 78.8

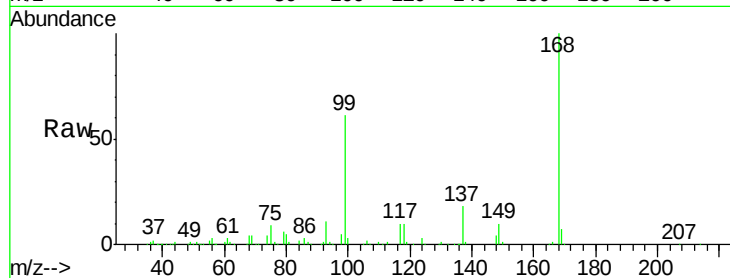

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

7.95

50000

40000



30000

20000

10000

0

Time-->

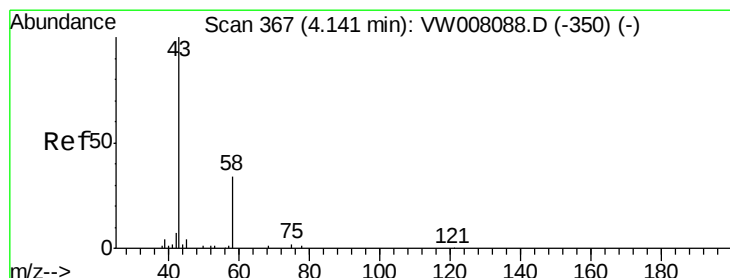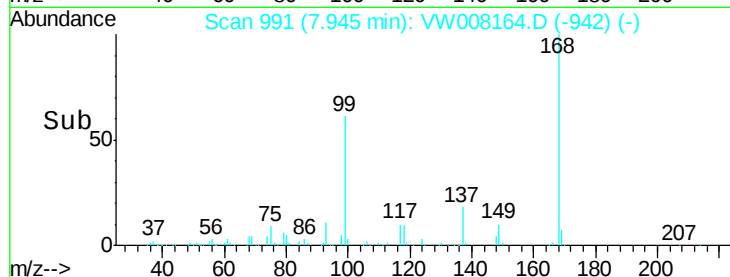

#16

Acetone

Concen: 20.445 ug/l

RT: 4.14 min Scan# 366

Delta R.T. -0.01 min

Lab File: VW008164.D


Acq: 10 Jan 2019 22:06

Tgt Ion: 43 Resp: 8214

Ion Ratio Lower Upper

43 100

58 30.9 27.5 41.3

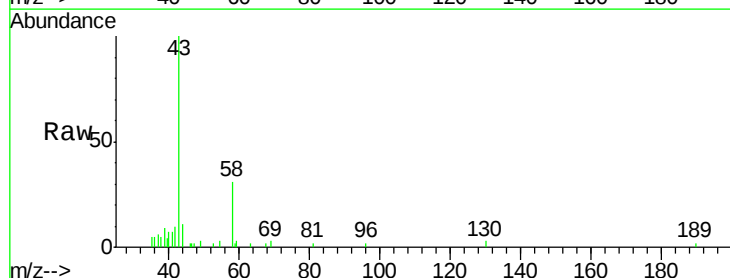

Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 58.00 (57.70 to 58.70): VW

4.14


3000


2000

1000

0

Time-->




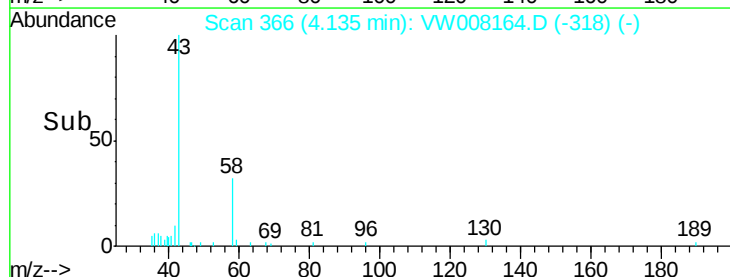


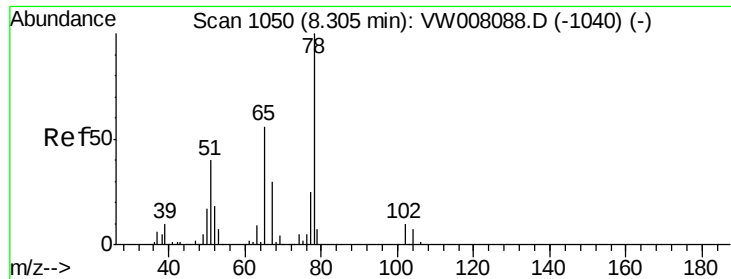

#33
 1,2-Dichloroethane-d4
 Concen: 50.859 ug/l
 RT: 8.31 min Scan# 1050
 Delta R.T. -0.00 min
 Lab File: VW008164.D
 Acq: 10 Jan 2019 22:06




Instrument :
 MSVOA_W
 ClientSampleId :
 CPSB-06(15-20)MSD


Tot Ion: 65 Resp: 58299
 Ion Ratio Lower Upper
 65 100
 67 54.5 0.0 106.8

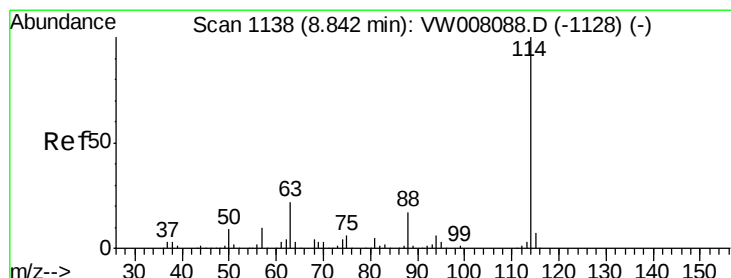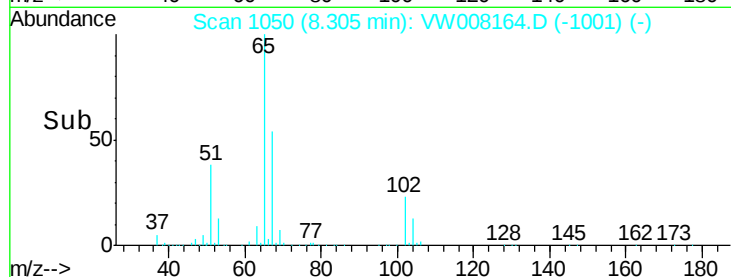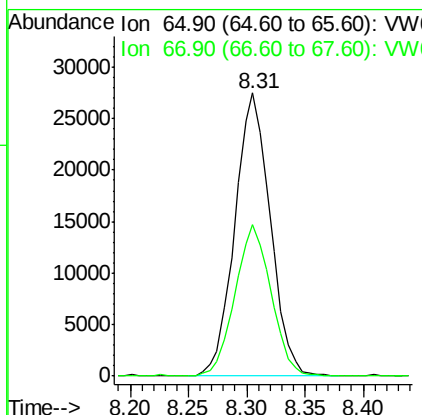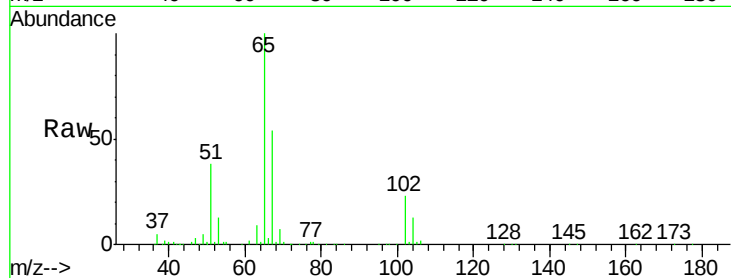

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.84 min Scan# 1138
 Delta R.T. -0.00 min
 Lab File: VW008164.D
 Acq: 10 Jan 2019 22:06

Tgt Ion: 114 Resp: 183044
 Ion Ratio Lower Upper
 114 100
 63 22.0 0.0 43.4
 88 15.8 0.0 33.4

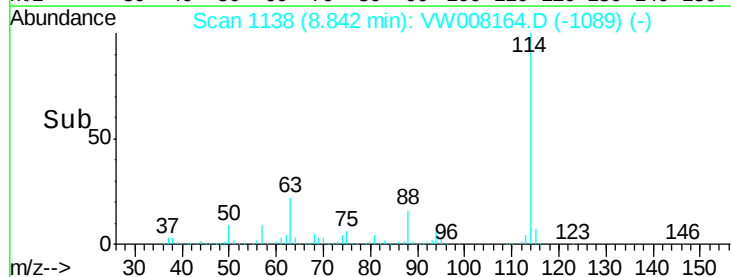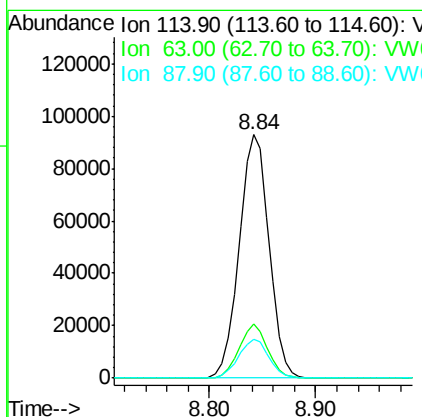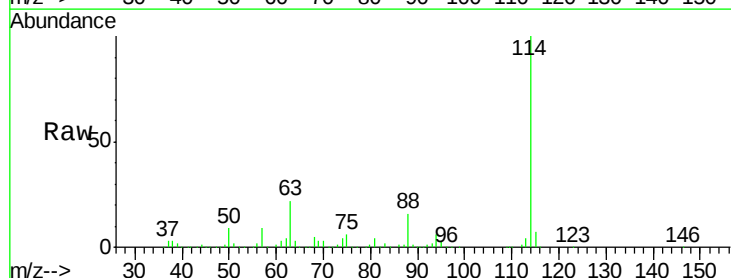

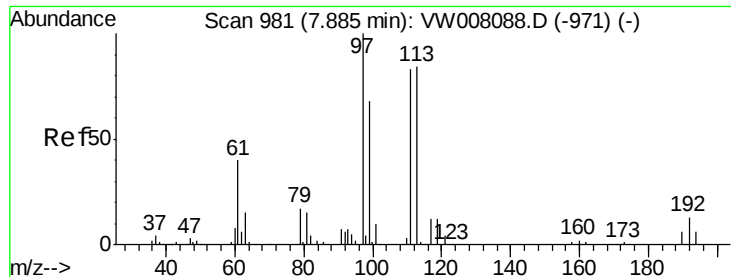

#35

Dibromofluoromethane

Concen: 52.997 ug/l

RT: 7.88 min Scan# 981

Delta R.T. 0.00 min

Lab File: VW008164.D

Acq: 10 Jan 2019 22:06

Instrument :

MSVOA_W

ClientSampleId :

CPSB-06(15-20)MSD


Tot Ion:113 Resp: 56579

Ion Ratio Lower Upper

113 100

111 103.0 81.8 122.8




192 18.1 12.8 19.2

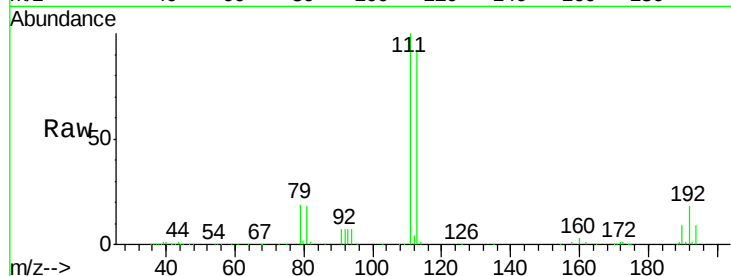

Abundance Ion 112.80 (112.50 to 113.50): V

Ion 110.80 (110.50 to 111.50): V

Ion 191.70 (191.40 to 192.40): V

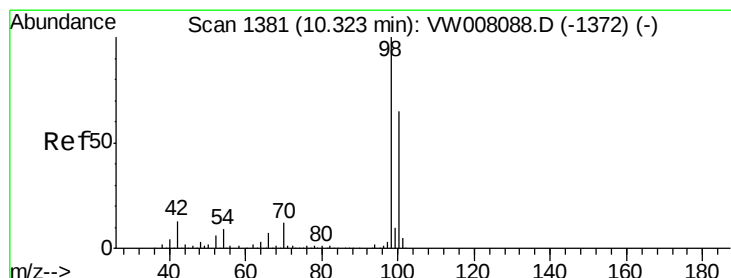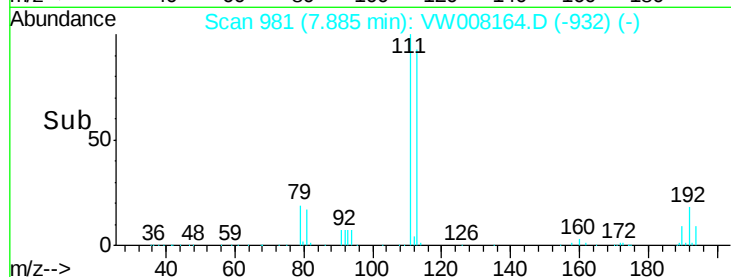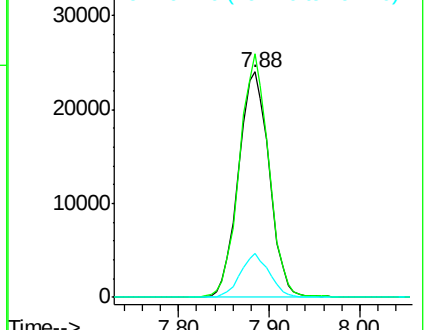

#50

Toluene-d8

Concen: 52.677 ug/l

RT: 10.32 min Scan# 1381

Delta R.T. 0.00 min

Lab File: VW008164.D


Acq: 10 Jan 2019 22:06

Tgt Ion: 98 Resp: 235992

Ion Ratio Lower Upper



98 100


100 64.5 51.7 77.5

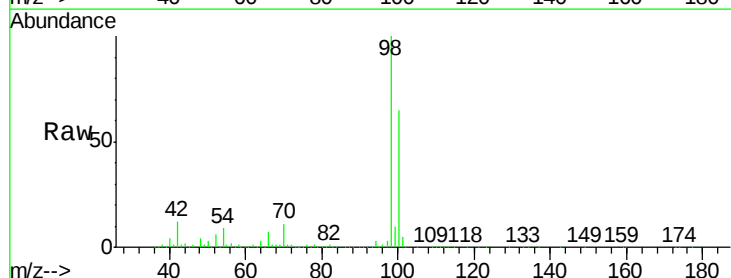

Abundance Ion 98.00 (97.70 to 98.70): VW

Ion 100.00 (99.70 to 100.70): VW



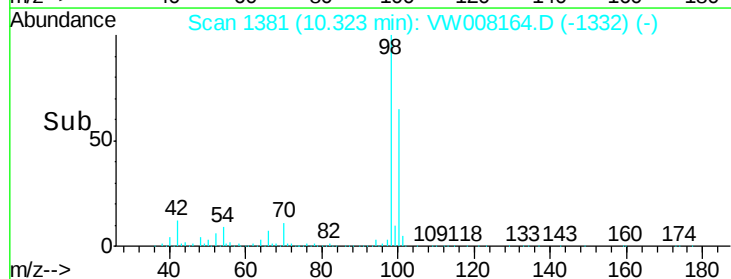
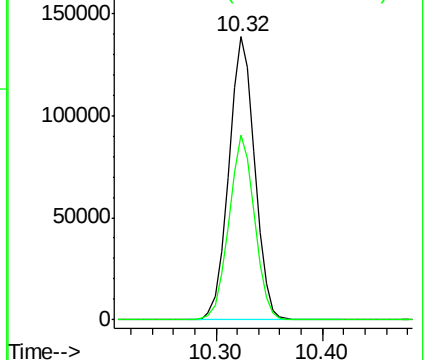


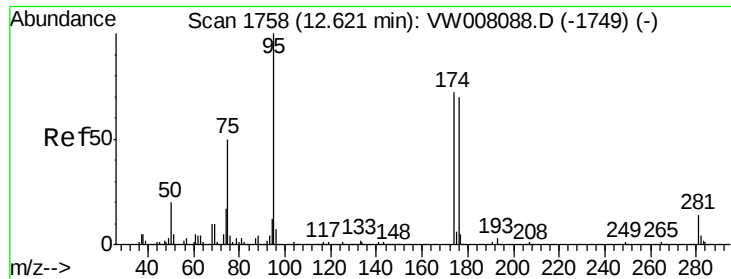

#62
4-Bromofluorobenzene
Concen: 52.158 ug/l
RT: 12.62 min Scan# 1758
Delta R.T. 0.00 min
Lab File: VW008164.D
Acq: 10 Jan 2019 22:06




Instrument :
MSVOA_W
ClientSampleId :
CPSB-06(15-20)MSD


Tot Ion: 95 Resp: 83770
Ion Ratio Lower Upper
95 100
174 72.8 0.0 143.0
176 71.1 0.0 140.2

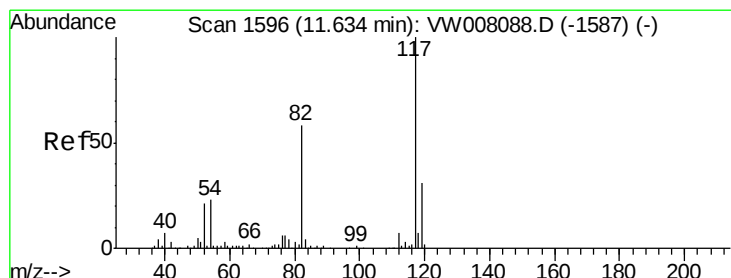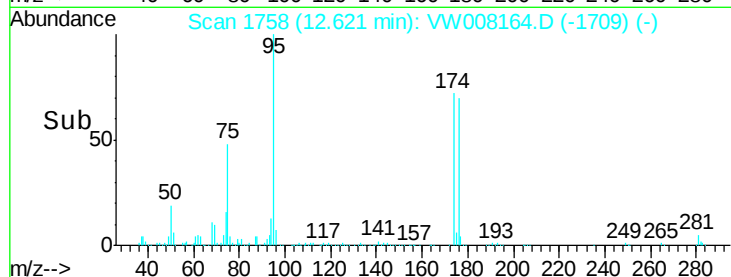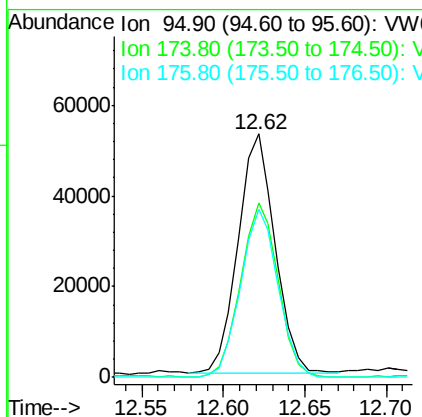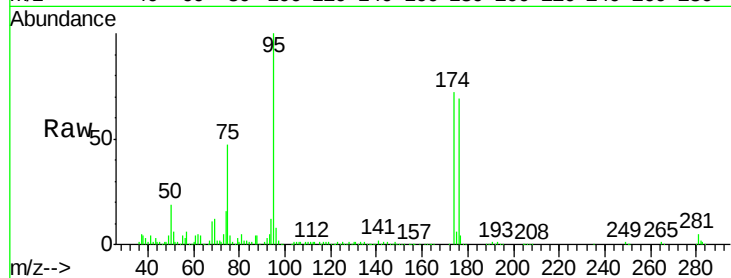

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.63 min Scan# 1596
Delta R.T. -0.00 min
Lab File: VW008164.D
Acq: 10 Jan 2019 22:06

Tgt Ion: 117 Resp: 170109
Ion Ratio Lower Upper
117 100
82 54.7 46.4 69.6
119 31.1 24.7 37.1

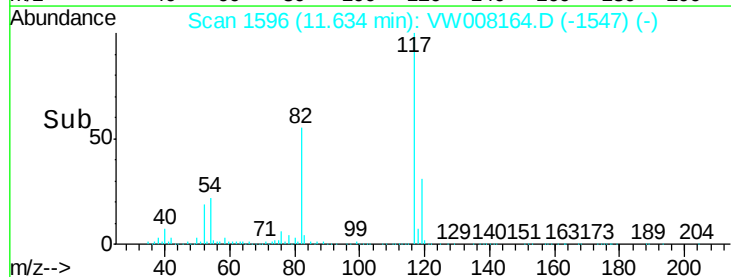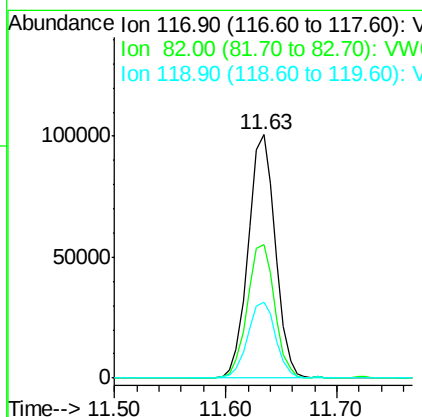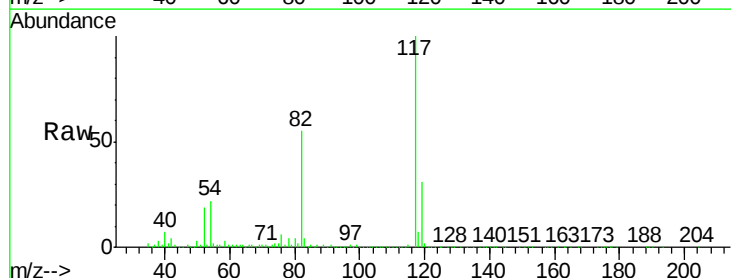

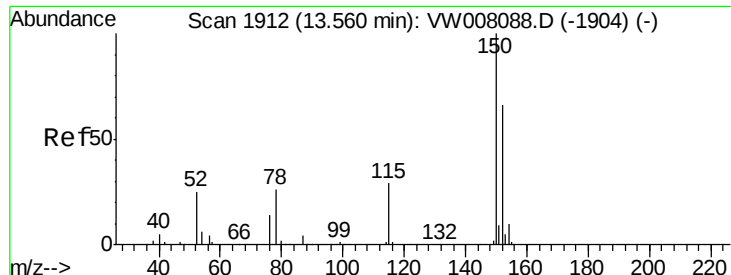

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.56 min Scan# 1912

Delta R.T. -0.00 min

Lab File: VW008164.D

Acq: 10 Jan 2019 22:06

Instrument :

MSVOA_W

ClientSampleId :

CPSB-06(15-20)MSD


Tot Ion:152 Resp: 79452

Ion Ratio Lower Upper

152 100

115 59.8 30.8 92.4

150 154.1 0.0 350.2

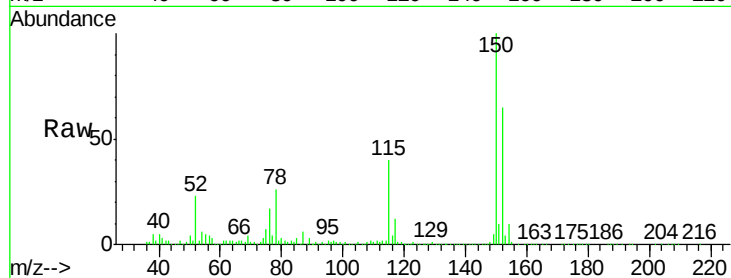

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

