


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW011019\
Data File : VW008165.D
Acq On : 10 Jan 2019 23:23
Operator : SY/AP
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W010819S.M
Title : SW846 8260
Last Update : Wed Jan 09 04:40:48 2019

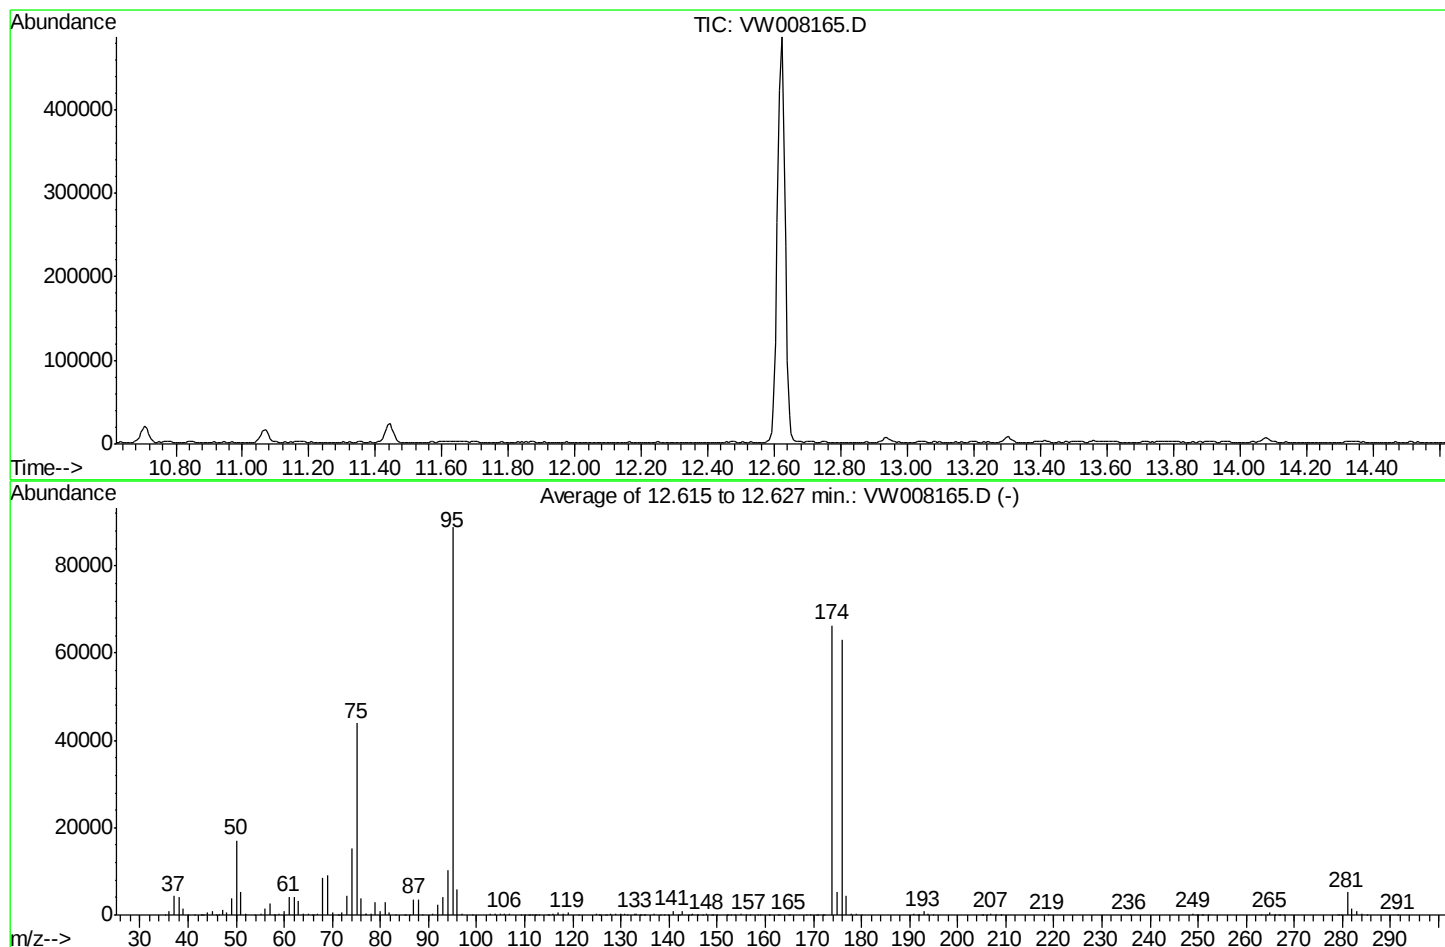

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	17021	PASS
75	95	30	60	49.5	43965	PASS
95	95	100	100	100.0	88842	PASS
96	95	5	9	6.7	5916	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	74.7	66400	PASS
175	174	5	9	8.1	5356	PASS
176	174	95	101	95.2	63200	PASS
177	176	5	9	6.8	4298	PASS