


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW011119\  
Data File : VW008191.D  
Acq On : 11 Jan 2019 12:20  
Operator : SY/AP  
Sample : BFB  
Misc : 5.00G/5ML/MSVOA W/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_W  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_W\METHOD\82W010819S.M  
Title : SW846 8260  
Last Update : Wed Jan 09 04:40:48 2019

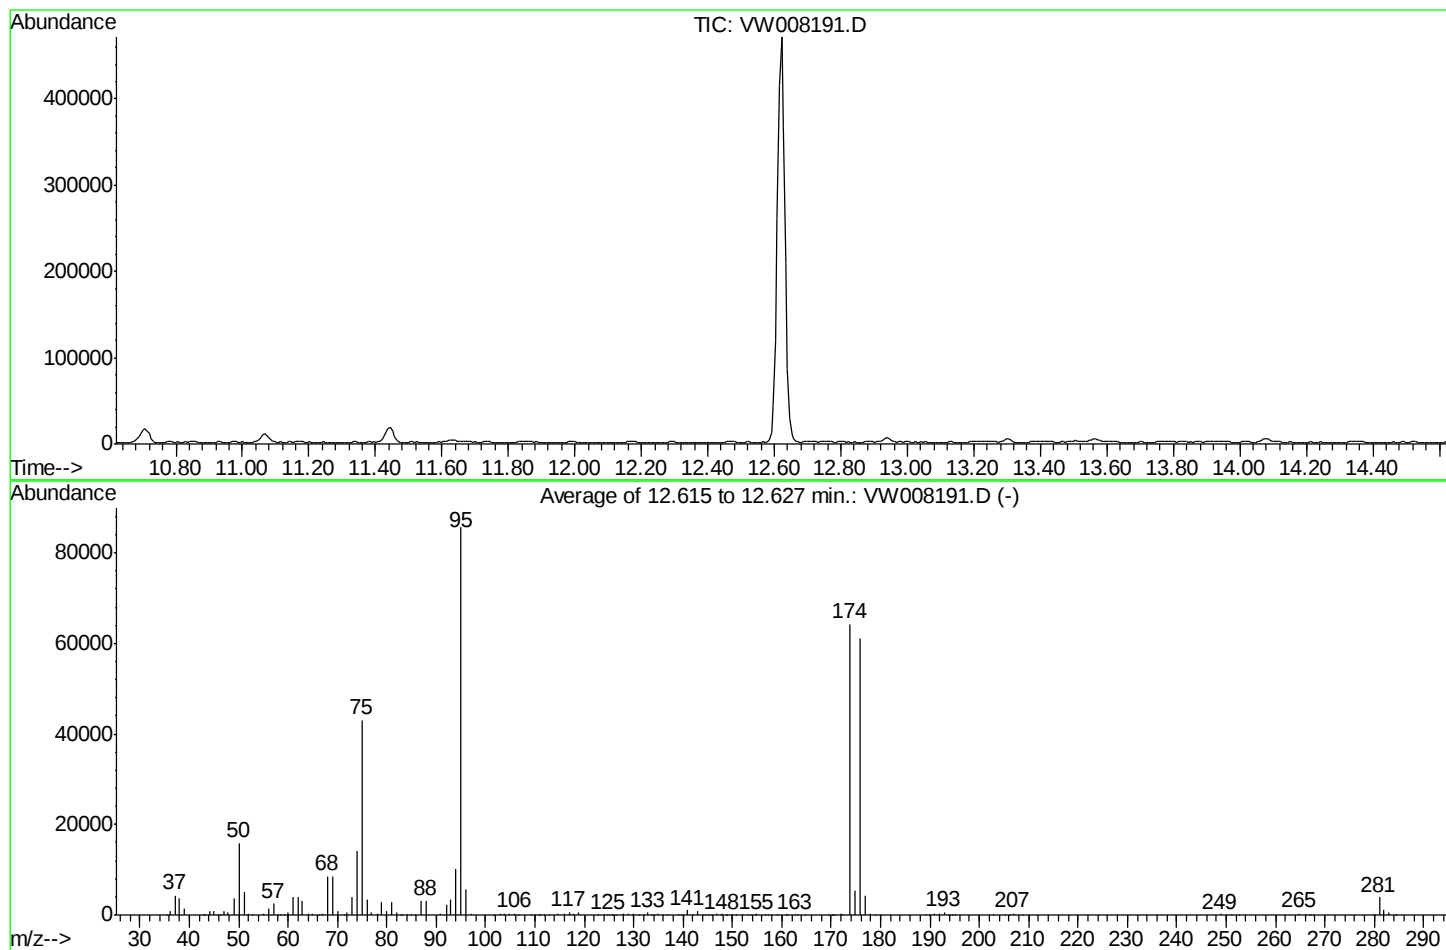

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 18.5      | 15882   | PASS             |
| 75          | 95           | 30           | 60           | 50.4      | 43122   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 85632   | PASS             |
| 96          | 95           | 5            | 9            | 6.7       | 5759    | PASS             |
| 173         | 174          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 174         | 95           | 50           | 100          | 75.0      | 64192   | PASS             |
| 175         | 174          | 5            | 9            | 8.5       | 5446    | PASS             |
| 176         | 174          | 95           | 101          | 95.3      | 61165   | PASS             |
| 177         | 176          | 5            | 9            | 7.0       | 4294    | PASS             |