

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW011121\
Data File : VW017812.D
Acq On : 11 Jan 2021 12:09
Operator : SY/VA
Sample : VW0111SBL01
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
VBLK20

Manual Integrations
APPROVED

SAM

1/12/2021 9:29:52 PM

Quant Time: Jan 12 05:35:06 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122420S.M
Quant Title : VOC Analysis
QLast Update : Tue Jan 12 05:24:52 2021
Response via : Initial Calibration

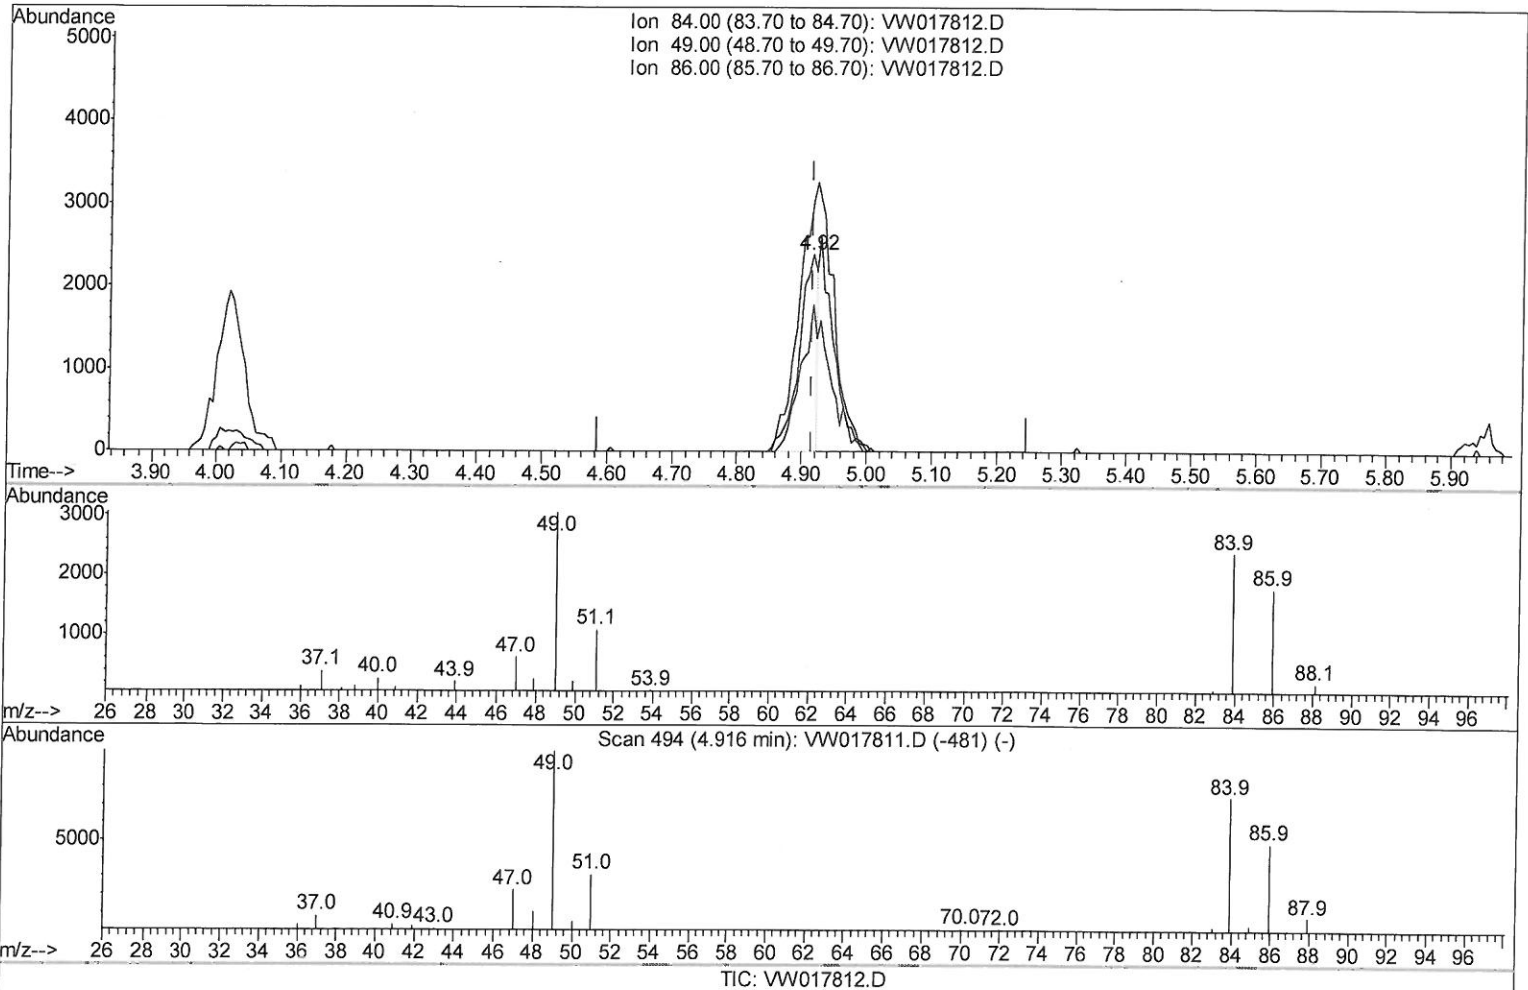

(16) Methylene chloride (T)

4.915min (-0.000) 1.05ug/L

response 4620

Ion	Exp%	Act%
84.00	100	100
49.00	129.30	127.49
86.00	64.00	74.64
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW011121\
 Data File : VW017812.D
 Acq On : 11 Jan 2021 12:09
 Operator : SY/VA
 Sample : VW0111SBL01
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1


Instrument :
 MSVOA_W
 ClientSampled :
 VBLK20

Manual Integrations
 APPROVED

Quant Time: Jan 12 05:35:06 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122420S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jan 12 05:24:52 2021
 Response via : Initial Calibration

SAM

1/12/2021 9:29:52 PM

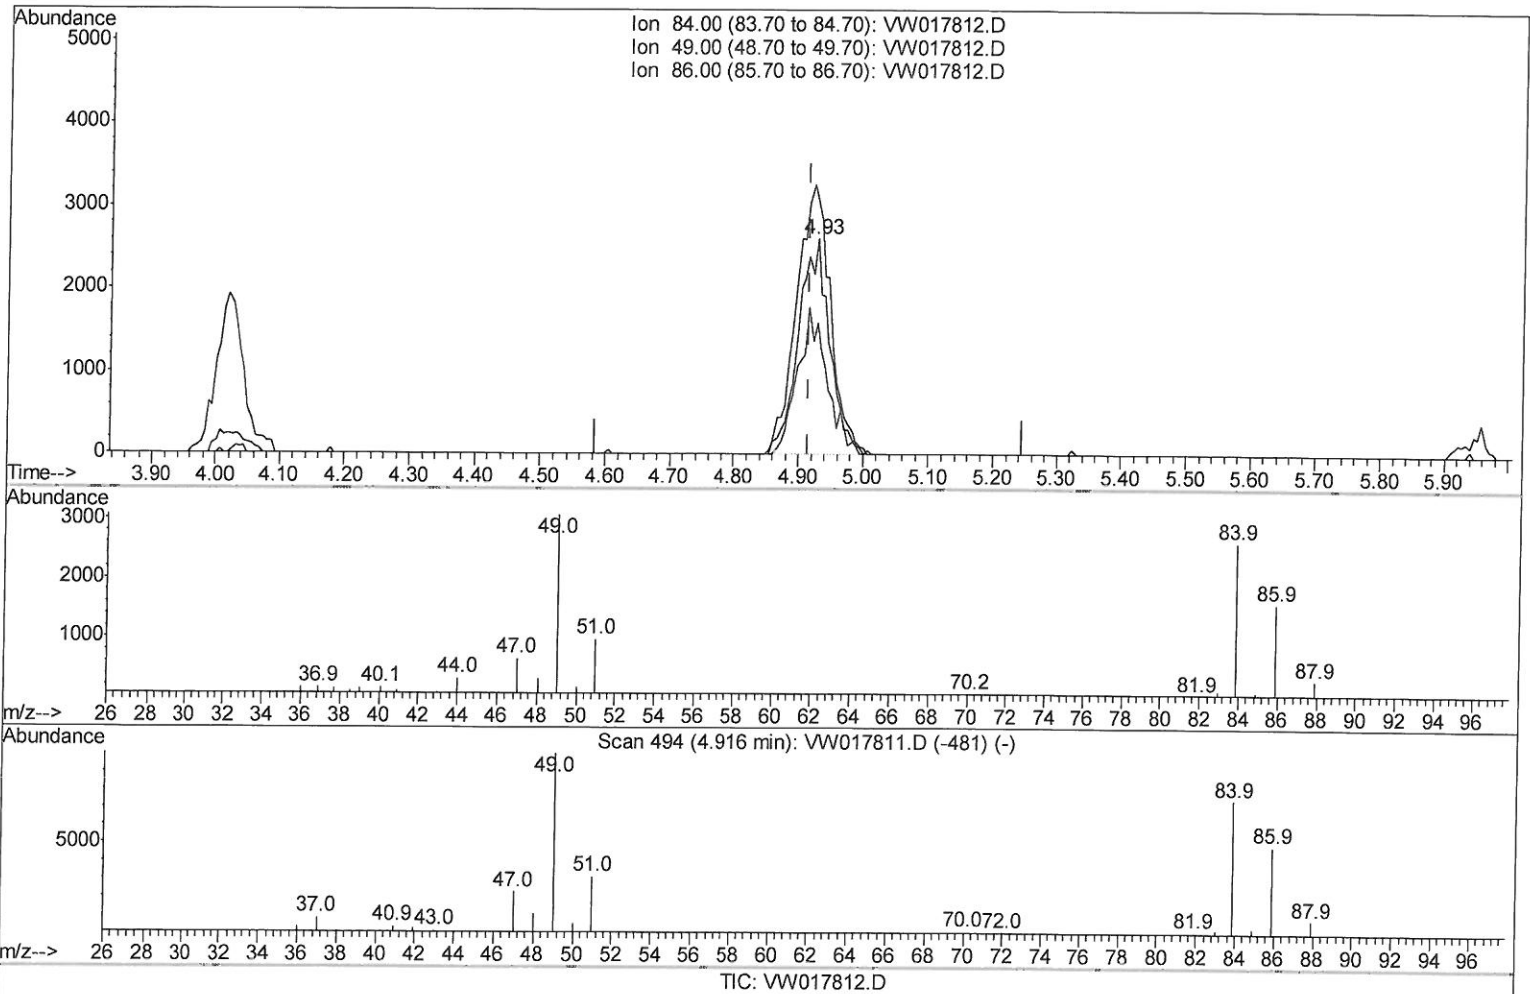

(16) Methylene chloride (T)

4.928min (+0.012) 1.98ug/L m

response 8732

Ion	Exp%	Act%
84.00	100	100
49.00	129.30	117.21
86.00	64.00	60.79
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW011121\
 Data File : VW017812.D
 Acq On : 11 Jan 2021 12:09
 Operator : SY/VA
 Sample : VW0111SBL01
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK20

Manual Integrations
 APPROVED

SAM

1/12/2021 9:29:52 PM

Quant Time: Jan 12 05:36:12 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122420S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jan 12 05:24:52 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	308930	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	277781	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	130269	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	99809	20.88	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.52%
7) Chloroethane-d5	2.89	69	88093	22.33	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.32%
10) 1,1-Dichloroethene-d2	4.02	63	142690	17.13	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.52%
20) 2-Butanone-d5	7.08	46	47387	61.17	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	122.34%
24) Chloroform-d	7.65	84	192665	23.87	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.48%
26) 1,2-Dichloroethane-d4	8.31	65	112097	26.83	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	107.32%
29) Benzene-d6	8.27	84	371423	23.74	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.96%
33) 1,2-Dichloropropane-d6	9.27	67	110571	25.64	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	102.56%
37) Toluene-d8	10.32	98	345554	22.99	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	91.96%
38) trans-1,3-Dichloropropene-	10.58	79	46903	24.40	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	97.60%
39) 2-Hexanone-d5	10.93	63	31006	57.24	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	114.48%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	82175	25.66	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	102.64%
61) 1,2-Dichlorobenzene-d4	13.85	152	104183	22.97	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	91.88%

Target Compounds

16) Methylene chloride	4.93	84	8732m	1.977	ug/L	Ovalue
------------------------	------	----	-------	-------	------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

01/15/21 by

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW011121\
Data File : VW017812.D
Acq On : 11 Jan 2021 12:09
Operator : SY/VA
Sample : VW0111SBL01
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
VBLK20

Manual Integrations
APPROVED

SAM

1/12/2021 9:29:52 PM

Quant Time: Jan 12 05:36:12 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122420S.M
Quant Title : VOC Analysis
QLast Update : Tue Jan 12 05:24:52 2021
Response via : Initial Calibration

