

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011122\
 Data File : VW021847.D
 Acq On : 11 Jan 2022 21:20
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jan 12 00:52:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jan 12 00:49:08 2022
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		8.848	114	109208	25.000	ug/L	# 0.00
28) Chlorobenzene-d5		11.628	117	111052	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.554	152	66677	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.349	65	55003	27.098	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	108.400%	
7) Chloroethane-d5		2.885	69	43074	23.500	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	94.000%	
11) 1,1-Dichloroethene-d2		4.013	63	62933	19.639	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	78.560%	
21) 2-Butanone-d5		7.092	46	17112	59.728	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	119.460%	
24) Chloroform-d		7.653	84	86789	24.600	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	98.400%	
26) 1,2-Dichloroethane-d4		8.305	65	45784	26.873	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	107.480%	
32) Benzene-d6		8.275	84	180137	24.999	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	100.000%	
36) 1,2-Dichloropropane-d6		9.274	67	46522	24.495	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	97.960%	
41) Toluene-d8		10.323	98	178906	24.629	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	98.520%	
43) trans-1,3-Dichloroprop...		10.579	79	18536	22.986	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	91.960%	
47) 2-Hexanone-d5		10.927	63	15943	61.863	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	123.720%	
56) 1,1,2,2-Tetrachloroeth...		12.688	84	40794	27.468	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	109.880%	
66) 1,2-Dichlorobenzene-d4		13.853	152	69887	25.491	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	101.960%	
Target Compounds							
34) Trichloroethene		8.842	95	3153	1.596	ug/L	# 5


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011122\
Data File : VW021847.D
Acq On : 11 Jan 2022 21:20
Operator : SY/VA
Sample : VIBLK
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Jan 12 00:52:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jan 12 00:49:08 2022
Response via : Initial Calibration

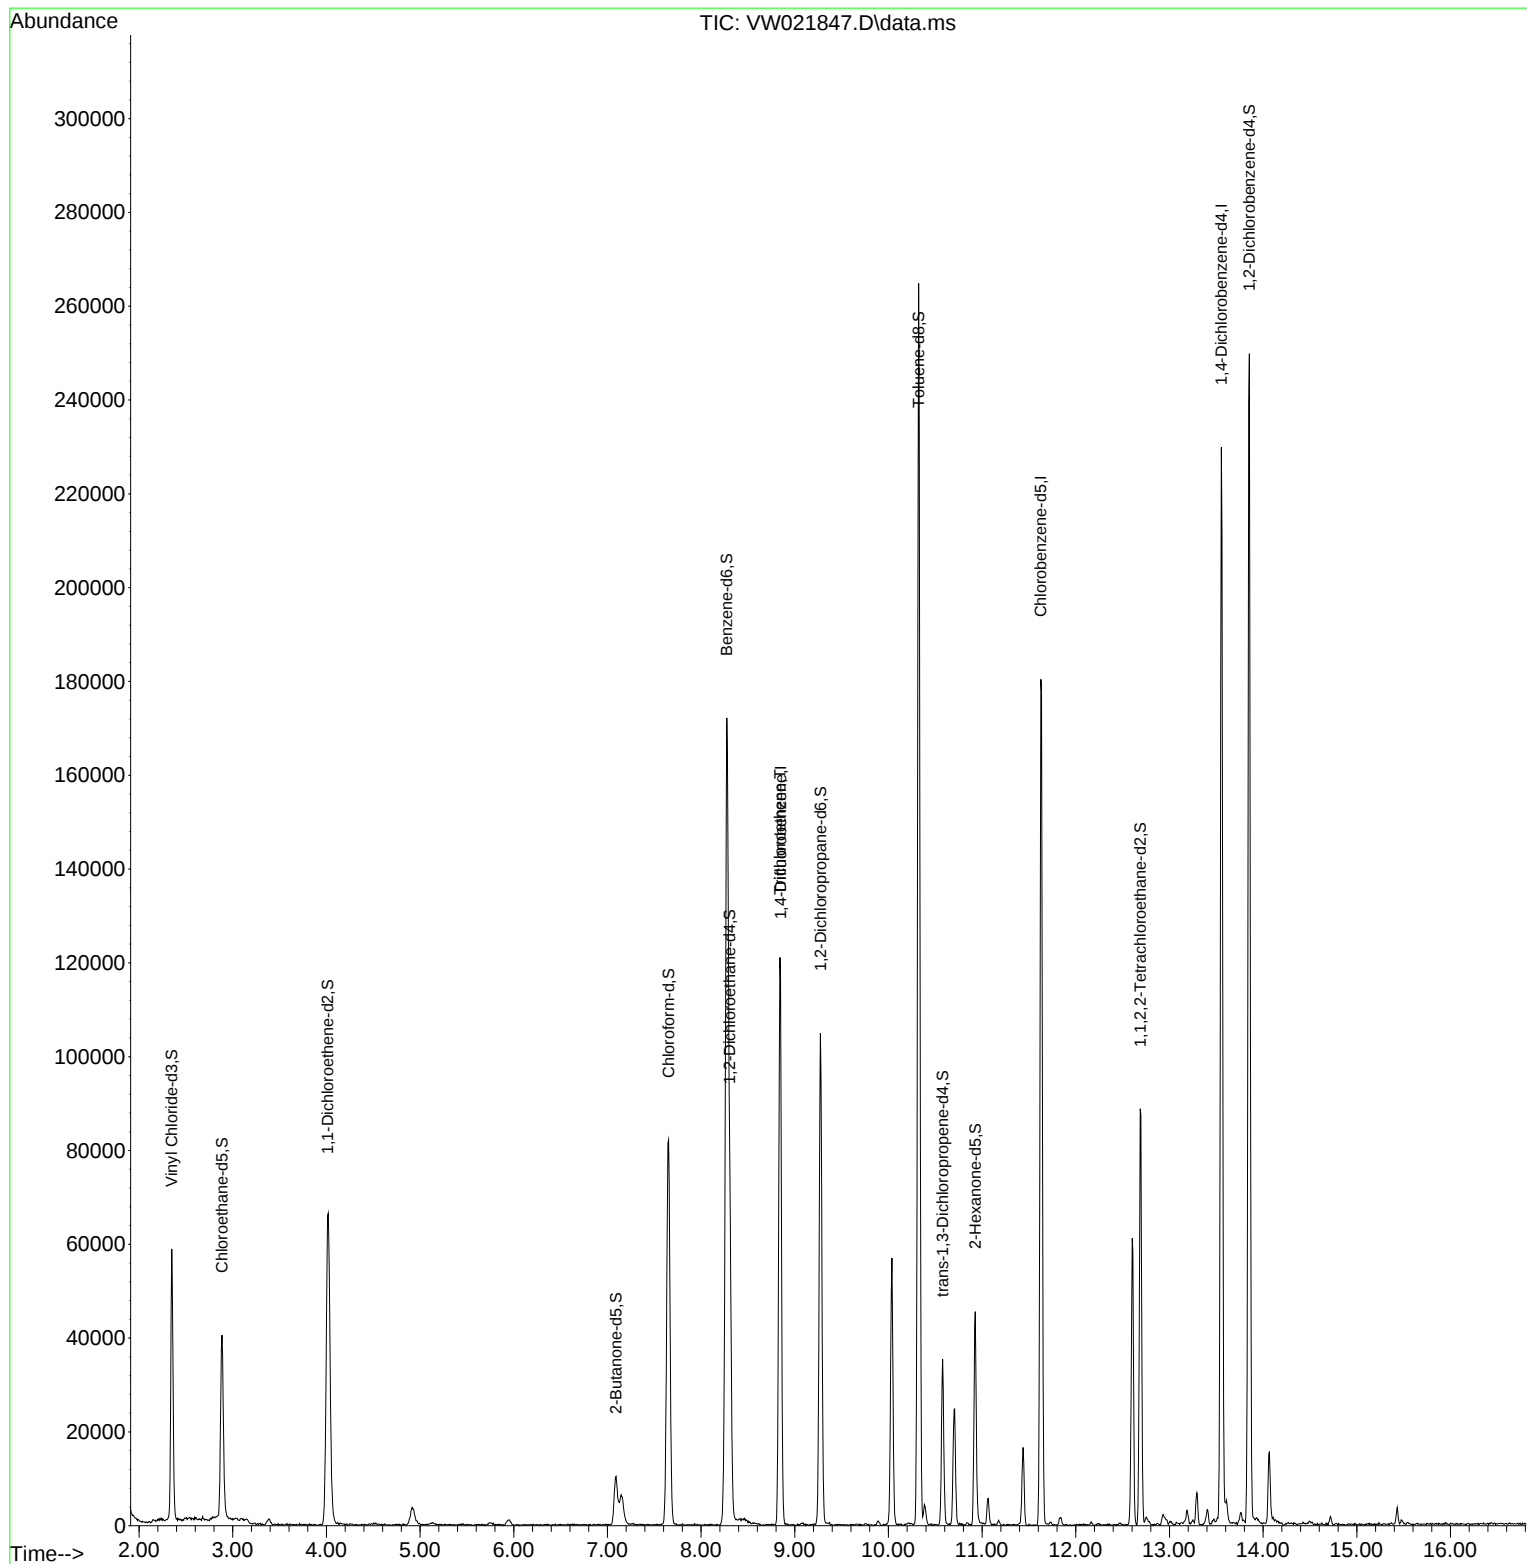

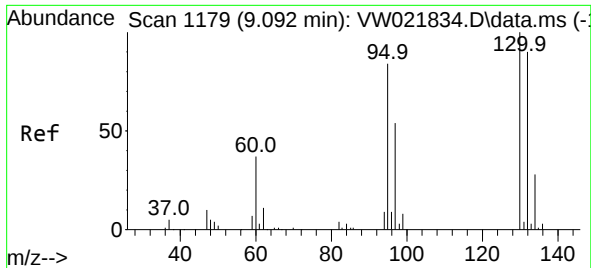

#34
 Trichloroethene
 Concen: 1.596 ug/L
 RT: 8.842 min Scan# 11
 Delta R.T. -0.250 min
 Lab File: VW021847.D
 Acq: 11 Jan 2022 21:20

Instrument :
 MSVOA_W
 ClientSampleId :

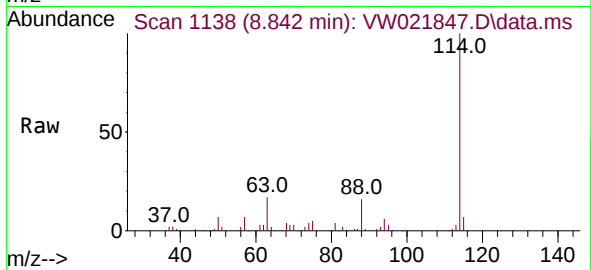

Tgt Ion:	95	Resp:	3153
Ion	Ratio	Lower	Upper
95	100		
97	0.0	47.0	87.2#
132	0.0	65.5	121.6#
130	0.0	69.4	128.8#

