




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011122\
 Data File : VW021844.D
 Acq On : 11 Jan 2022 20:08
 Operator : SY/VA
 Sample : N1084-05
 Misc : 6.43g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLM8

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/12/2022
 Supervised By :Mahesh Dadoda 01/12/2022

Quant Time: Jan 12 00:52:08 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jan 12 00:49:08 2022
 Response via : Initial Calibration

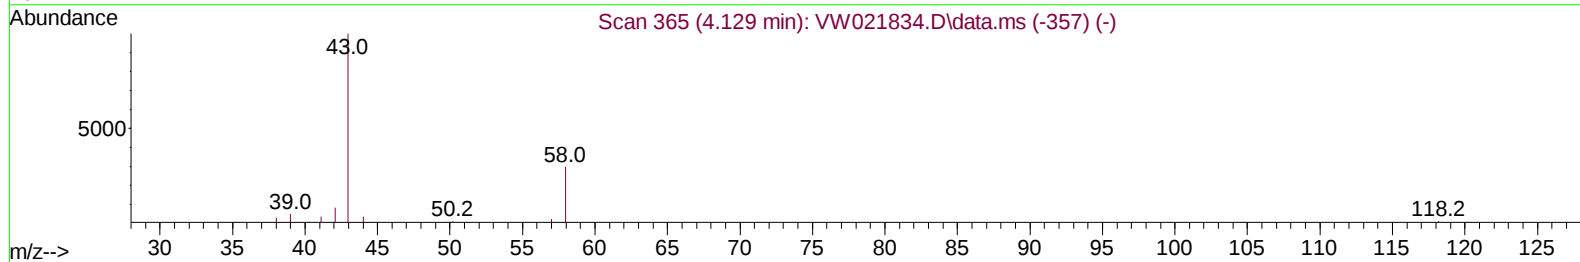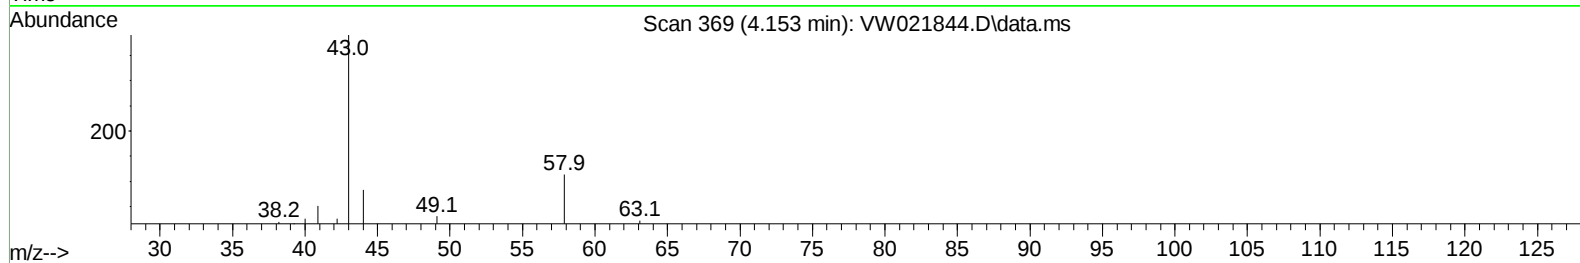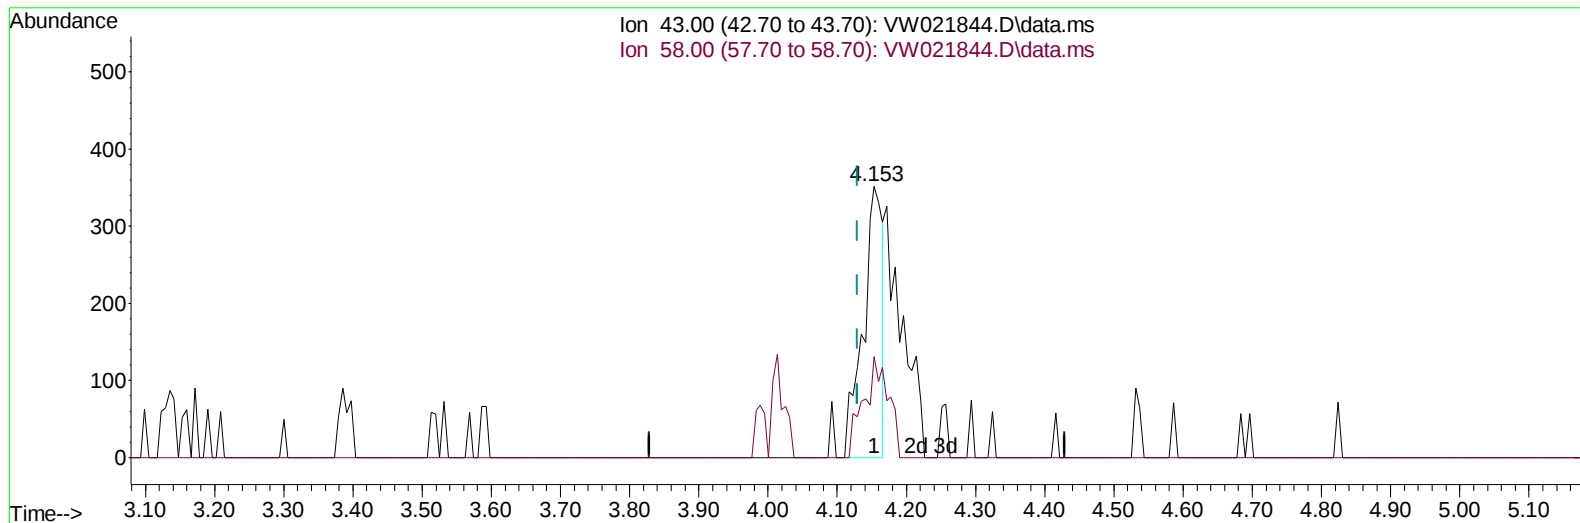

TIC: VW021844.D\data.ms

(13) Acetone (T)

4.153min (+ 0.024) 2.47 ug/L

response 691

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.40	10.71
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011122\
 Data File : VW021844.D
 Acq On : 11 Jan 2022 20:08
 Operator : SY/VA
 Sample : N1084-05
 Misc : 6.43g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLM8

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/12/2022
 Supervised By :Mahesh Dadoda 01/12/2022

Quant Time: Jan 12 00:52:08 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jan 12 00:49:08 2022
 Response via : Initial Calibration

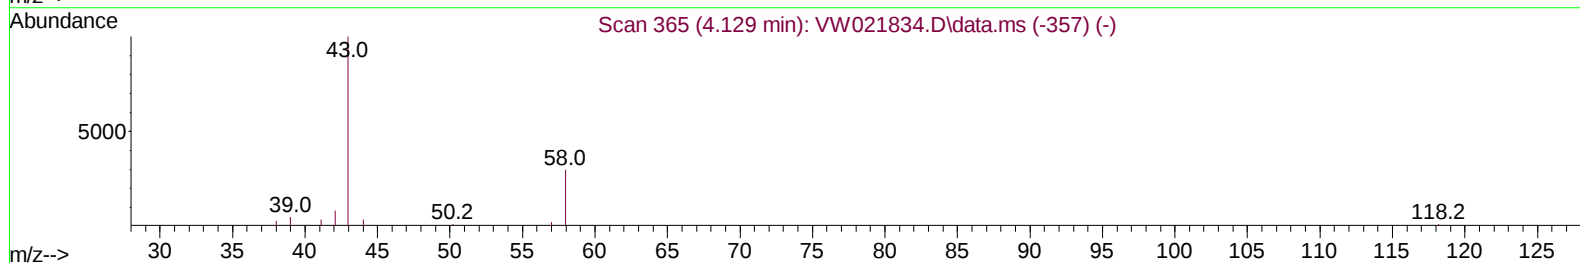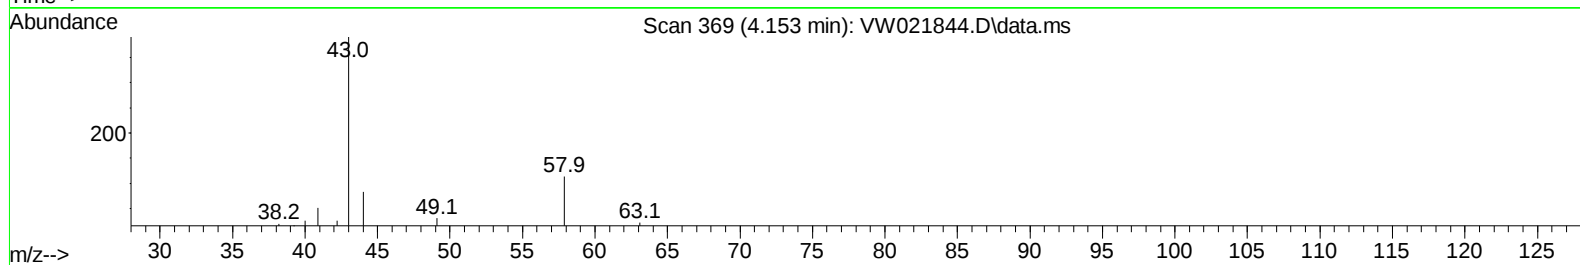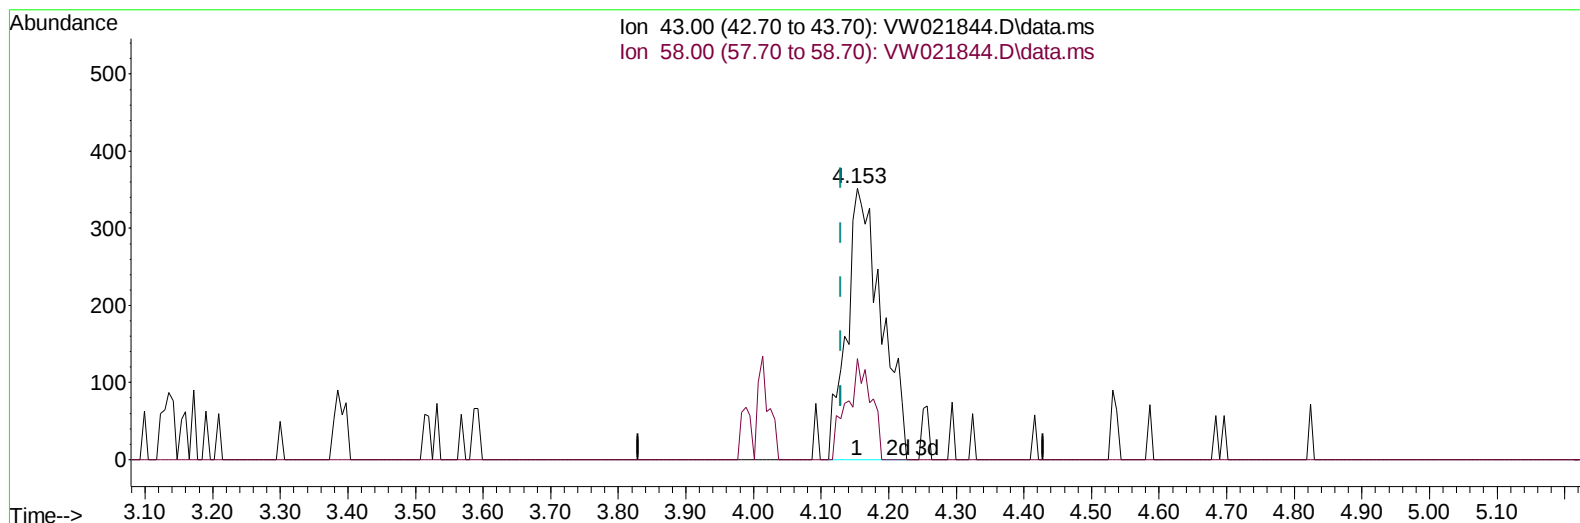

TIC: VW021844.D\data.ms

(13) Acetone (T)

4.153min (+ 0.024) 4.50 ug/L m

response 1257

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.40	5.89
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011122\
 Data File : VW021844.D
 Acq On : 11 Jan 2022 20:08
 Operator : SY/VA
 Sample : N1084-05
 Misc : 6.43g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLM8

Manual IntegrationsAPPROVED

Quant Time: Jan 12 00:52:08 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jan 12 00:49:08 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/12/2022
 Supervised By :Mahesh Dadoda 01/12/2022

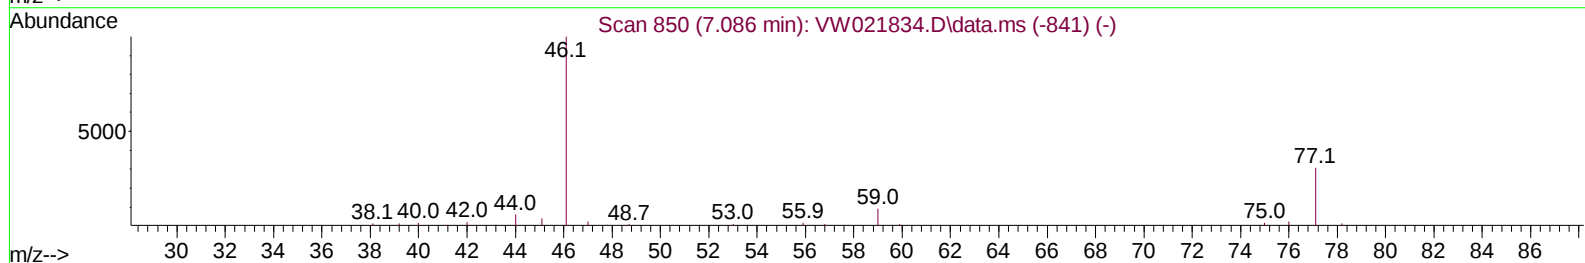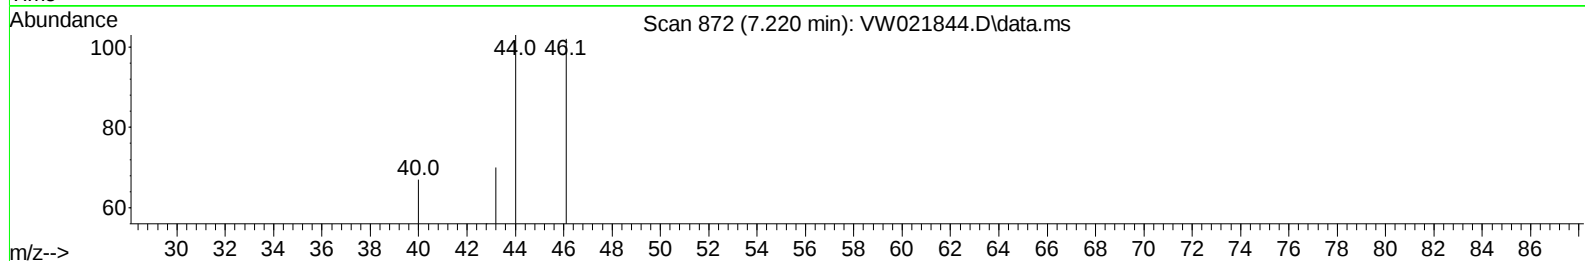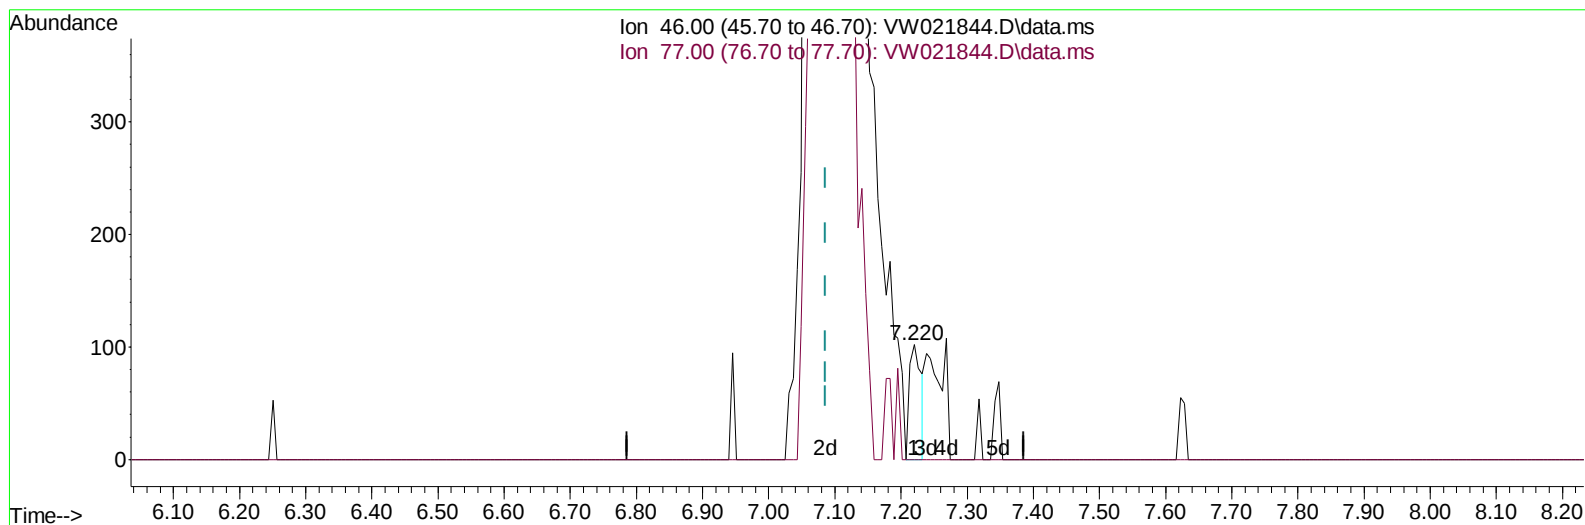

TIC: VW021844.D\data.ms

(21) 2-Butanone-d5 (S)

7.220min (+ 0.134) 0.37 ug/L

response 126

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	20.20	23.81
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011122\
 Data File : VW021844.D
 Acq On : 11 Jan 2022 20:08
 Operator : SY/VA
 Sample : N1084-05
 Misc : 6.43g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLM8

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/12/2022
 Supervised By :Mahesh Dadoda 01/12/2022

Quant Time: Jan 12 00:52:08 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jan 12 00:49:08 2022
 Response via : Initial Calibration

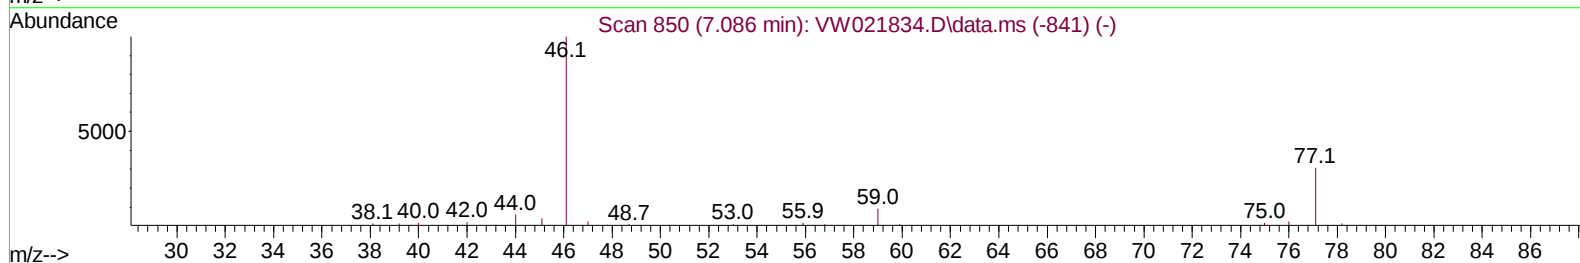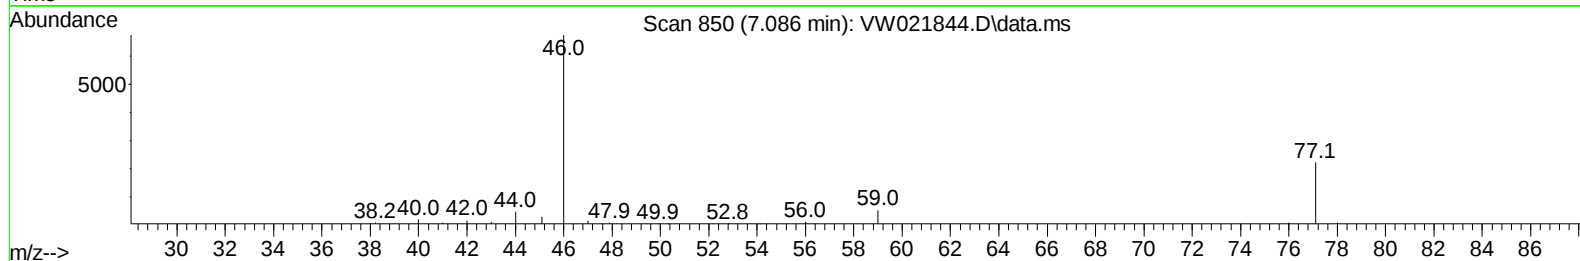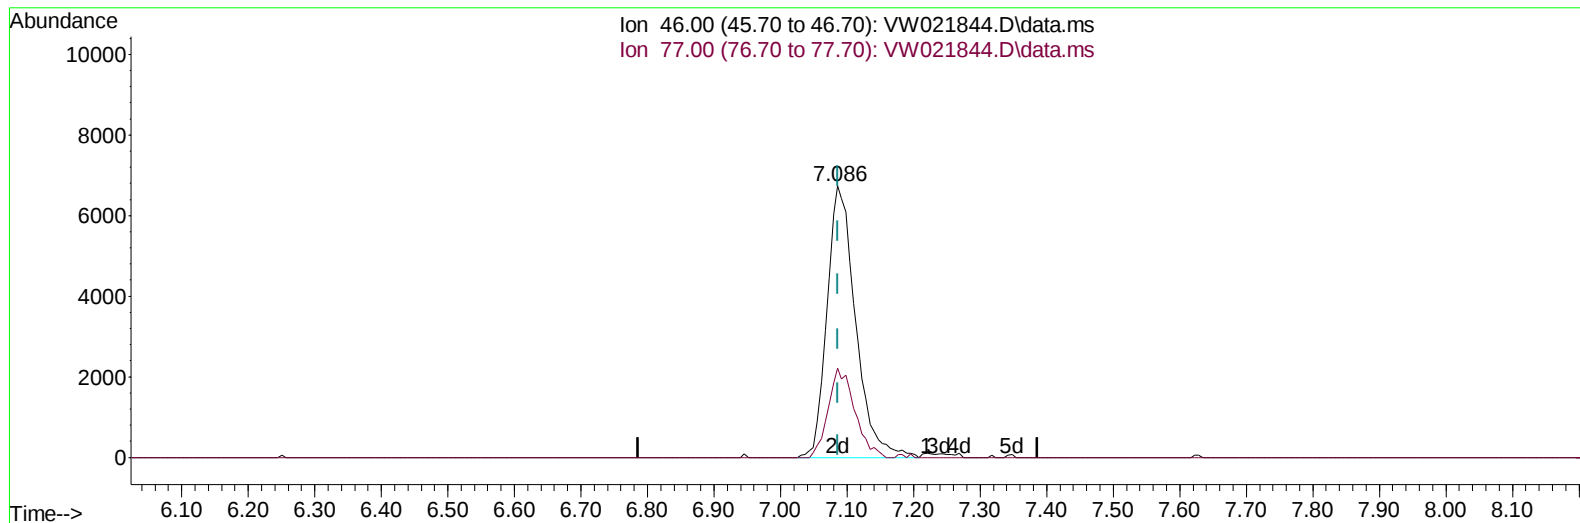

TIC: VW021844.D\data.ms

(21) 2-Butanone-d5 (S)

7.086min (-0.000) 59.30 ug/L m

response 20055

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	20.20	0.15#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011122\
 Data File : VW021844.D
 Acq On : 11 Jan 2022 20:08
 Operator : SY/VA
 Sample : N1084-05
 Misc : 6.43g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLM8

Manual IntegrationsAPPROVED

Quant Time: Jan 12 00:52:08 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jan 12 00:49:08 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/12/2022
 Supervised By :Mahesh Dadoda 01/12/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		128909	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117		114220	25.000	ug/L	# 0.00
58) 1,4-Dichlorobenzene-d4	13.560	152		42821	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65		36593	15.273	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	61.080%	
7) Chloroethane-d5	2.885	69		32508	15.025	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	60.080%	
11) 1,1-Dichloroethene-d2	4.013	63		47322	12.510	ug/L	-0.01
Spiked Amount 25.000	Range 45	- 110		Recovery	=	50.040%	
21) 2-Butanone-d5	7.086	46		20055m	59.302	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	118.600%	
24) Chloroform-d	7.647	84		81820	19.647	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	78.600%	
26) 1,2-Dichloroethane-d4	8.305	65		45297	22.524	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	90.080%	
32) Benzene-d6	8.275	84		160306	21.630	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	86.520%	
36) 1,2-Dichloropropane-d6	9.274	67		44820	22.944	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	91.760%	
41) Toluene-d8	10.323	98		148608	19.891	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	79.560%	
43) trans-1,3-Dichloroprop...	10.579	79		18251	22.005	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	88.040%	
47) 2-Hexanone-d5	10.927	63		17471	65.911	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	131.820%	
56) 1,1,2,2-Tetrachloroeth...	12.695	84		41071	26.887	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	107.560%	
66) 1,2-Dichlorobenzene-d4	13.853	152		38811	22.042	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	88.160%	
Target Compounds							
13) Acetone	4.153	43		1257m	4.499	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011122\
Data File : VW021844.D
Acq On : 11 Jan 2022 20:08
Operator : SY/VA
Sample : N1084-05
Misc : 6.43g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLM8

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/12/2022
Supervised By :Mahesh Dadoda 01/12/2022

Quant Time: Jan 12 00:52:08 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jan 12 00:49:08 2022
Response via : Initial Calibration

