

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011122\
 Data File : VW021846.D
 Acq On : 11 Jan 2022 20:56
 Operator : SY/VA
 Sample : N1084-06
 Misc : 6.21g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLM9

Quant Time: Jan 12 00:52:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jan 12 00:49:08 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	116995	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.628	117	90214	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	31683	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	36241	16.666	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	66.680%
7) Chloroethane-d5	2.879	69	34254	17.444	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	69.760%
11) 1,1-Dichloroethene-d2	4.013	63	45069	13.128	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	52.520%
21) 2-Butanone-d5	7.086	46	18562	60.477	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	120.960%
24) Chloroform-d	7.647	84	75386	19.945	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	79.800%
26) 1,2-Dichloroethane-d4	8.305	65	40871	22.393	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	89.560%
32) Benzene-d6	8.275	84	145553	24.865	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	99.440%
36) 1,2-Dichloropropane-d6	9.274	67	39926	25.877	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	103.520%
41) Toluene-d8	10.323	98	127235	21.562	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	86.240%
43) trans-1,3-Dichloroprop...	10.579	79	13402	20.459	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	81.840%
47) 2-Hexanone-d5	10.927	63	14400	68.782	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	137.560%#
56) 1,1,2,2-Tetrachloroeth...	12.688	84	31690	26.266	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	105.080%
66) 1,2-Dichlorobenzene-d4	13.853	152	25224	19.362	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	77.440%
Target Compounds						
13) Acetone	4.153	43	1716	6.767	ug/L	Qvalue 85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011122\
Data File : VW021846.D
Acq On : 11 Jan 2022 20:56
Operator : SY/VA
Sample : N1084-06
Misc : 6.21g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLM9

Quant Time: Jan 12 00:52:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jan 12 00:49:08 2022
Response via : Initial Calibration

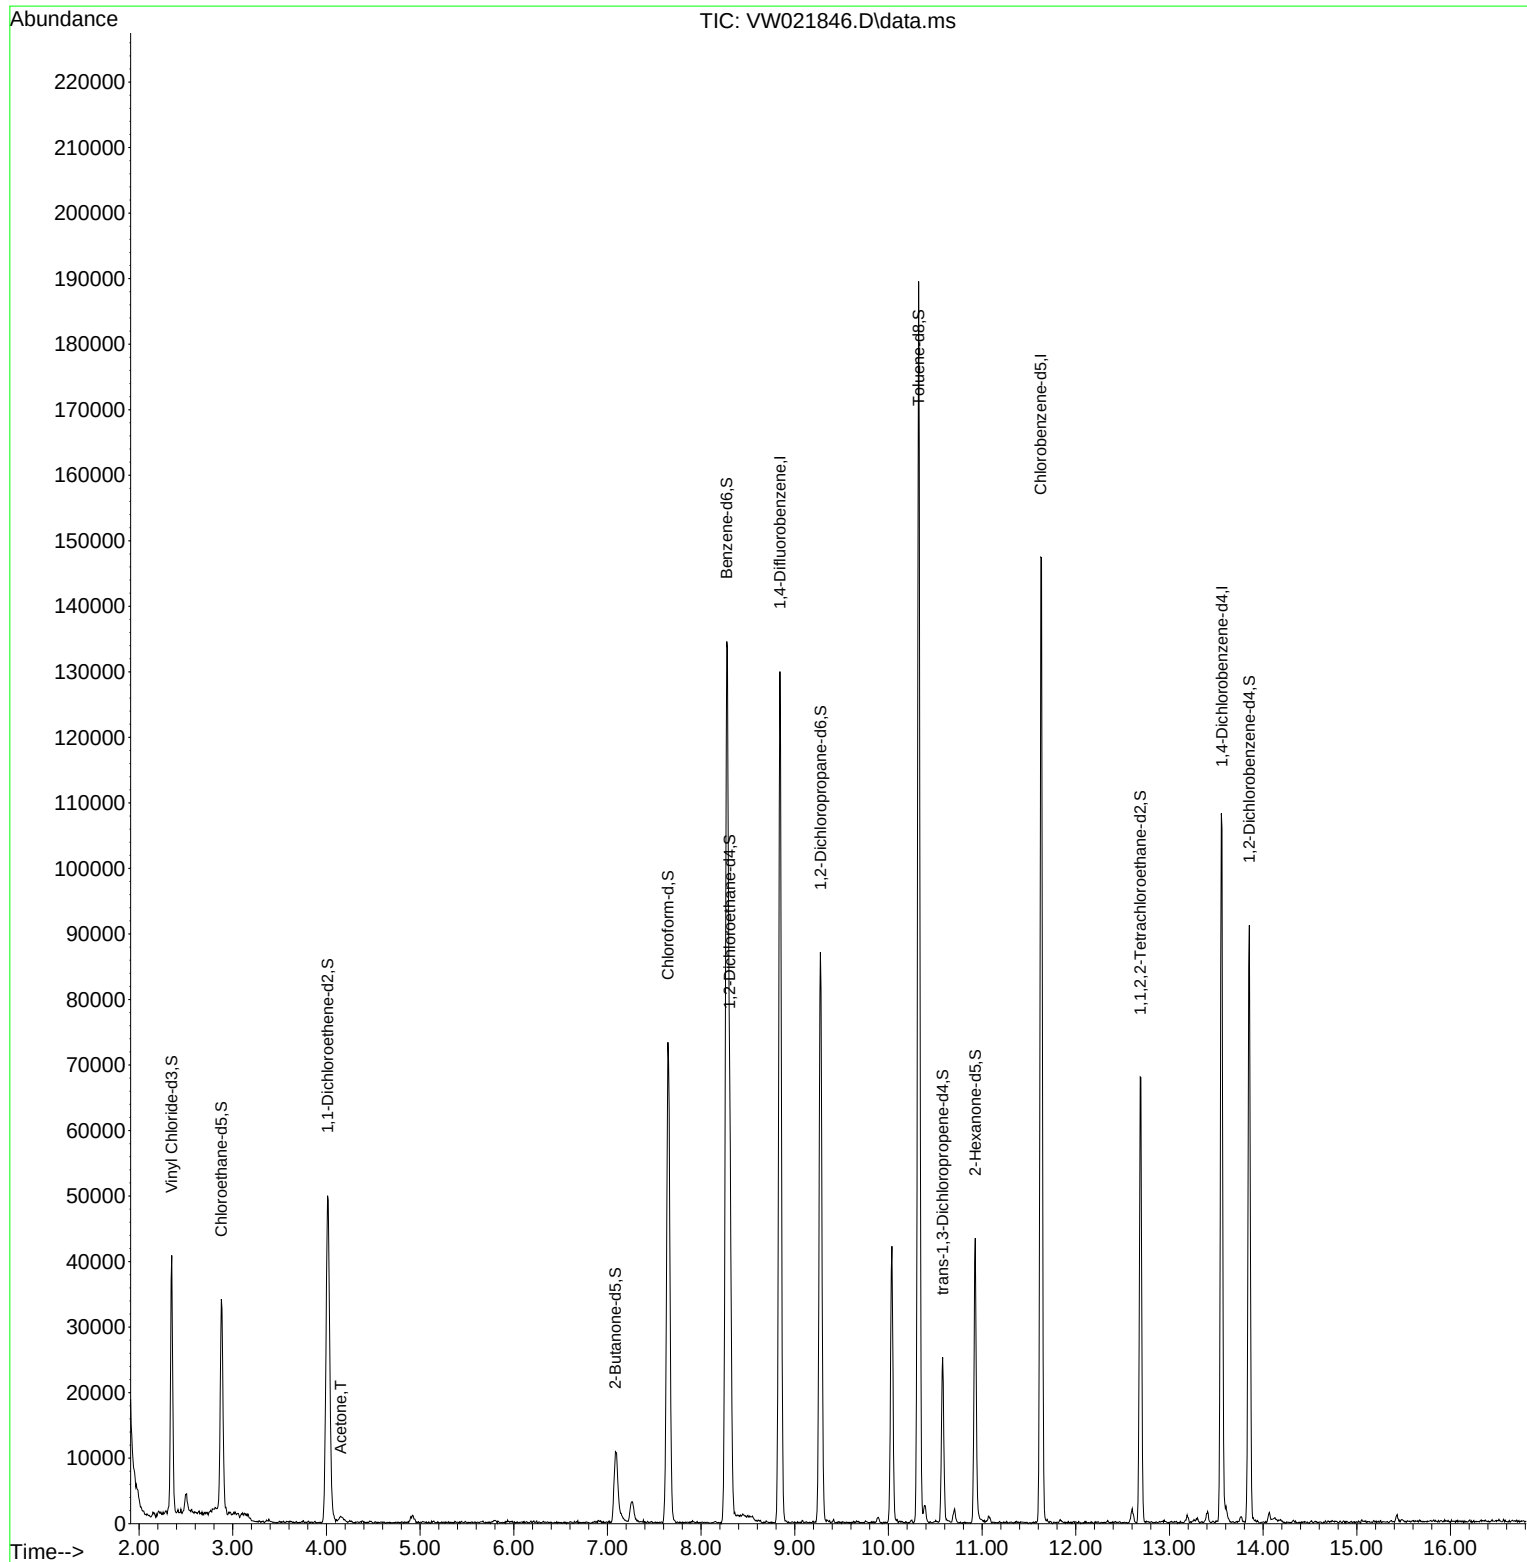

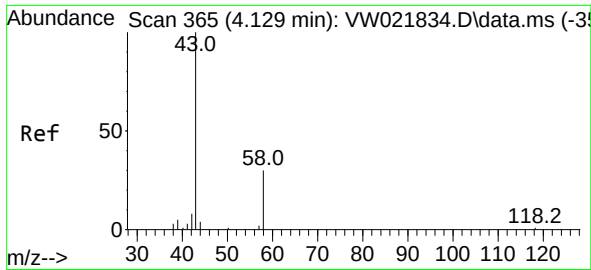

#13

Acetone

Concen: 6.767 ug/L

RT: 4.153 min Scan# 30

Delta R.T. 0.024 min

Lab File: VW021846.D

Acq: 11 Jan 2022 20:56

Instrument :

MSVOA_W

ClientSampleId :

BGLM9

Tgt Ion: 43 Resp: 1716

Ion Ratio Lower Upper

43 100

58 18.6 0.0 52.8

