




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011222\
Data File : VW021857.D
Acq On : 12 Jan 2022 11:07
Operator : SY/VA
Sample : N1084-06
Misc : 6.41g/10mL/MSVOA_W/SoIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLM9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/13/2022
Supervised By :Mahesh Dadoda 01/13/2022

Quant Time: Jan 12 23:49:59 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM01122SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jan 12 23:48:31 2022
Response via : Initial Calibration

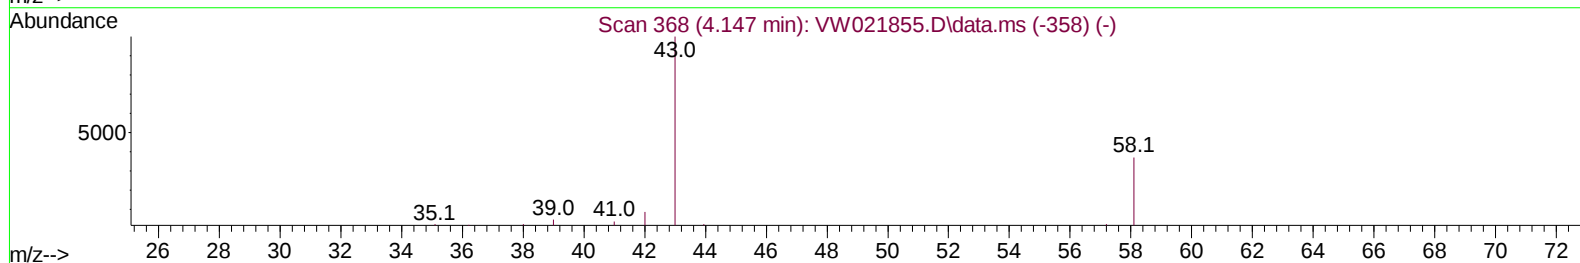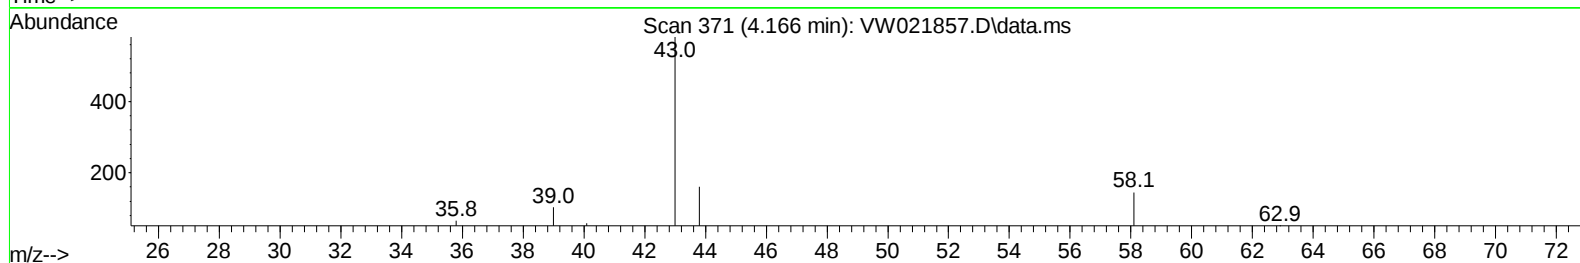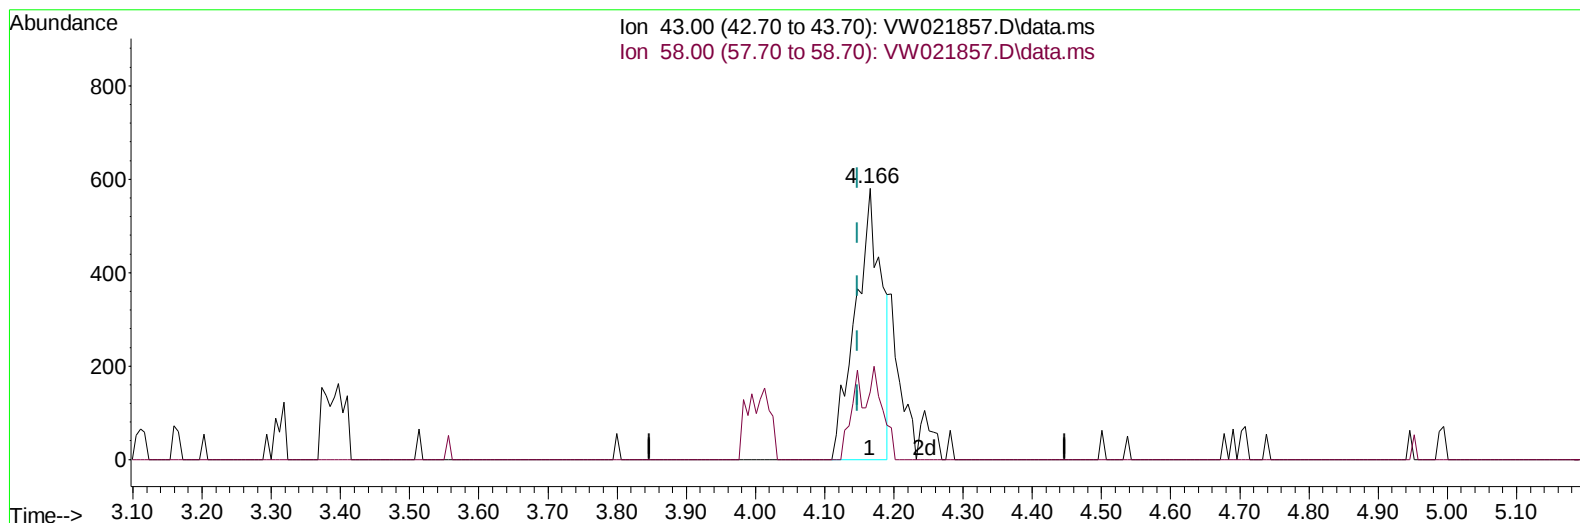

TIC: VW021857.D\data.ms

(13) Acetone (T)

4.166min (+ 0.018) 3.24 ug/L

response 1524

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.40	17.45
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011222\
 Data File : VW021857.D
 Acq On : 12 Jan 2022 11:07
 Operator : SY/VA
 Sample : N1084-06
 Misc : 6.41g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLM9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/13/2022
 Supervised By :Mahesh Dadoda 01/13/2022

Quant Time: Jan 12 23:49:59 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM01122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jan 12 23:48:31 2022
 Response via : Initial Calibration

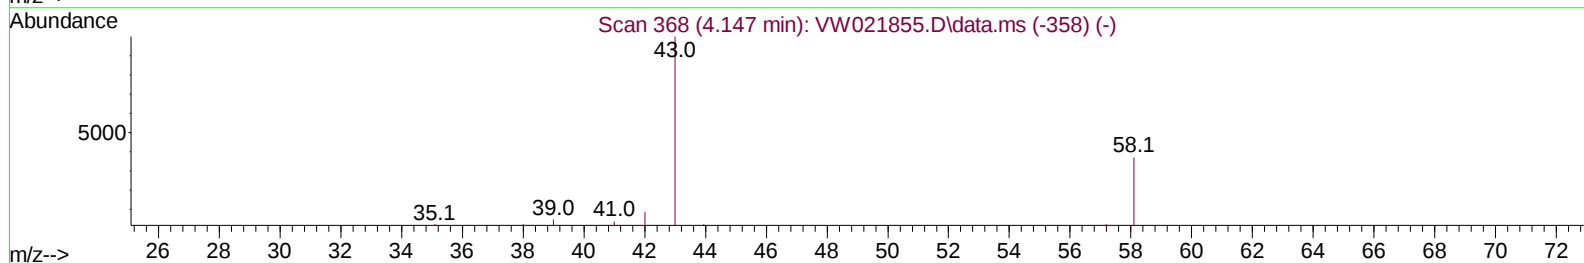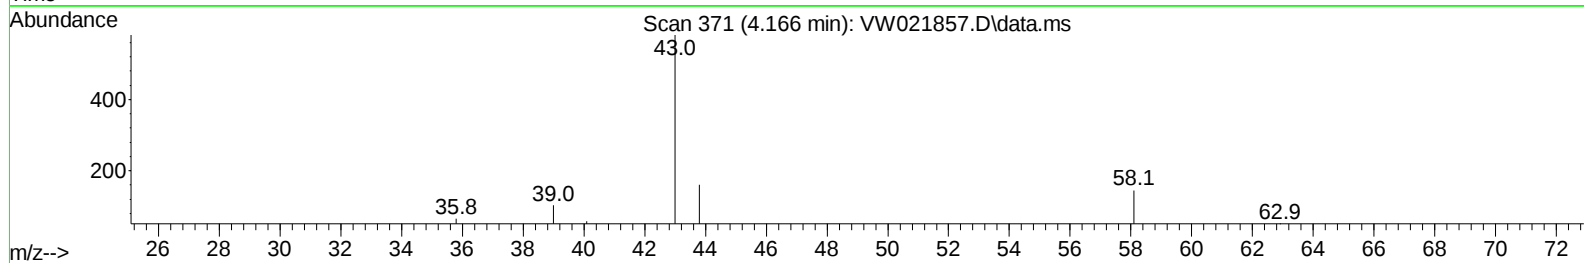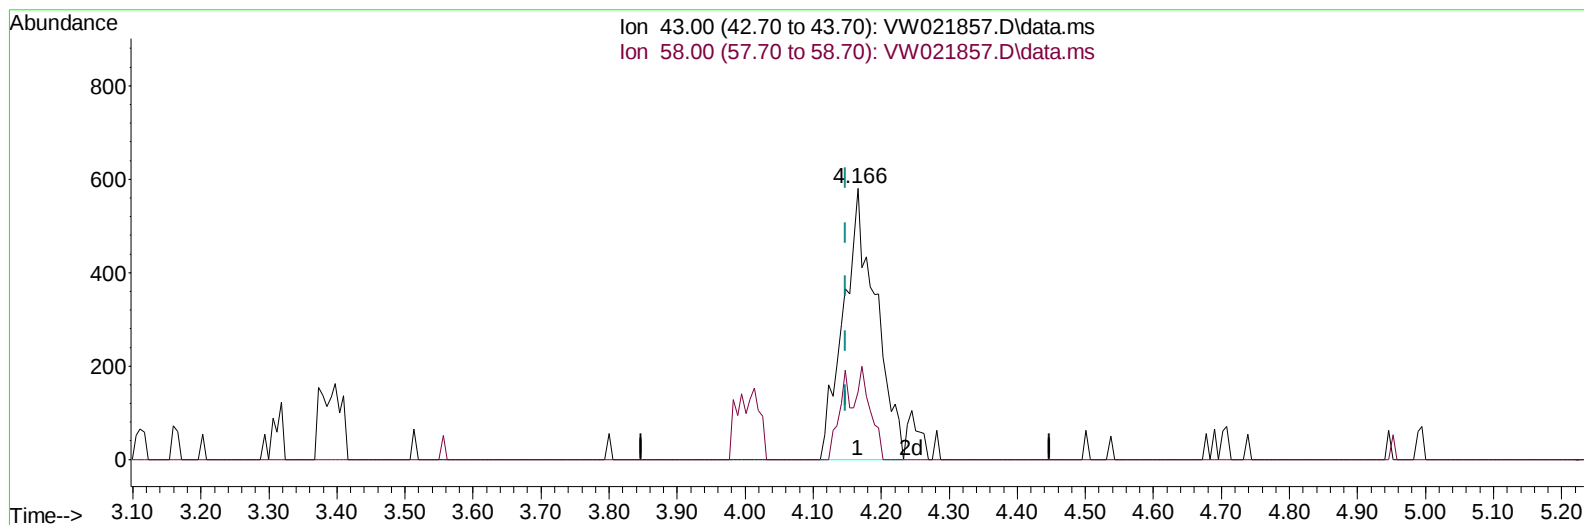

TIC: VW021857.D\data.ms

(13) Acetone (T)

4.166min (+ 0.018) 4.05 ug/L m

response 1907

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.40	13.95
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011222\
 Data File : VW021857.D
 Acq On : 12 Jan 2022 11:07
 Operator : SY/VA
 Sample : N1084-06
 Misc : 6.41g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLM9

Manual IntegrationsAPPROVED

Quant Time: Jan 12 23:49:59 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM01122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jan 12 23:48:31 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/13/2022
 Supervised By :Mahesh Dadoda 01/13/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.848	114		217172	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117		181947	25.000	ug/L	# 0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		69624	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.355	65		44296	10.974	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	43.880%	
7) Chloroethane-d5	2.891	69		36027	9.884	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	39.520%	
11) 1,1-Dichloroethene-d2	4.019	63		67342	10.567	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	42.280%#	
21) 2-Butanone-d5	7.092	46		20622	36.196	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	72.400%	
24) Chloroform-d	7.653	84		103812	14.797	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	59.200%	
26) 1,2-Dichloroethane-d4	8.305	65		51667	15.250	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	61.000%#	
32) Benzene-d6	8.275	84		211683	17.930	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	71.720%	
36) 1,2-Dichloropropane-d6	9.274	67		56534	18.168	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	72.680%	
41) Toluene-d8	10.323	98		200768	16.869	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	67.480%	
43) trans-1,3-Dichloroprop...	10.579	79		20485	15.505	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	62.040%	
47) 2-Hexanone-d5	10.927	63		16007	37.910	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	75.820%	
56) 1,1,2,2-Tetrachloroeth...	12.695	84		36356	14.941	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	59.760%	
66) 1,2-Dichlorobenzene-d4	13.853	152		45934	16.045	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	64.160%#	
Target Compounds							
13) Acetone	4.166	43		1907m	4.051	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011222\
Data File : VW021857.D
Acq On : 12 Jan 2022 11:07
Operator : SY/VA
Sample : N1084-06
Misc : 6.41g/10mL/MSVOA_W/soil
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLM9

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/13/2022
Supervised By :Mahesh Dadoda 01/13/2022

Quant Time: Jan 12 23:49:59 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM01122SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jan 12 23:48:31 2022
Response via : Initial Calibration

