




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011222\
Data File : VW021868.D
Acq On : 12 Jan 2022 16:05
Operator : SY/VA
Sample : N1114-08
Misc : 6.27g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLQ0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/13/2022
Supervised By :Mahesh Dadoda 01/13/2022

Quant Time: Jan 12 23:51:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM01122SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jan 12 23:48:31 2022
Response via : Initial Calibration

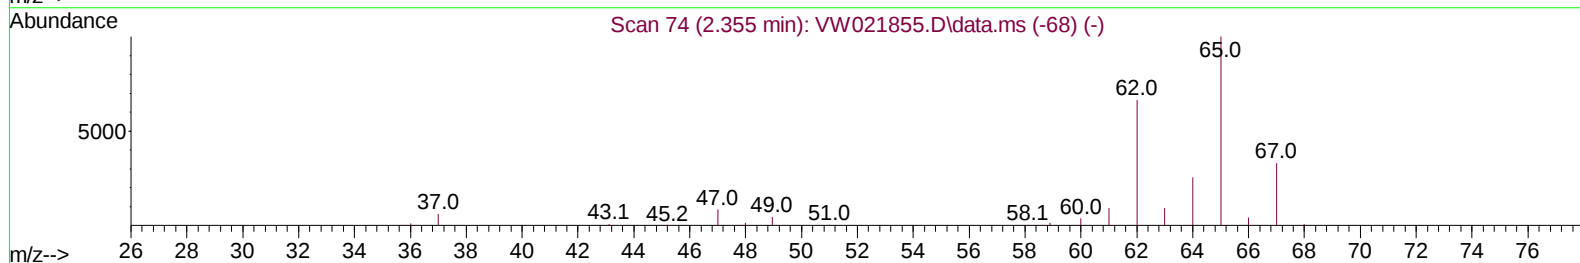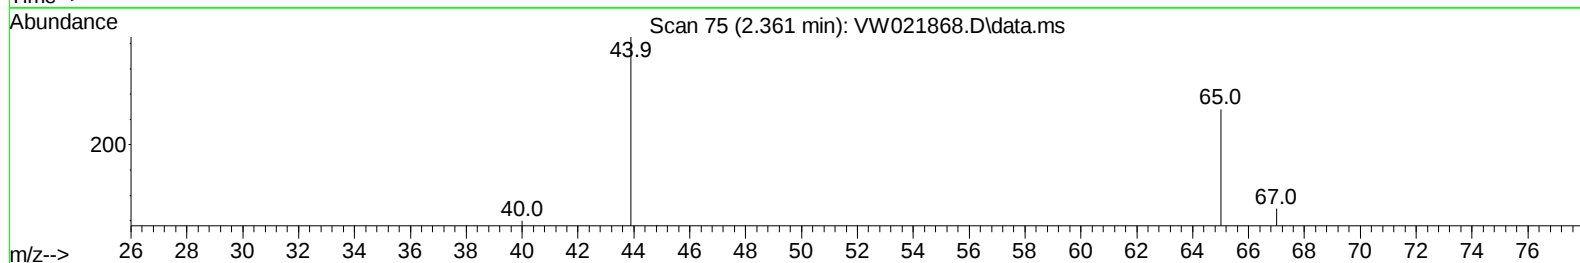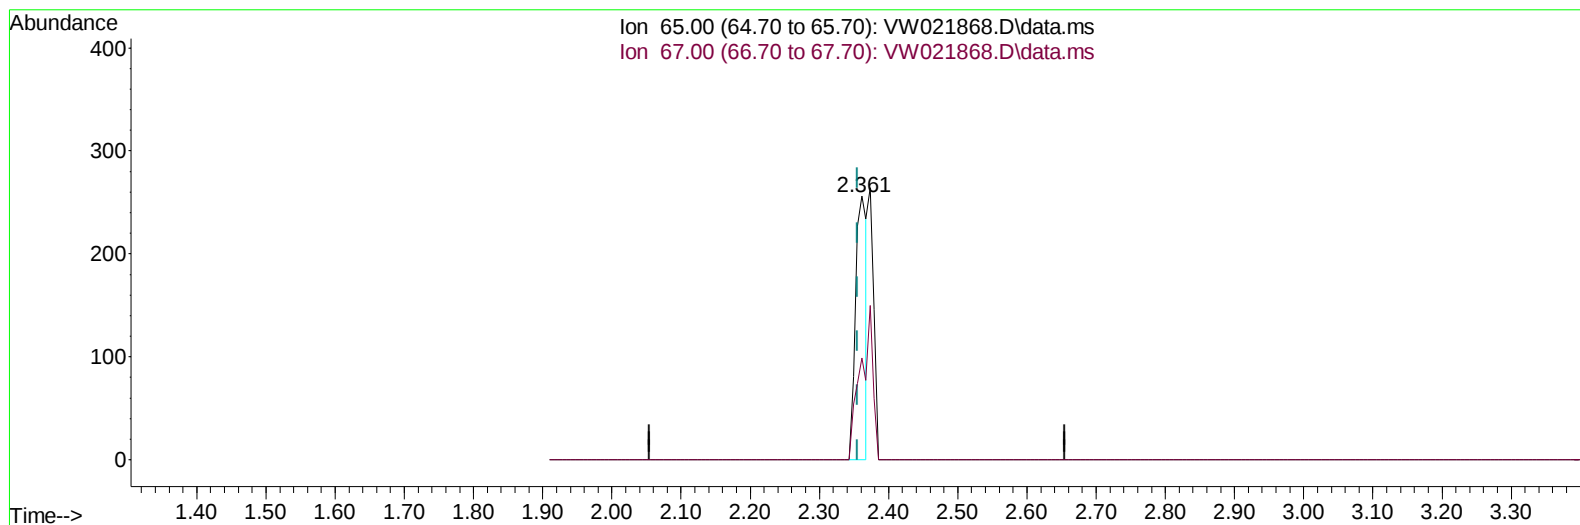

TIC: VW021868.D\data.ms

(4) Vinyl Chloride-d3 (S)

2.361min (+ 0.006) 10.91 ug/L

response 292

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.70	38.01
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011222\
 Data File : VW021868.D
 Acq On : 12 Jan 2022 16:05
 Operator : SY/VA
 Sample : N1114-08
 Misc : 6.27g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLQ0

Manual IntegrationsAPPROVED

Quant Time: Jan 12 23:51:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM01122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jan 12 23:48:31 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/13/2022
 Supervised By :Mahesh Dadoda 01/13/2022

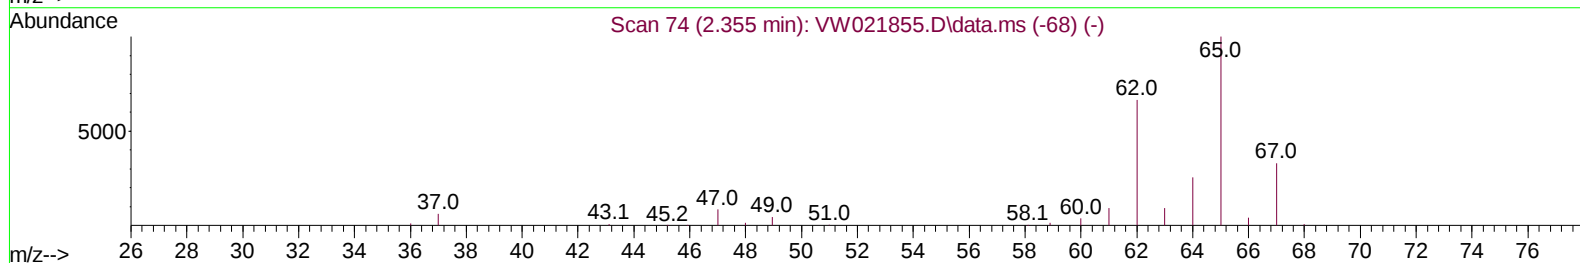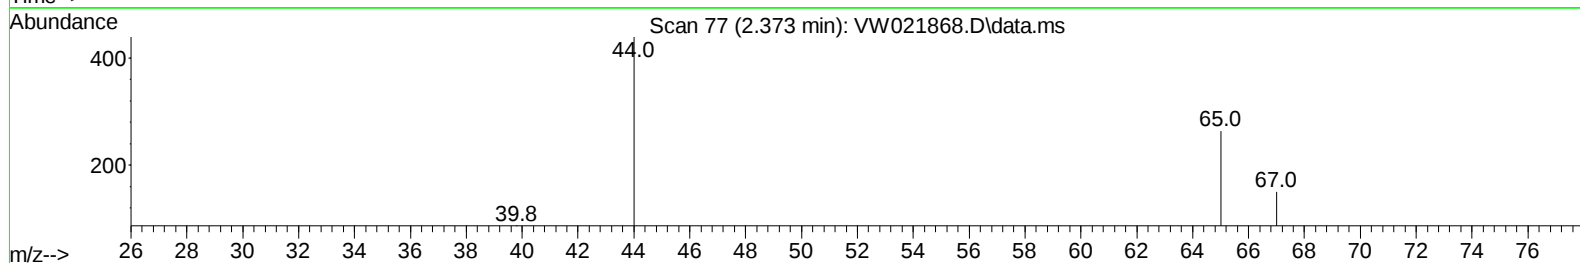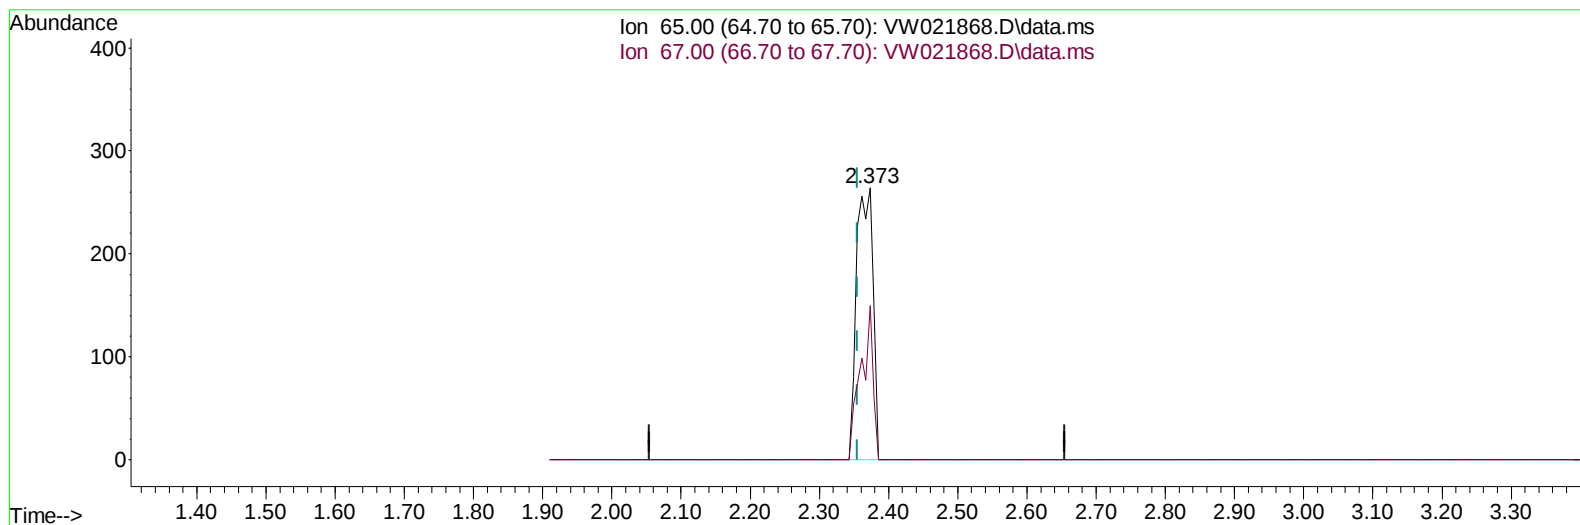

TIC: VW021868.D\data.ms

(4) Vinyl Chloride-d3 (S)

2.373min (+ 0.018) 16.51 ug/L m

response 442

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	31.70	25.11
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011222\
 Data File : VW021868.D
 Acq On : 12 Jan 2022 16:05
 Operator : SY/VA
 Sample : N1114-08
 Misc : 6.27g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLQ0

Manual IntegrationsAPPROVED

Quant Time: Jan 12 23:51:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM01122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jan 12 23:48:31 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/13/2022
 Supervised By :Mahesh Dadoda 01/13/2022

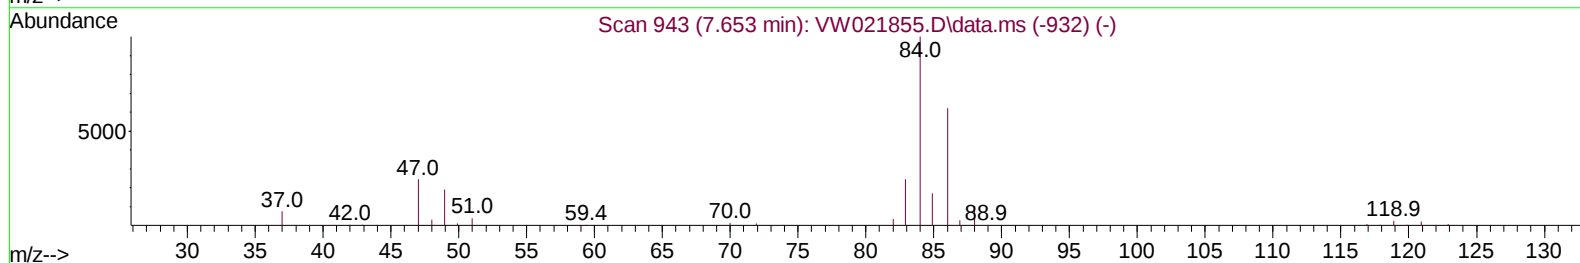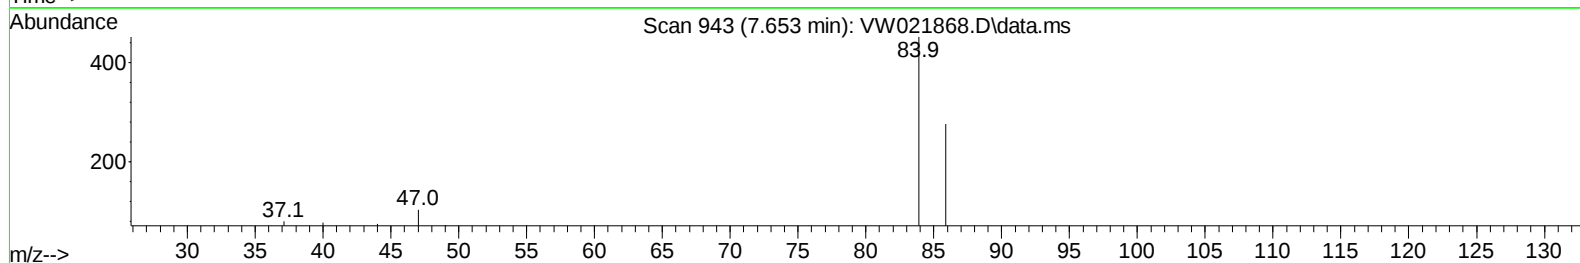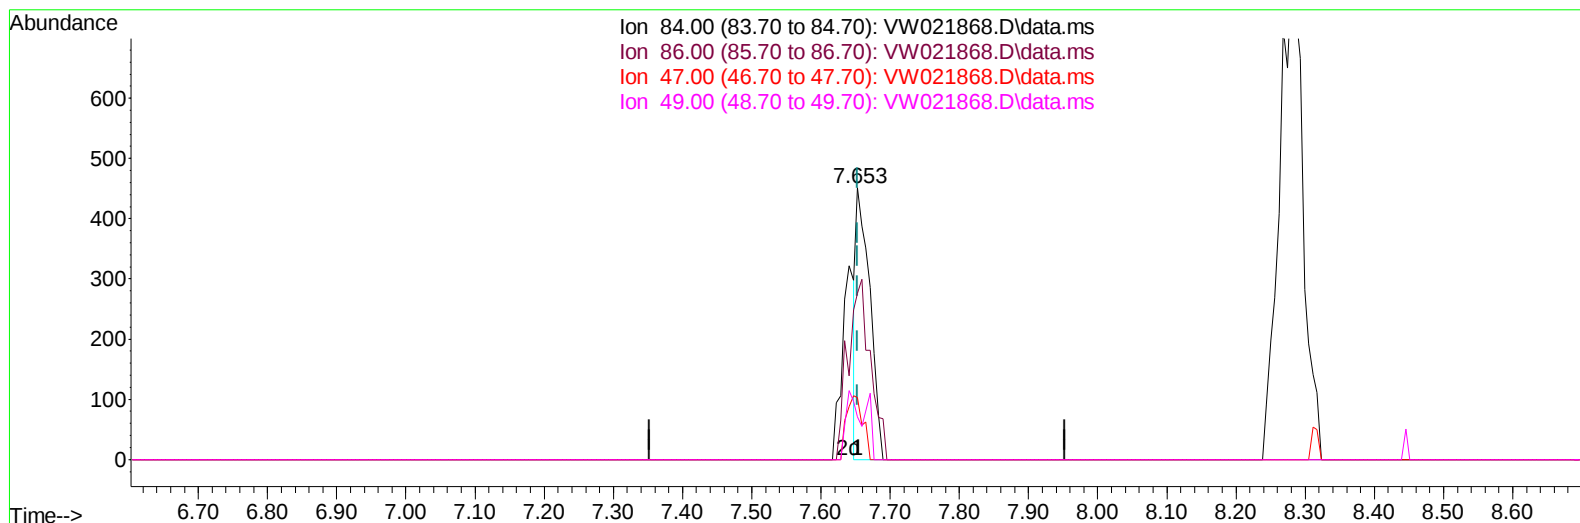

TIC: VW021868.D\data.ms

(24) Chloroform-d (S)

7.653min (+ 0.000) 13.56 ug/L

response 631

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.20	106.34#
47.00	52.60	27.89#
49.00	29.60	11.09#




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011222\
Data File : VW021868.D
Acq On : 12 Jan 2022 16:05
Operator : SY/VA
Sample : N1114-08
Misc : 6.27g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLQ0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/13/2022
Supervised By :Mahesh Dadoda 01/13/2022

Quant Time: Jan 12 23:51:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM01122SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jan 12 23:48:31 2022
Response via : Initial Calibration

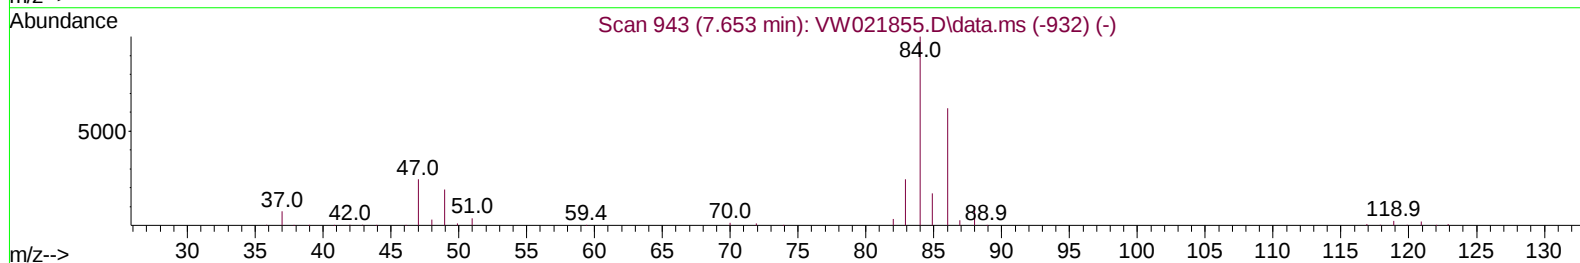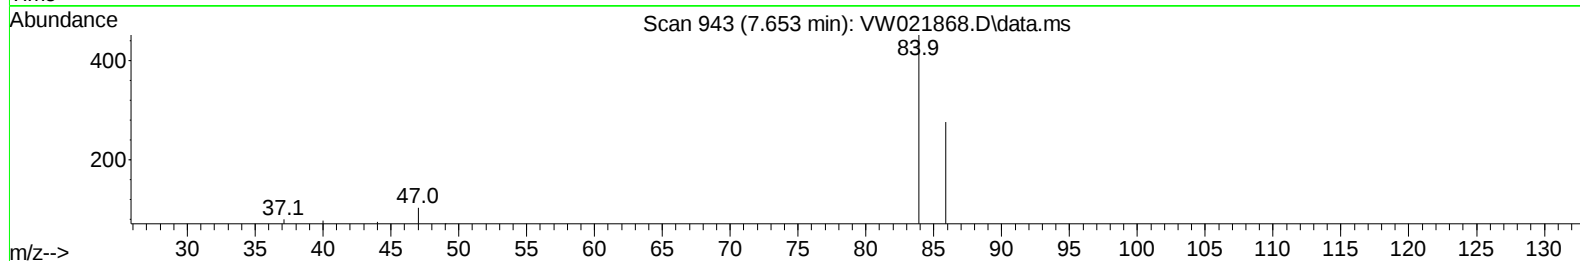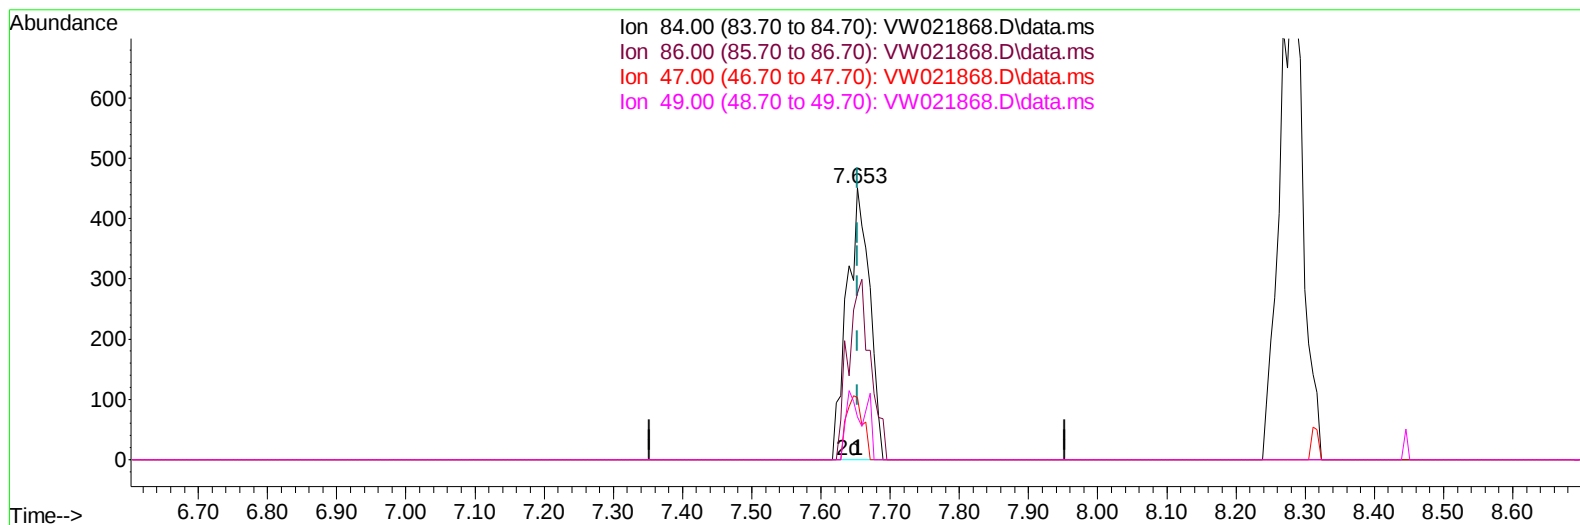

TIC: VW021868.D\data.ms

(24) Chloroform-d (S)

7.653min (+ 0.000) 22.10 ug/L m

response 1028

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.20	65.27
47.00	52.60	17.12#
49.00	29.60	6.81#




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011222\
 Data File : VW021868.D
 Acq On : 12 Jan 2022 16:05
 Operator : SY/VA
 Sample : N1114-08
 Misc : 6.27g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLQ0

Manual IntegrationsAPPROVED

Quant Time: Jan 12 23:51:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM01122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jan 12 23:48:31 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/13/2022
 Supervised By :Mahesh Dadoda 01/13/2022

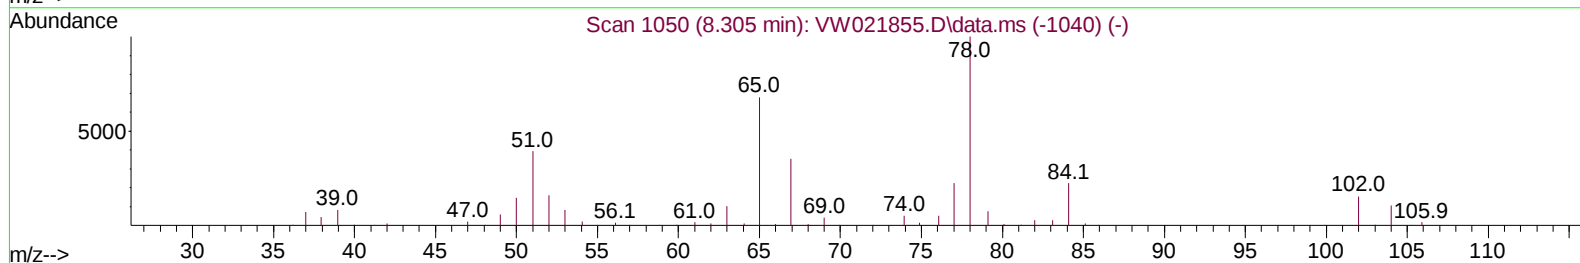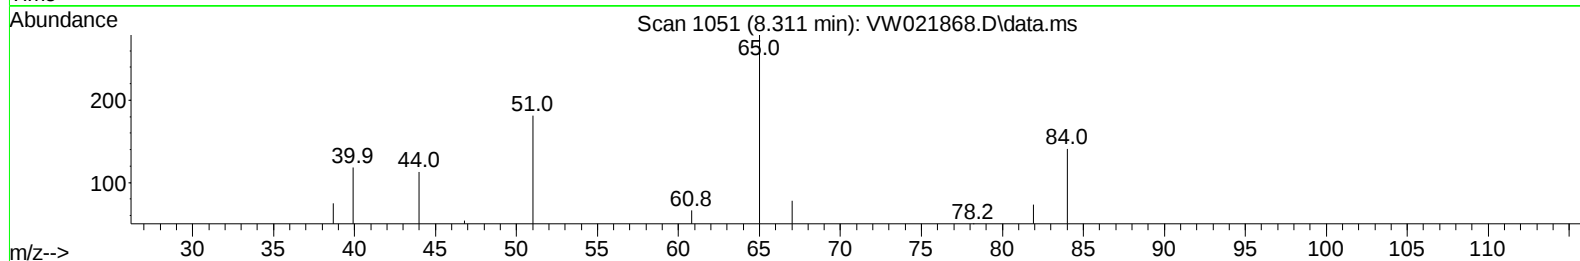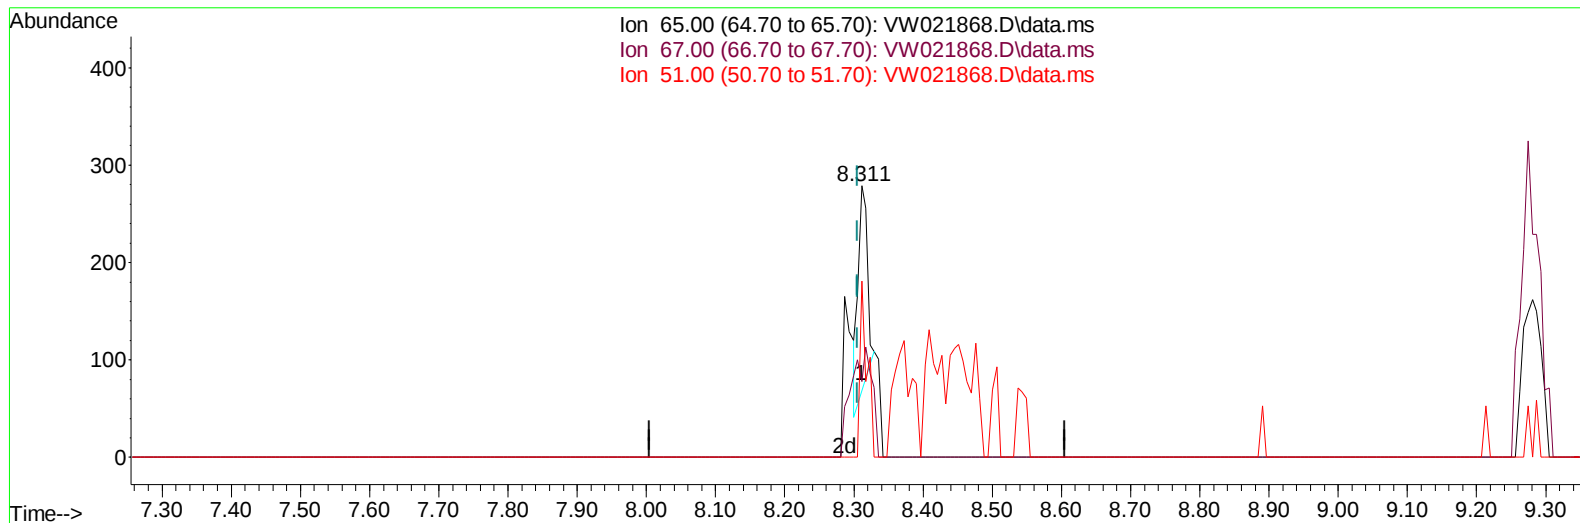

TIC: VW021868.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.311min (+ 0.006) 8.95 ug/L

response 201

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.10	49.25
51.00	111.40	65.67#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011222\
 Data File : VW021868.D
 Acq On : 12 Jan 2022 16:05
 Operator : SY/VA
 Sample : N1114-08
 Misc : 6.27g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLQ0

Manual IntegrationsAPPROVED

Quant Time: Jan 12 23:51:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM01122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jan 12 23:48:31 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/13/2022
 Supervised By :Mahesh Dadoda 01/13/2022

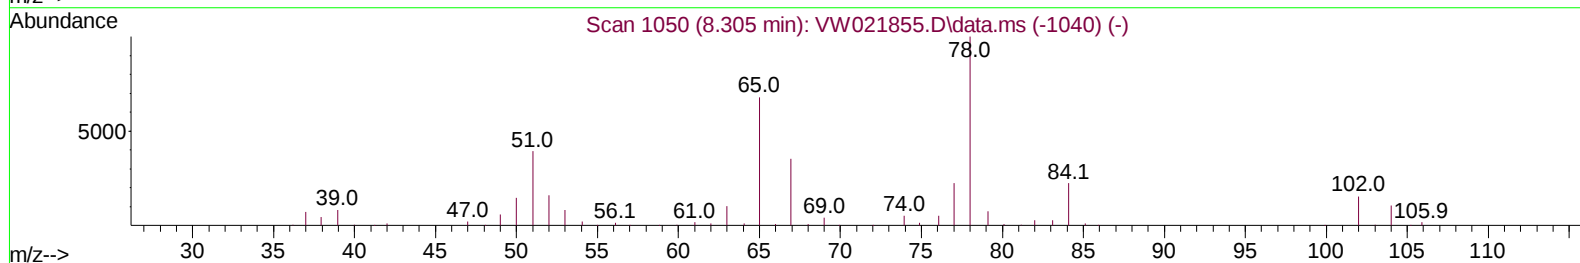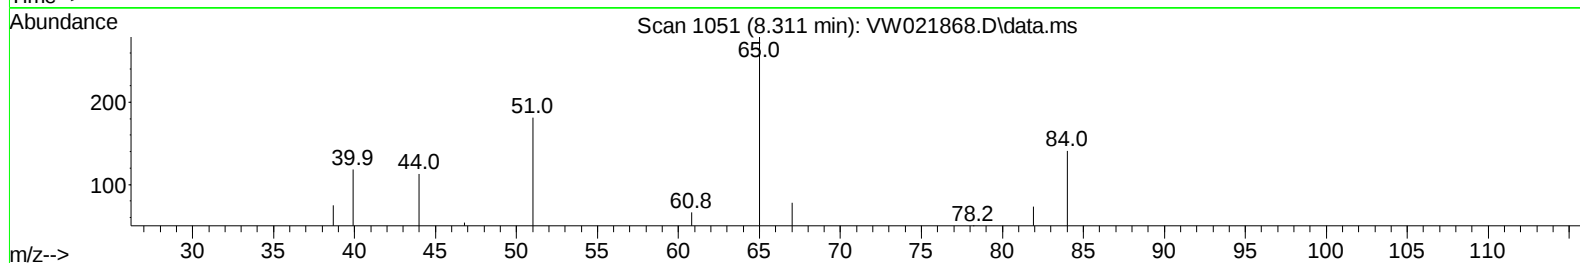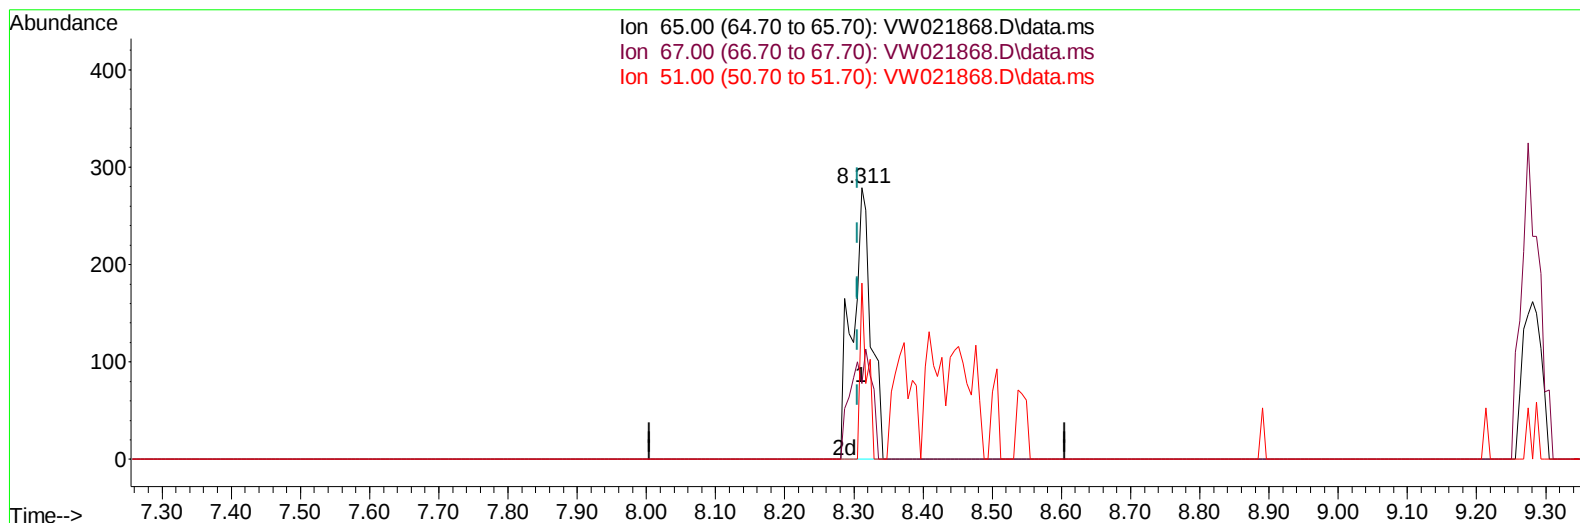

TIC: VW021868.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.311min (+ 0.006) 23.46 ug/L m

response 527

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.10	18.79#
51.00	111.40	25.05#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011222\
Data File : VW021868.D
Acq On : 12 Jan 2022 16:05
Operator : SY/VA
Sample : N1114-08
Misc : 6.27g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLQ0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/13/2022
Supervised By :Mahesh Dadoda 01/13/2022

Quant Time: Jan 12 23:51:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM01122SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jan 12 23:48:31 2022
Response via : Initial Calibration

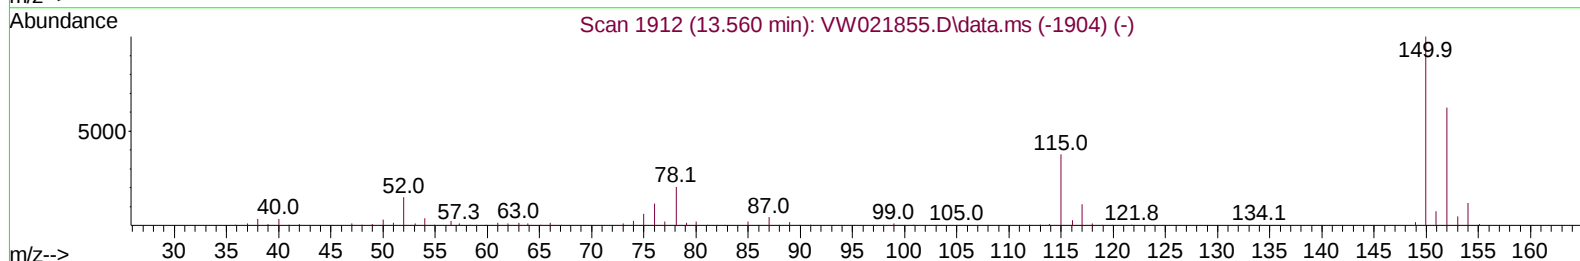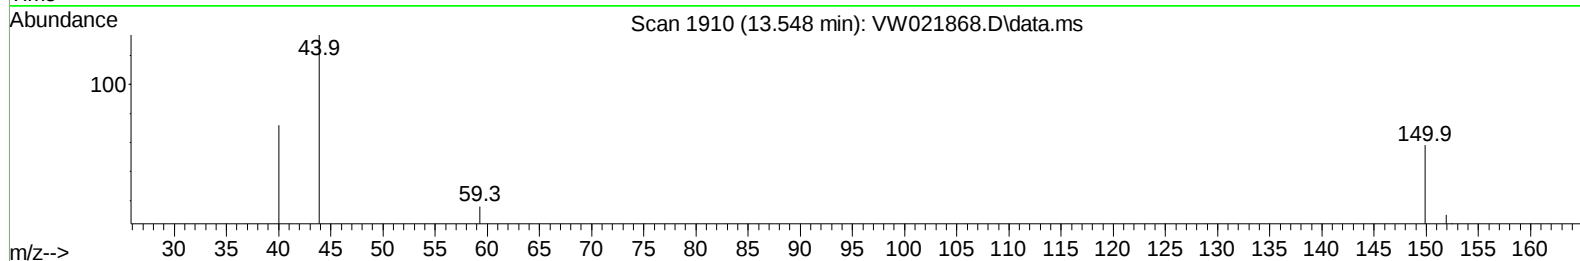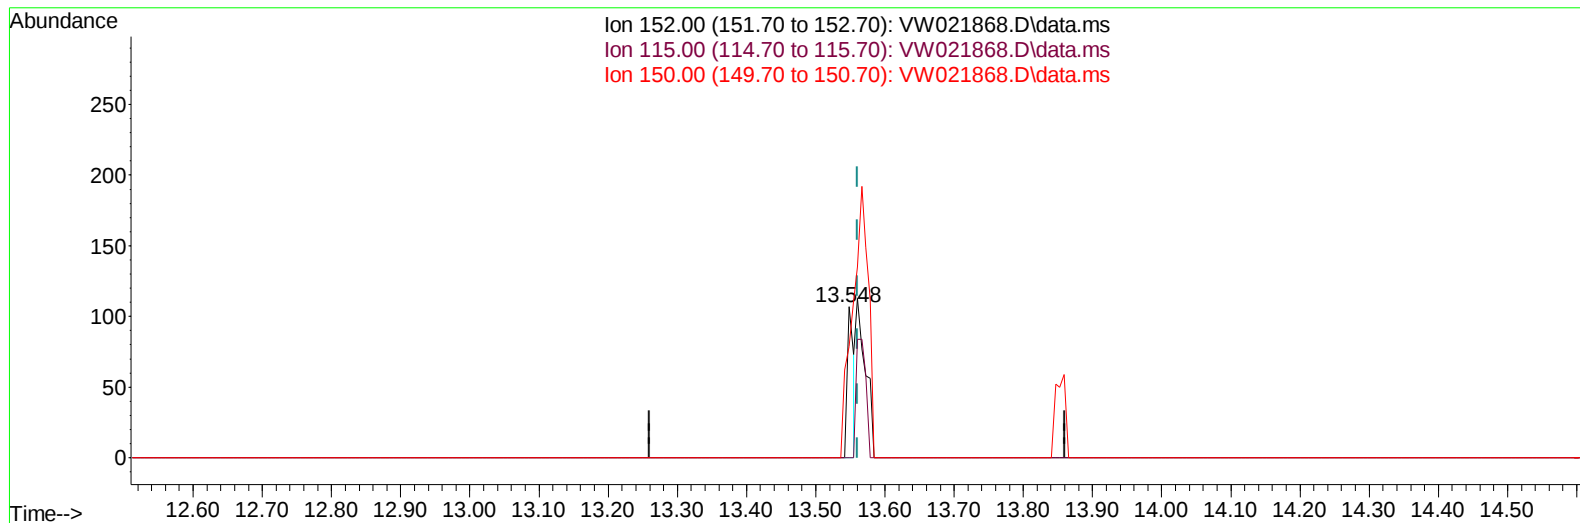

TIC: VW021868.D\data.ms

(58) 1,4-Dichlorobenzene-d4 (I)

13.548min (-0.012) 25.00 ug/L

response 66

Ion	Exp%	Act%
152.00	100.00	100.00
115.00	63.00	125.76
150.00	172.50	465.15#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011222\
 Data File : VW021868.D
 Acq On : 12 Jan 2022 16:05
 Operator : SY/VA
 Sample : N1114-08
 Misc : 6.27g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLQ0

Manual IntegrationsAPPROVED

Quant Time: Jan 12 23:51:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM01122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jan 12 23:48:31 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/13/2022
 Supervised By :Mahesh Dadoda 01/13/2022

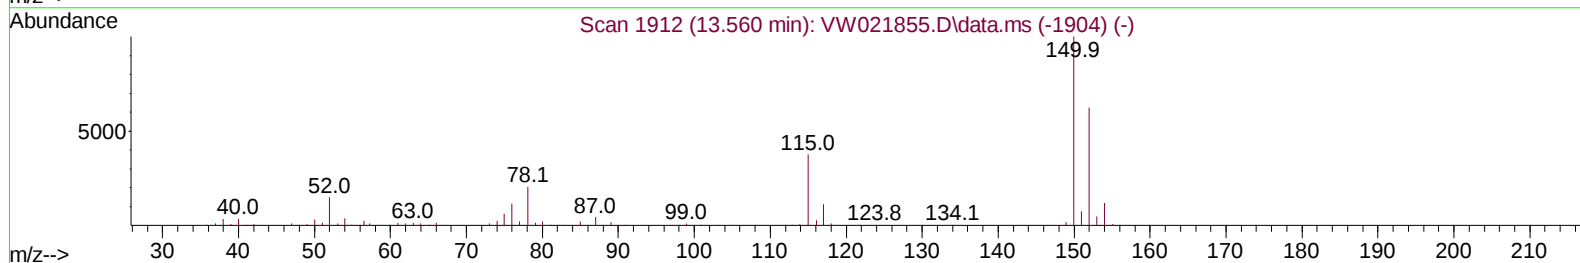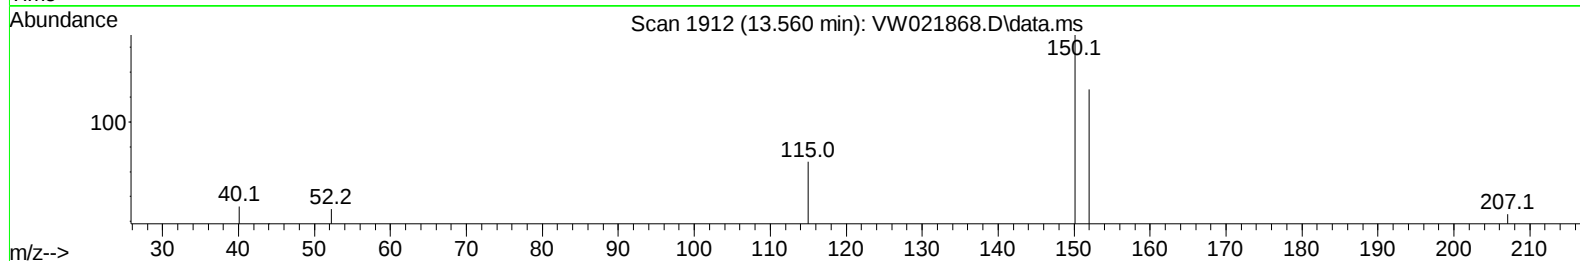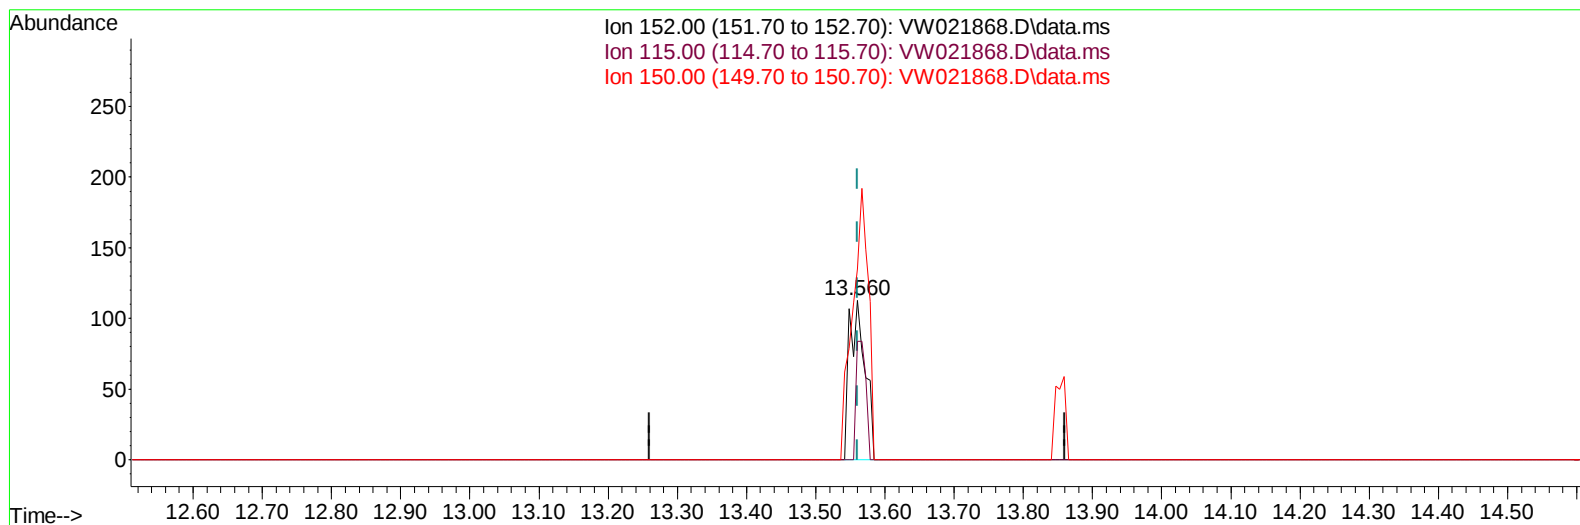

TIC: VW021868.D\data.ms

(58) 1,4-Dichlorobenzene-d4 (I)

13.560min (+ 0.000) 25.00 ug/L m

response 177

Ion	Exp%	Act%
152.00	100.00	100.00
115.00	63.00	46.89
150.00	172.50	173.45
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011222\
Data File : VW021868.D
Acq On : 12 Jan 2022 16:05
Operator : SY/VA
Sample : N1114-08
Misc : 6.27g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLQ0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/13/2022
Supervised By :Mahesh Dadoda 01/13/2022

Quant Time: Jan 12 23:51:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM01122SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jan 12 23:48:31 2022
Response via : Initial Calibration

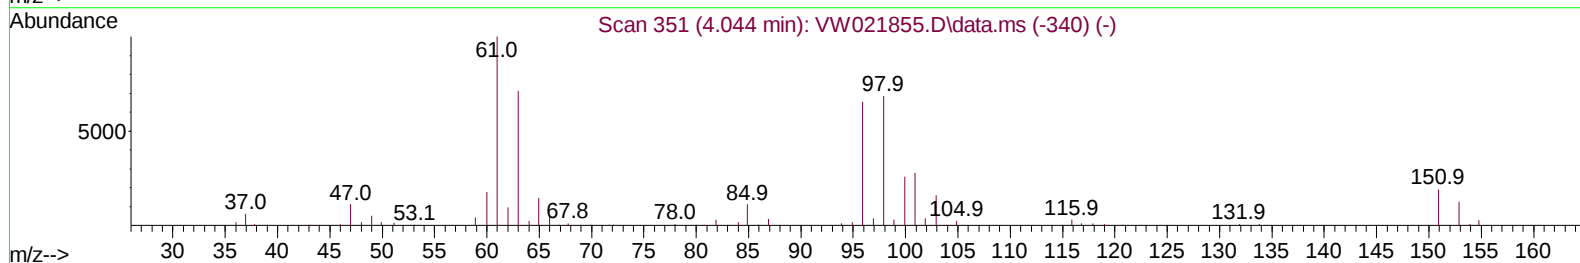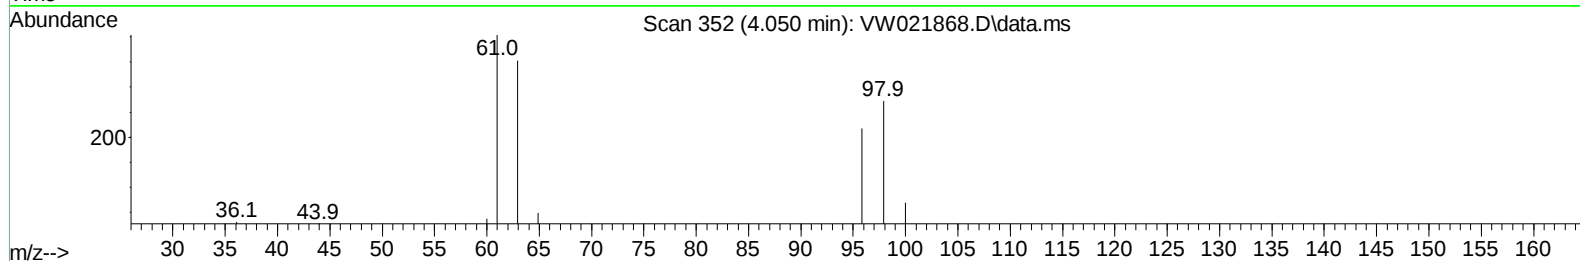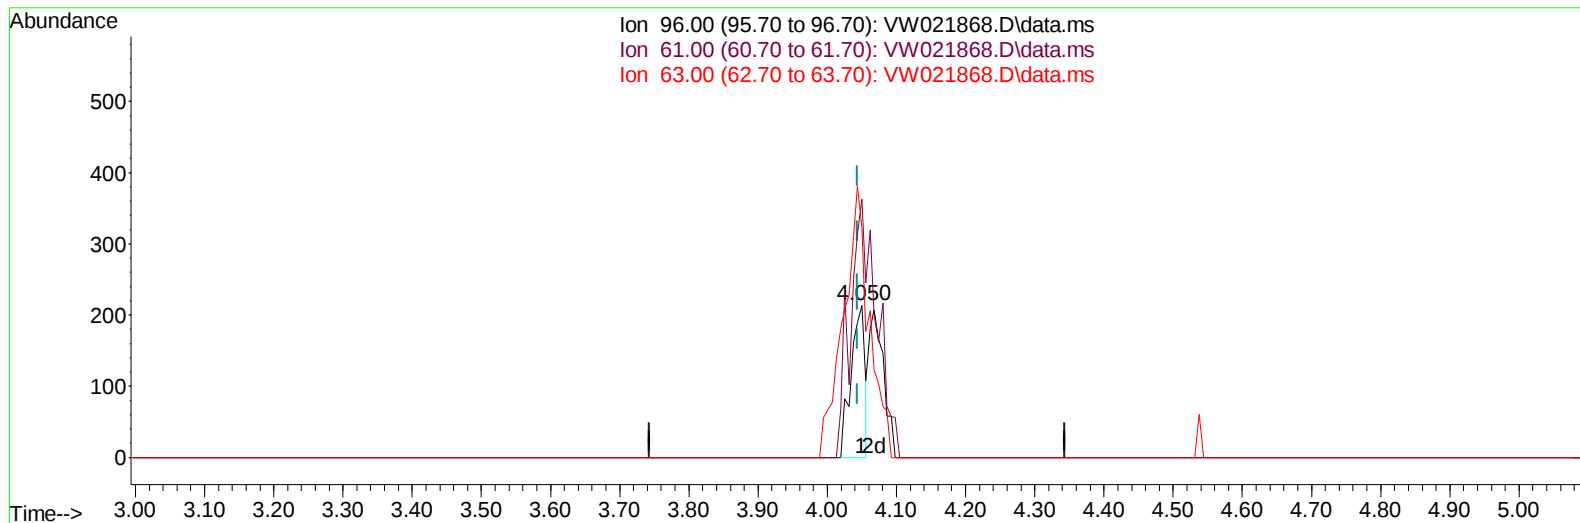

TIC: VW021868.D\data.ms

(12) 1,1-Dichloroethene (T)

4.050min (+ 0.006) 14.10 ug/L

response 303

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	197.60	169.63
63.00	118.00	150.47
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011222\
Data File : VW021868.D
Acq On : 12 Jan 2022 16:05
Operator : SY/VA
Sample : N1114-08
Misc : 6.27g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLQ0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/13/2022
Supervised By :Mahesh Dadoda 01/13/2022

Quant Time: Jan 12 23:51:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM01122SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jan 12 23:48:31 2022
Response via : Initial Calibration

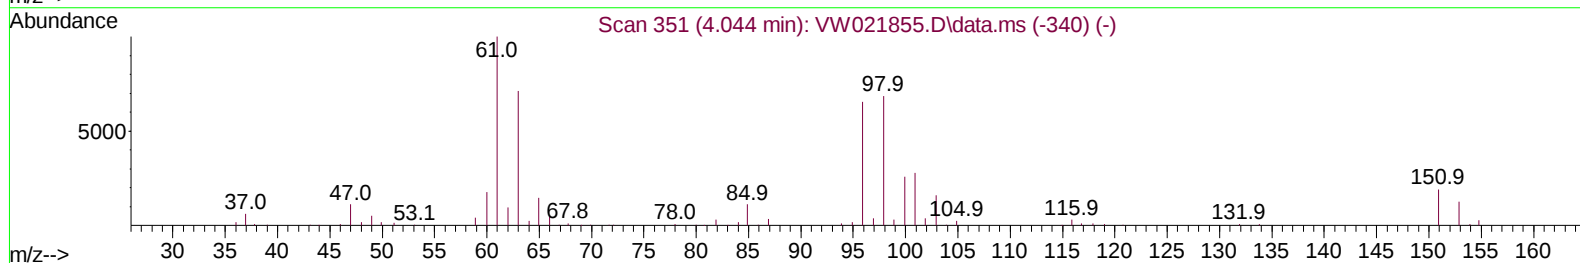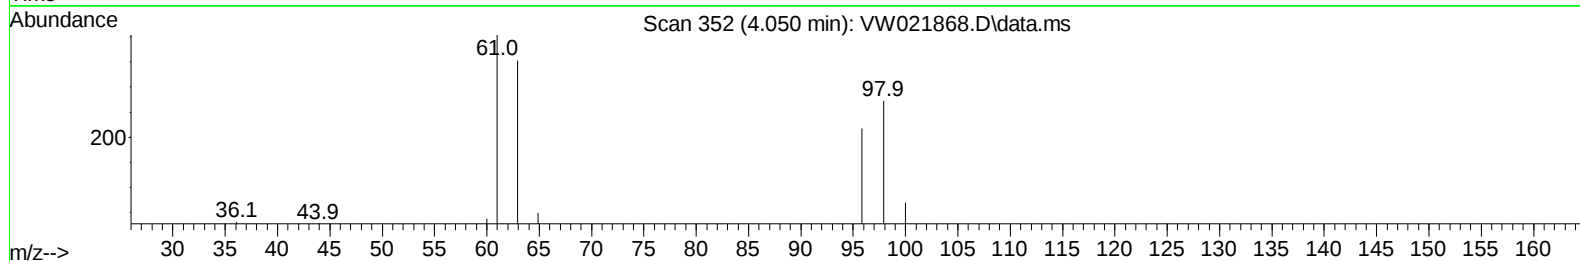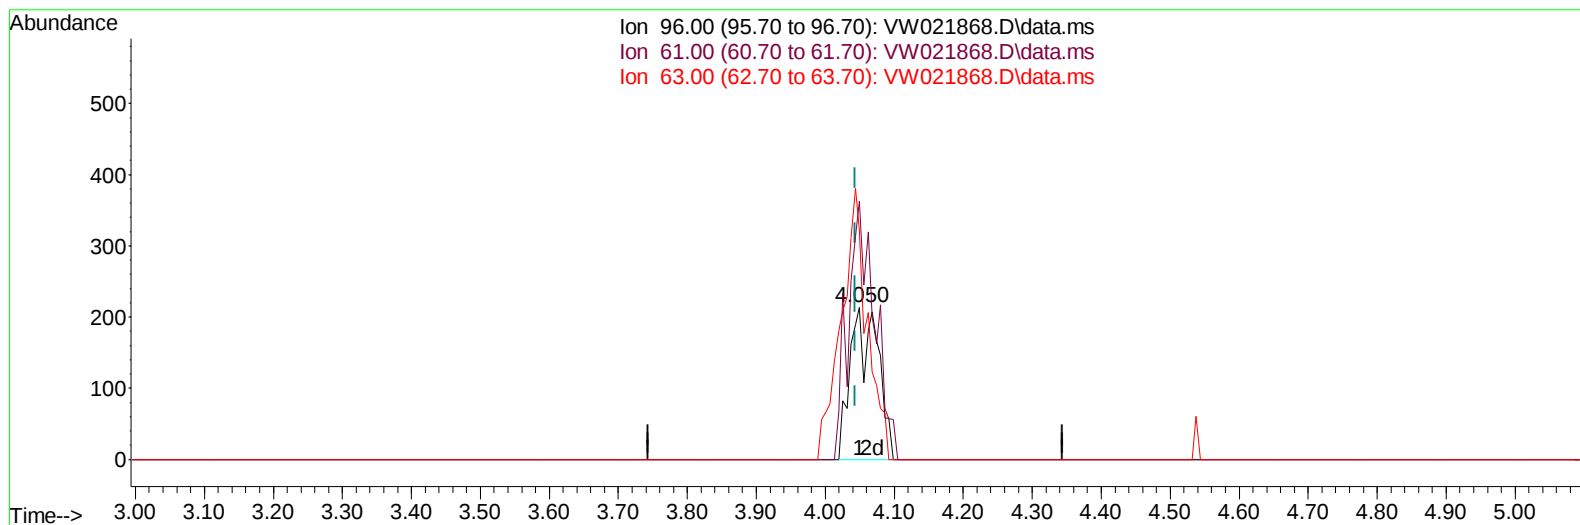

TIC: VW021868.D\data.ms

(12) 1,1-Dichloroethene (T)

4.050min (+ 0.006) 27.96 ug/L m

response 601

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	197.60	169.63
63.00	118.00	150.47
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011222\
Data File : VW021868.D
Acq On : 12 Jan 2022 16:05
Operator : SY/VA
Sample : N1114-08
Misc : 6.27g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLQ0

Manual IntegrationsAPPROVED

Quant Time: Jan 12 23:51:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM01122SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jan 12 23:48:31 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/13/2022
Supervised By :Mahesh Dadoda 01/13/2022

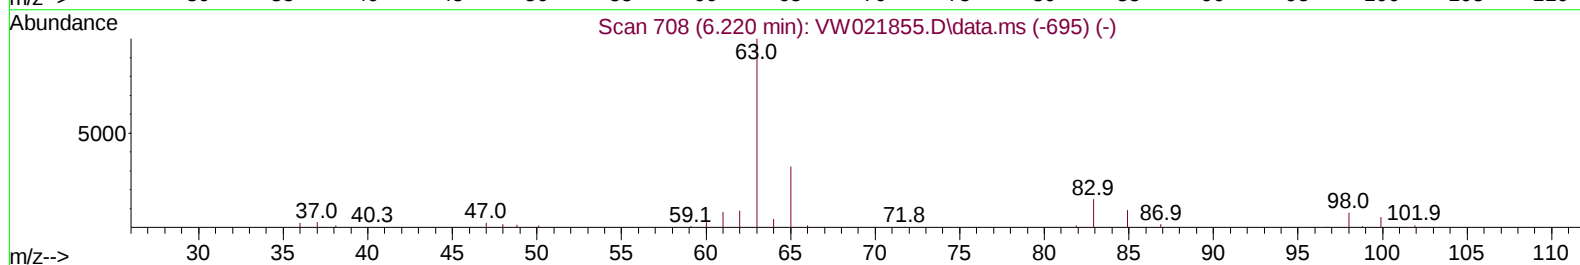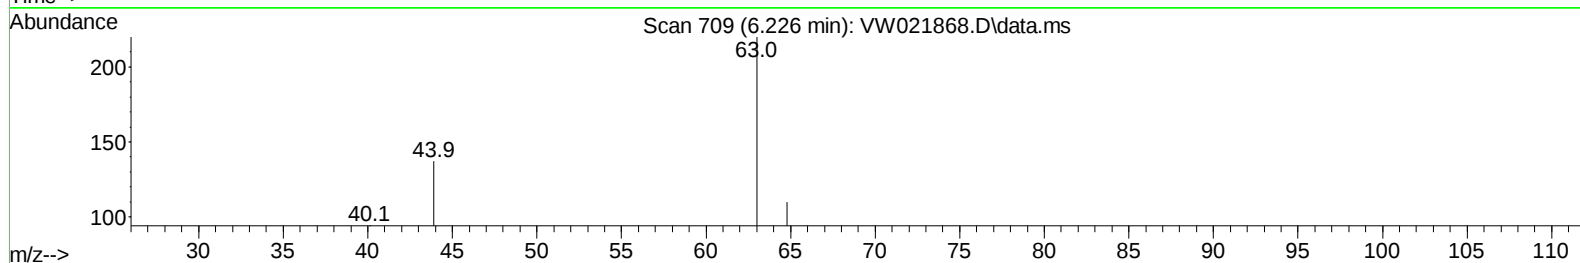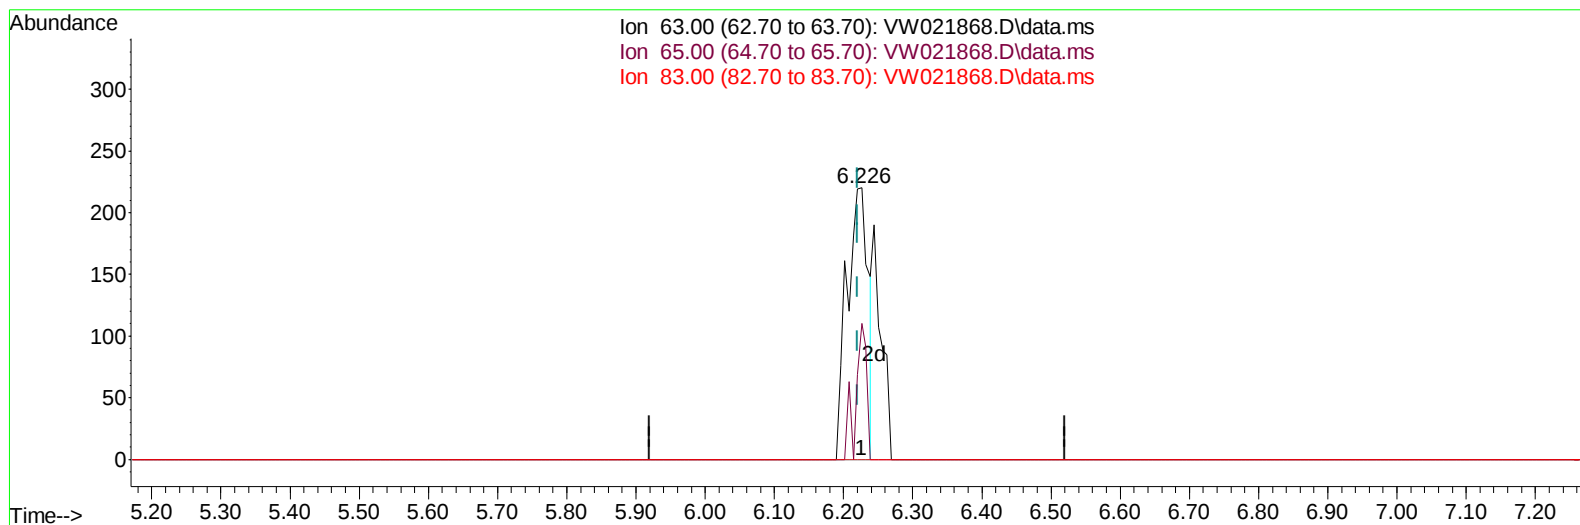

TIC: VW021868.D\data.ms

(19) 1,1-Dichloroethane (T)

6.226min (+ 0.006) 13.80 ug/L

response 470

Ion	Exp%	Act%
63.00	100.00	100.00
65.00	31.60	50.00#
83.00	13.20	0.00#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011222\
Data File : VW021868.D
Acq On : 12 Jan 2022 16:05
Operator : SY/VA
Sample : N1114-08
Misc : 6.27g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLQ0

Manual IntegrationsAPPROVED

Quant Time: Jan 12 23:51:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM01122SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jan 12 23:48:31 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/13/2022
Supervised By :Mahesh Dadoda 01/13/2022

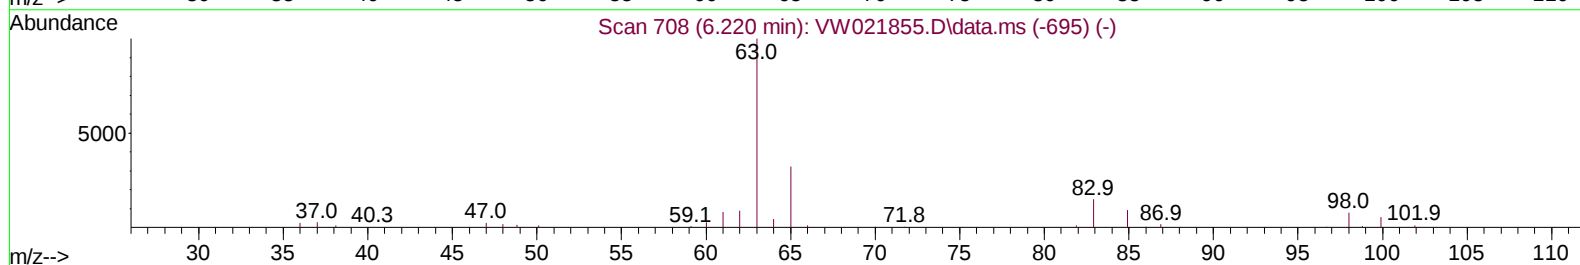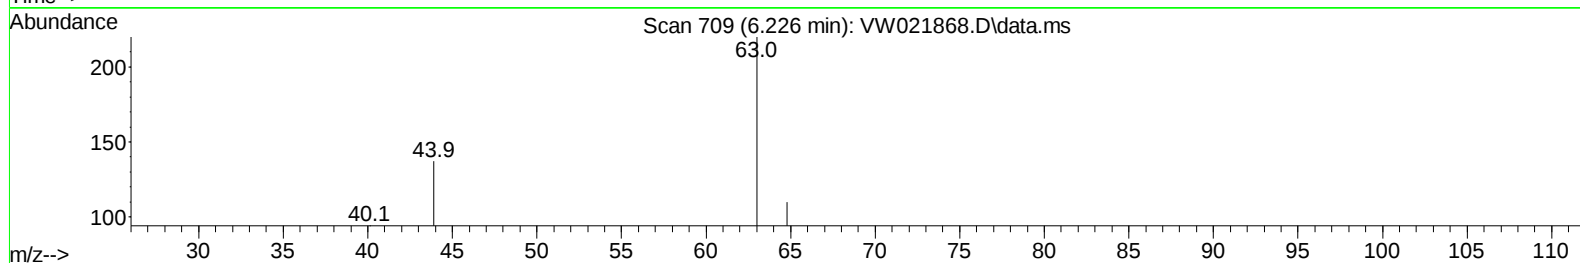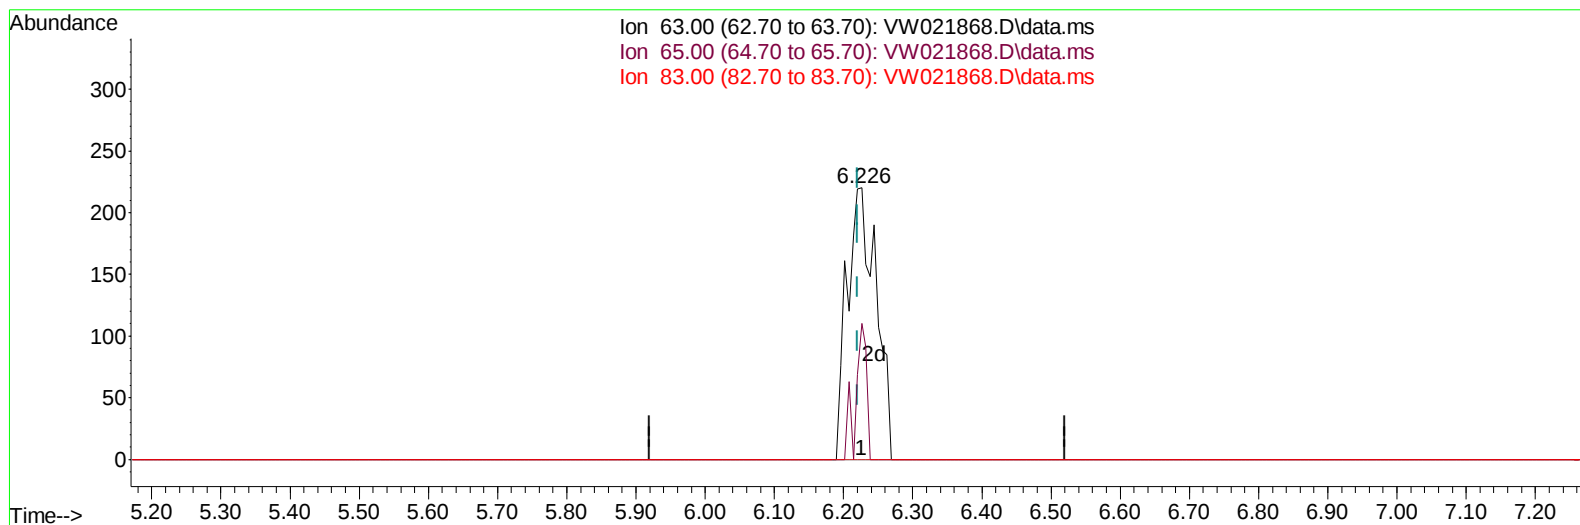

TIC: VW021868.D\data.ms

(19) 1,1-Dichloroethane (T)

6.226min (+ 0.006) 18.85 ug/L m

response 642

Ion	Exp%	Act%
63.00	100.00	100.00
65.00	31.60	50.00#
83.00	13.20	0.00#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011222\
 Data File : VW021868.D
 Acq On : 12 Jan 2022 16:05
 Operator : SY/VA
 Sample : N1114-08
 Misc : 6.27g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLQ0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/13/2022
 Supervised By :Mahesh Dadoda 01/13/2022

Quant Time: Jan 12 23:51:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM01122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jan 12 23:48:31 2022
 Response via : Initial Calibration

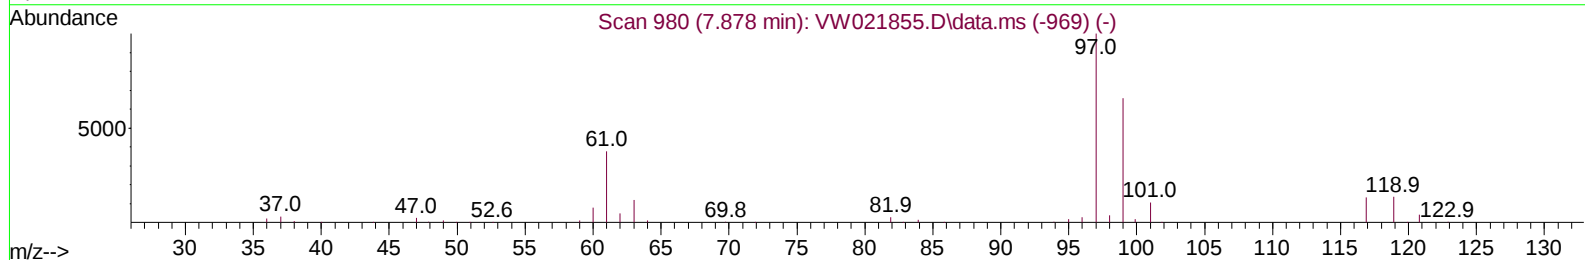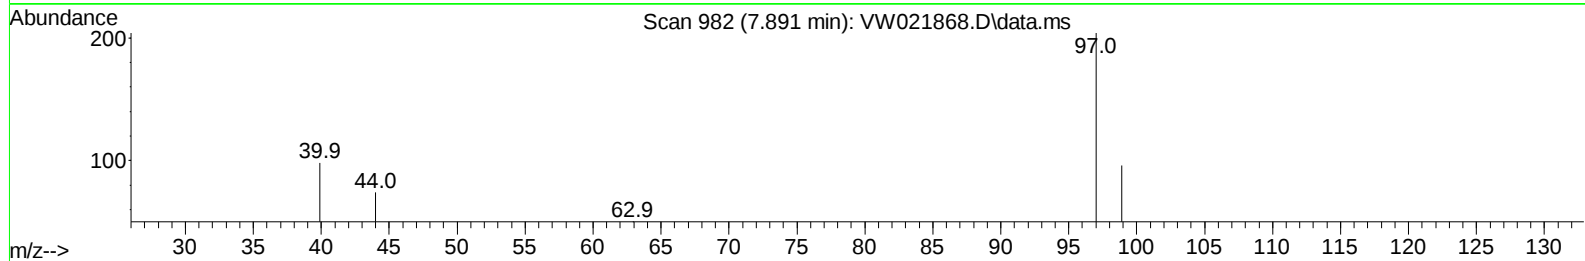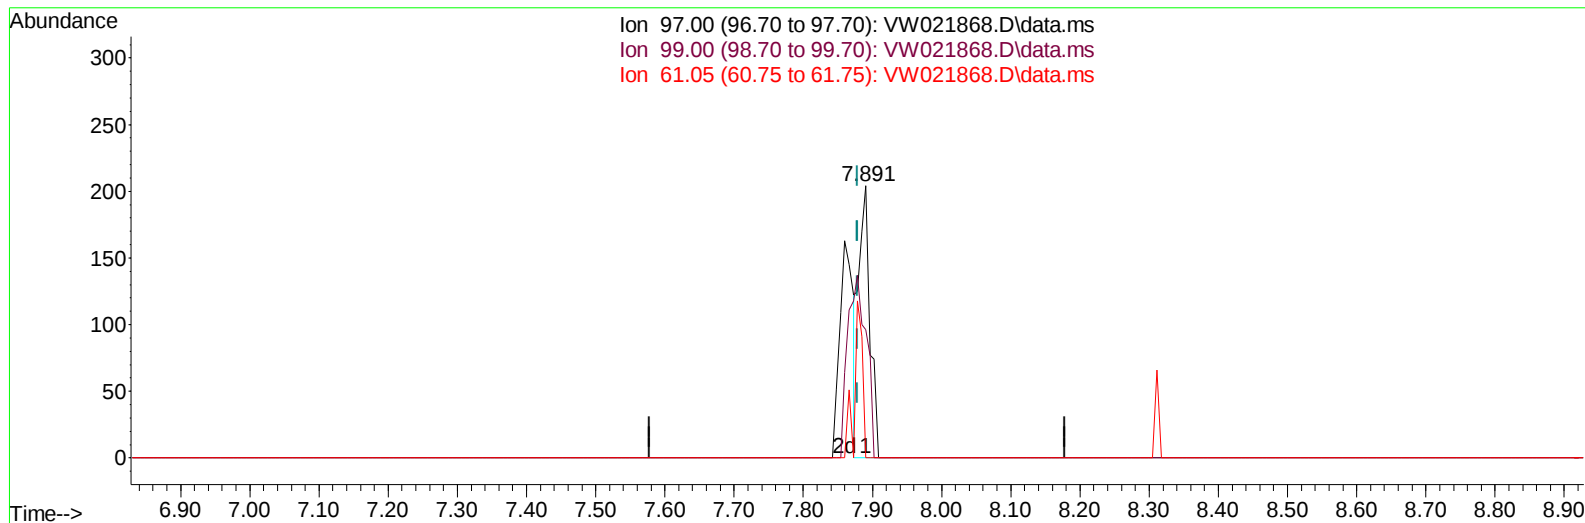

TIC: VW021868.D\data.ms

(30) 1,1,1-Trichloroethane (T)

7.891min (+ 0.012) 8.16 ug/L

response 238

Ion	Exp%	Act%
97.00	100.00	100.00
99.00	64.50	107.98#
61.05	51.10	31.93#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011222\
 Data File : VW021868.D
 Acq On : 12 Jan 2022 16:05
 Operator : SY/VA
 Sample : N1114-08
 Misc : 6.27g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLQ0

Manual IntegrationsAPPROVED

Quant Time: Jan 12 23:51:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM01122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jan 12 23:48:31 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/13/2022
 Supervised By :Mahesh Dadoda 01/13/2022

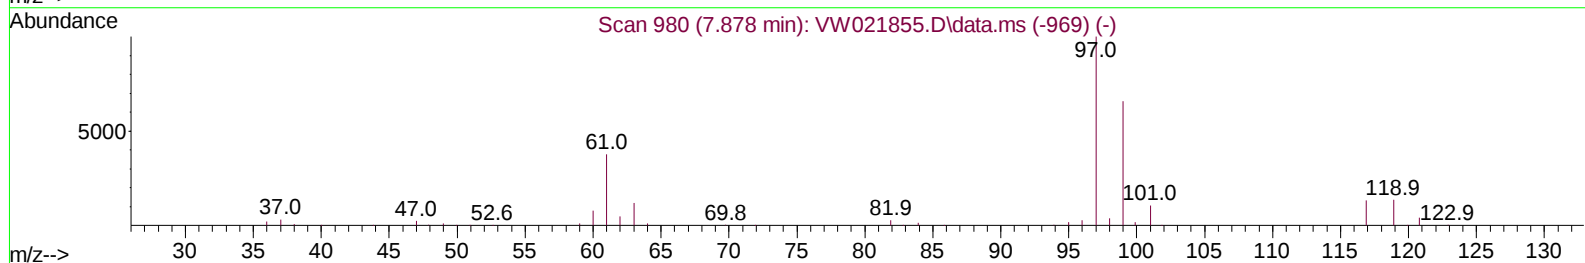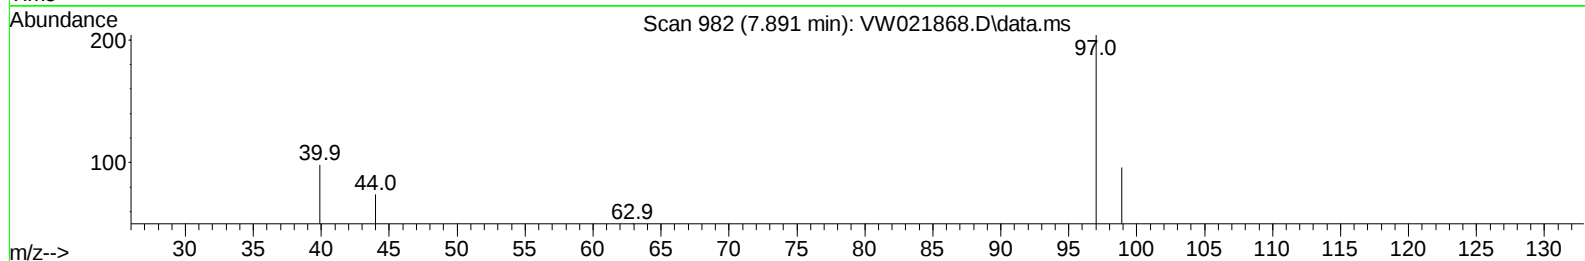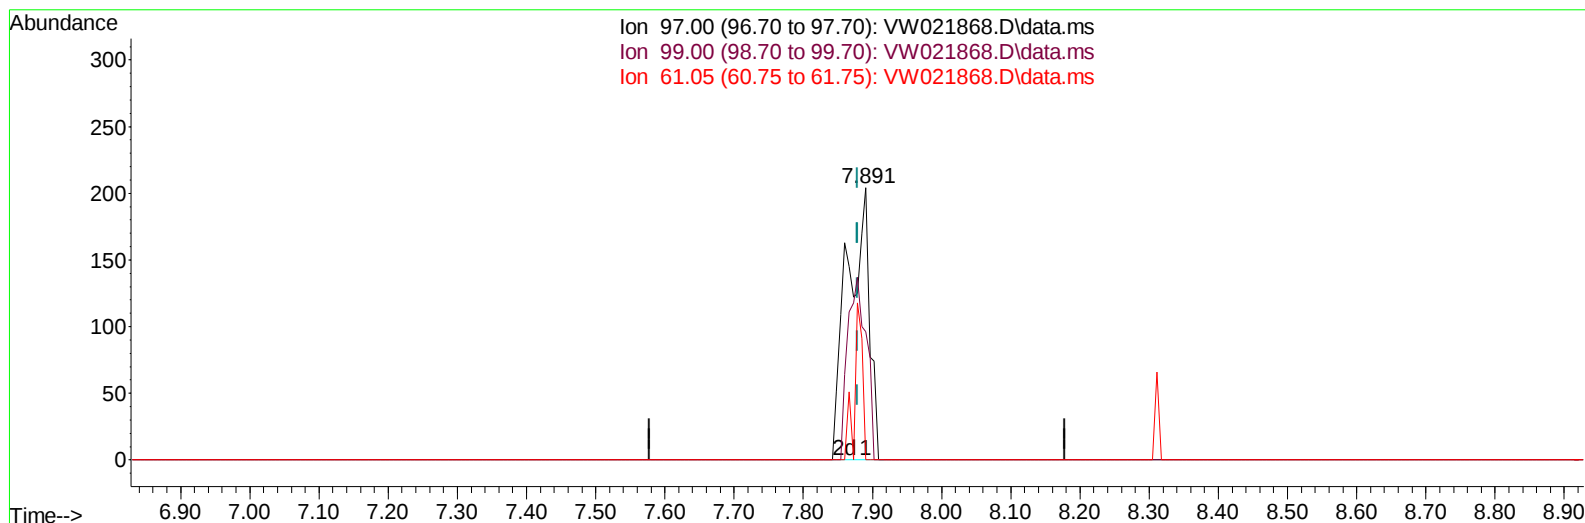

TIC: VW021868.D\data.ms

(30) 1,1,1-Trichloroethane (T)

7.891min (+ 0.012) 15.57 ug/L m

response 454

Ion	Exp%	Act%
97.00	100.00	100.00
99.00	64.50	56.61
61.05	51.10	16.74#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011222\
 Data File : VW021868.D
 Acq On : 12 Jan 2022 16:05
 Operator : SY/VA
 Sample : N1114-08
 Misc : 6.27g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLQ0

Manual IntegrationsAPPROVED

Quant Time: Jan 12 23:51:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM01122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jan 12 23:48:31 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/13/2022
 Supervised By :Mahesh Dadoda 01/13/2022

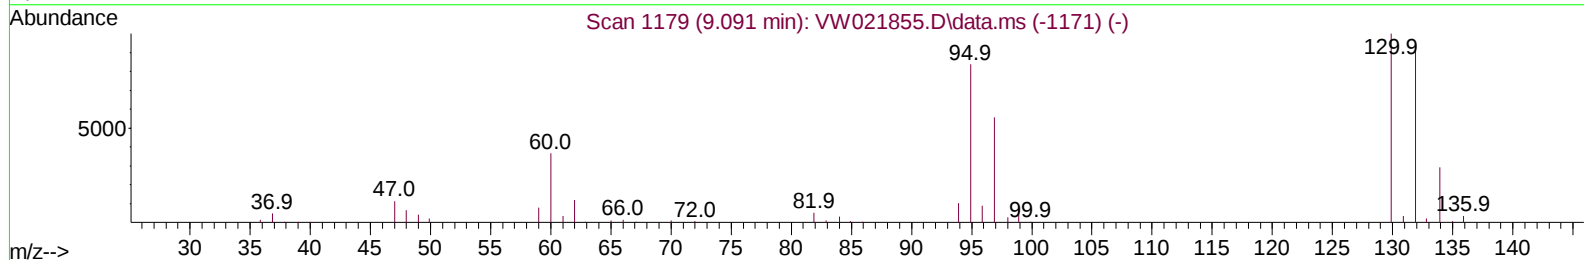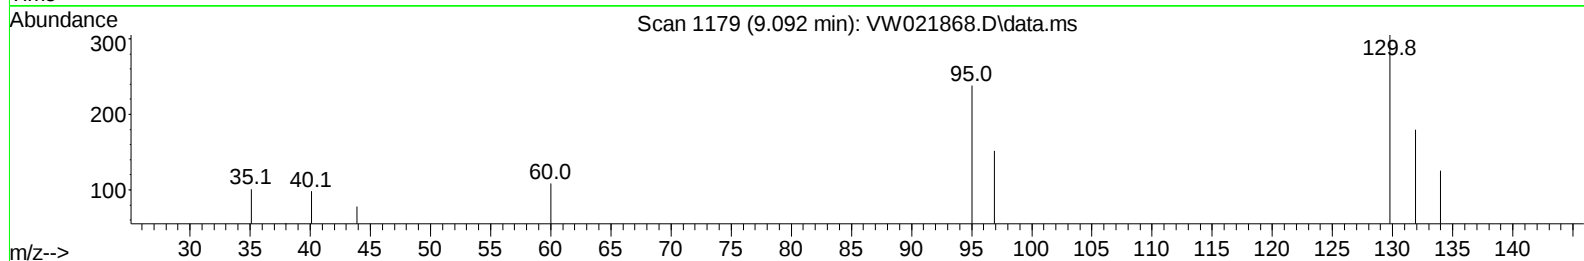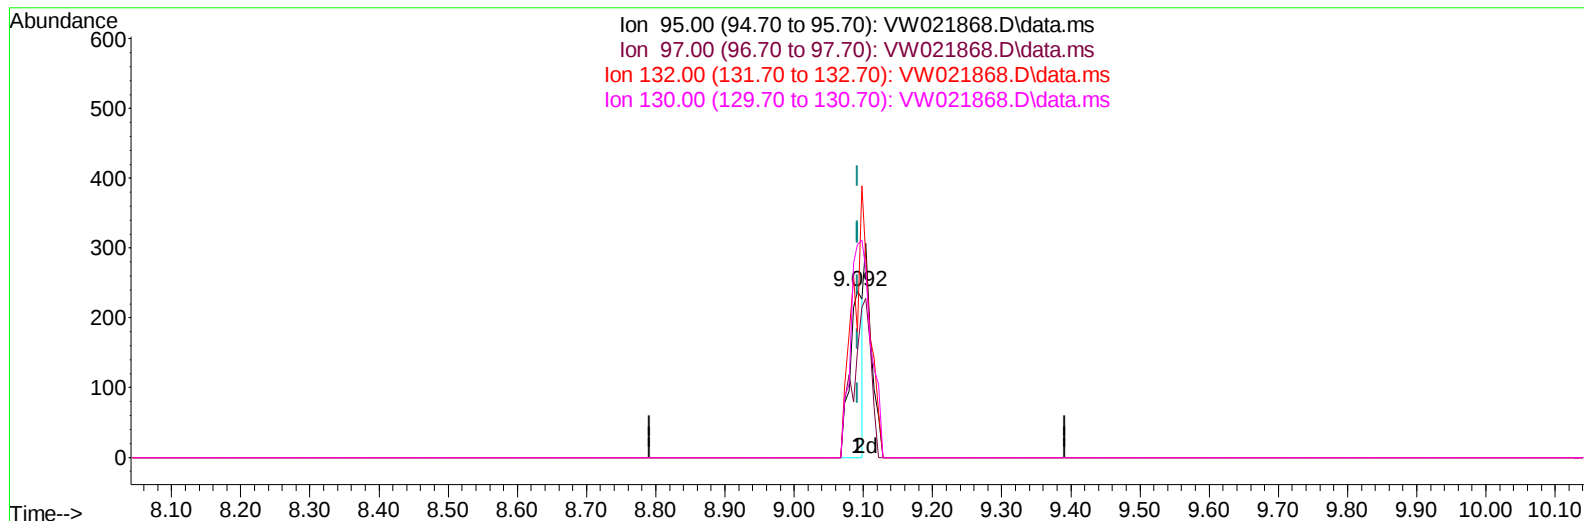

TIC: VW021868.D\data.ms

(34) Trichloroethene (T)

9.092min (+ 0.000) 15.59 ug/L

response 312

Ion	Exp%	Act%
95.00	100.00	100.00
97.00	67.10	63.87
132.00	93.50	75.63
130.00	99.10	128.15




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011222\
 Data File : VW021868.D
 Acq On : 12 Jan 2022 16:05
 Operator : SY/VA
 Sample : N1114-08
 Misc : 6.27g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLQ0

Manual IntegrationsAPPROVED

Quant Time: Jan 12 23:51:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM01122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jan 12 23:48:31 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/13/2022
 Supervised By :Mahesh Dadoda 01/13/2022

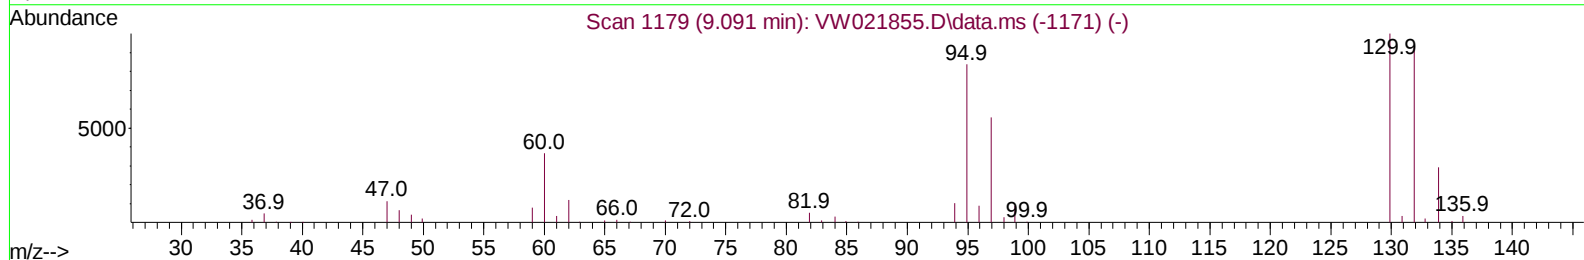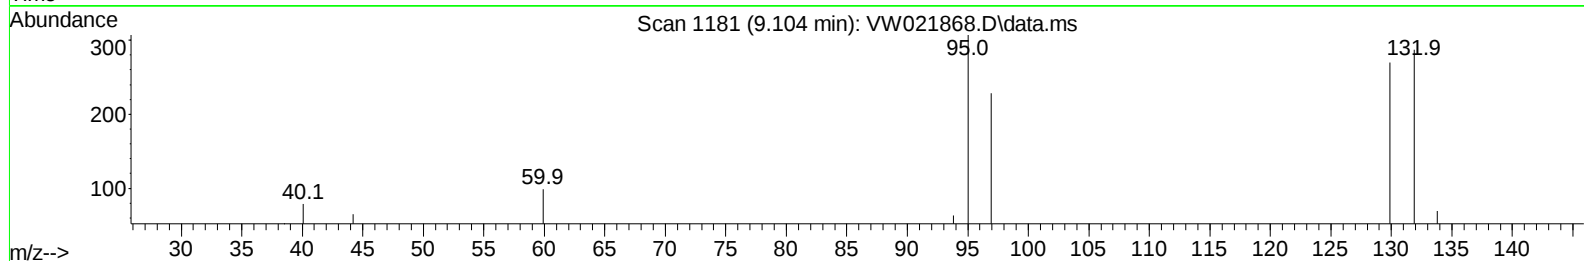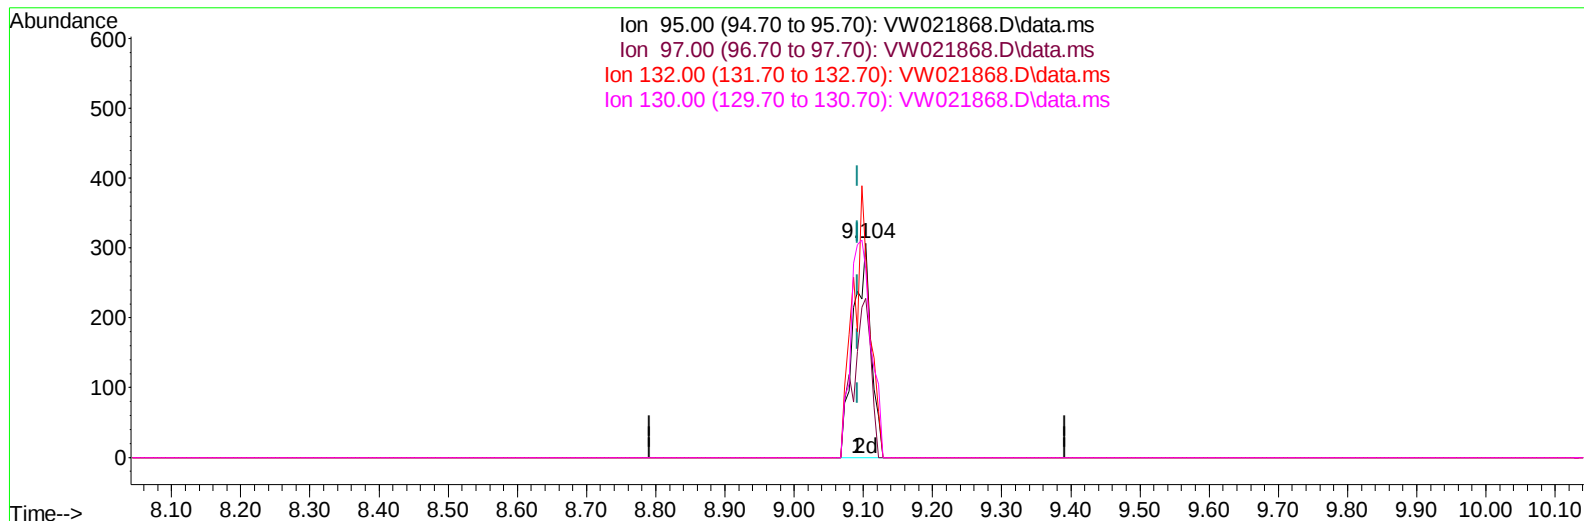

TIC: VW021868.D\data.ms

(34) Trichloroethene (T)

9.104min (+ 0.012) 27.28 ug/L m

response 546

Ion	Exp%	Act%
95.00	100.00	100.00
97.00	67.10	74.27
132.00	93.50	93.49
130.00	99.10	87.95

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011222\
 Data File : VW021868.D
 Acq On : 12 Jan 2022 16:05
 Operator : SY/VA
 Sample : N1114-08
 Misc : 6.27g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLQ0

Manual IntegrationsAPPROVED

Quant Time: Jan 12 23:51:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM01122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jan 12 23:48:31 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/13/2022
 Supervised By :Mahesh Dadoda 01/13/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	1440	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117	1125	25.000	ug/L	# 0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	177m	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.373	65	442m	16.514	ug/L	0.02
Spiked Amount 25.000	Range 30	- 150	Recovery	=	66.040%	
7) Chloroethane-d5	2.904	69	405	16.757	ug/L	0.02
Spiked Amount 25.000	Range 30	- 150	Recovery	=	67.040%	
11) 1,1-Dichloroethene-d2	4.044	63	995	23.548	ug/L	0.02
Spiked Amount 25.000	Range 45	- 110	Recovery	=	94.200%	
21) 2-Butanone-d5	0.000	46	0	0.000	ug/L	
Spiked Amount 50.000	Range 20	- 135	Recovery	=	0.000%#	
24) Chloroform-d	7.653	84	1028m	22.098	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	88.400%	
26) 1,2-Dichloroethane-d4	8.311	65	527m	23.459	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	93.840%	
32) Benzene-d6	8.281	84	1945	26.644	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	106.560%	
36) 1,2-Dichloropropane-d6	9.274	67	578	30.041	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	120.160%#	
41) Toluene-d8	10.323	98	1442	19.596	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	78.400%	
43) trans-1,3-Dichloroprop...	0.000	79	0	0.000	ug/L	
Spiked Amount 25.000	Range 30	- 135	Recovery	=	0.000%#	
47) 2-Hexanone-d5	0.000	63	0	0.000	ug/L	
Spiked Amount 50.000	Range 20	- 135	Recovery	=	0.000%#	
56) 1,1,2,2-Tetrachloroeth...	0.000	84	0	0.000	ug/L	
Spiked Amount 25.000	Range 45	- 120	Recovery	=	0.000%#	
66) 1,2-Dichlorobenzene-d4	0.000	152	0d	0.000	ug/L	
Spiked Amount 25.000	Range 75	- 120	Recovery	=	0.000%#	
Target Compounds						
						Qvalue
12) 1,1-Dichloroethene	4.050	96	601m	27.961	ug/L	
19) 1,1-Dichloroethane	6.226	63	642m	18.848	ug/L	
30) 1,1,1-Trichloroethane	7.891	97	454m	15.569	ug/L	
34) Trichloroethene	9.104	95	546m	27.281	ug/L	
46) Tetrachloroethene	10.860	164	2819	142.441	ug/L	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011222\
Data File : VW021868.D
Acq On : 12 Jan 2022 16:05
Operator : SY/VA
Sample : N1114-08
Misc : 6.27g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLQ0

Manual IntegrationsAPPROVED

Quant Time: Jan 12 23:51:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM01122SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jan 12 23:48:31 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/13/2022
Supervised By :Mahesh Dadoda 01/13/2022

