

Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW011321\
 Data File : VW017848.D
 Acq On : 13 Jan 2021 15:31
 Operator : SY/VA
 Sample : M1074-12
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK01

Manual Integrations
 APPROVED

MMDadoda
 1/15/2021 4:06:52 PM

Quant Time: Jan 14 14:14:36 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122420S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 14 11:39:57 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	351865	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	320293	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	144563	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	125529	23.06	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	92.24%
7) Chloroethane-d5	2.89	69	102394	22.79	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.16%
10) 1,1-Dichloroethene-d2	4.02	63	169312	17.85	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	71.40%
20) 2-Butanone-d5	7.08	46	43495	49.29	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.58%
24) Chloroform-d	7.65	84	209797	22.82	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.28%
26) 1,2-Dichloroethane-d4	8.30	65	120550	25.33	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	101.32%
29) Benzene-d6	8.27	84	430595	23.87	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.48%
33) 1,2-Dichloropropane-d6	9.27	67	121582	24.45	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	97.80%
37) Toluene-d8	10.32	98	397473	22.94	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	91.76%
38) trans-1,3-Dichloropropene-	10.58	79	49402	22.29	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	89.16%
39) 2-Hexanone-d5	10.93	63	28277	45.28	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.56%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	83280	22.56	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	90.24%
61) 1,2-Dichlorobenzene-d4	13.85	152	112765	22.40	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	89.60%

Target Compounds					Ovalue
13) Acetone	4.14	43	1587m	2.083 ug/L	
16) Methylene chloride	4.92	84	10091	2.005 ug/L	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW011321\
Data File : VW017848.D
Acq On : 13 Jan 2021 15:31
Operator : SY/VA
Sample : M1074-12
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 5 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
VHBLK01

Manual Integrations
APPROVED

MMDadoda
1/15/2021 4:06:52 PM

Quant Time: Jan 14 14:14:36 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122420S.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 14 11:39:57 2021
Response via : Initial Calibration

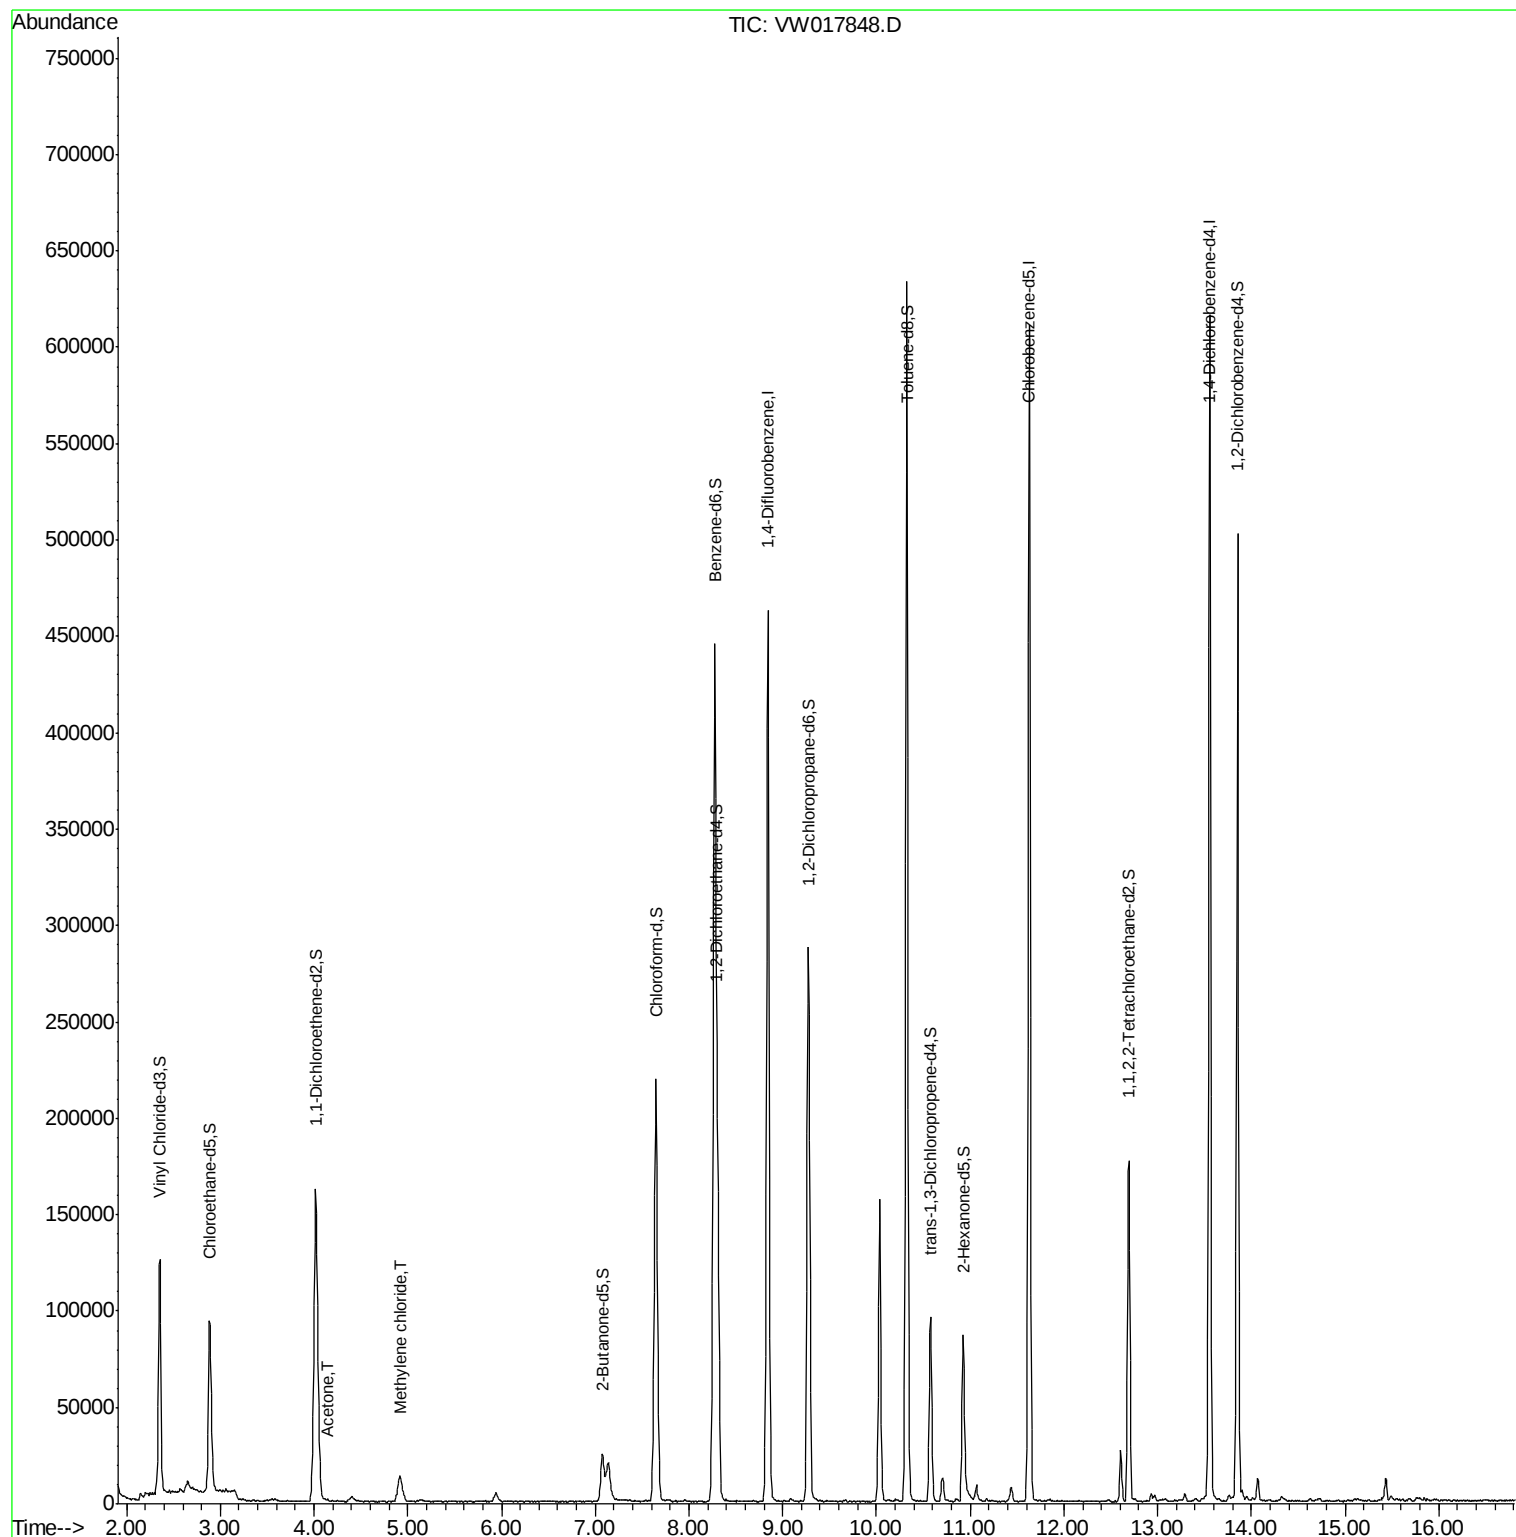

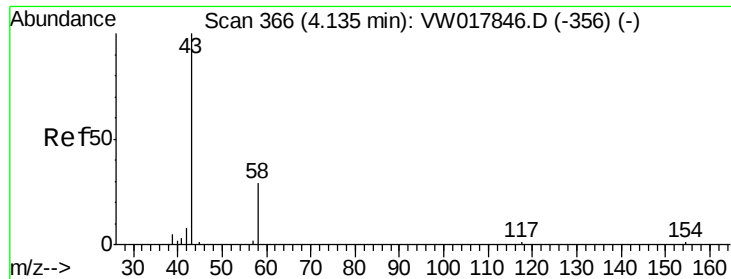





#13
Acetone
Concen: 2.083 ug/L m
RT: 4.14 min Scan# 367
Delta R.T. 0.01 min
Lab File: VW017848.D
Acq: 13 Jan 2021 15:31

Instrument :
MSVOA_W
ClientSampled :
VHBLK01

Tot Ion: 43 Resp: 1587
Ion Ratio Lower Upper
43 100
58 2.1 0.0 60.8

Manual Integrations
APPROVED

MMDadoda
1/15/2021 4:06:52 PM

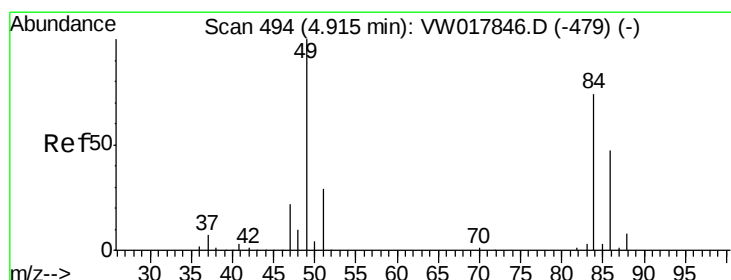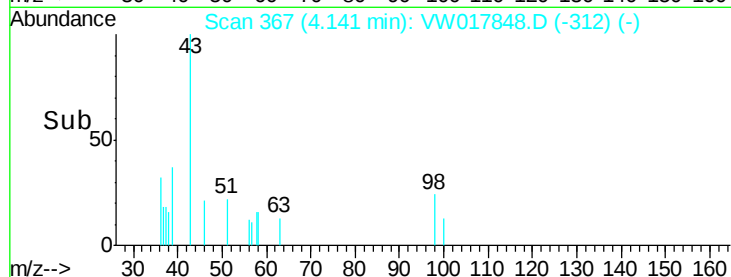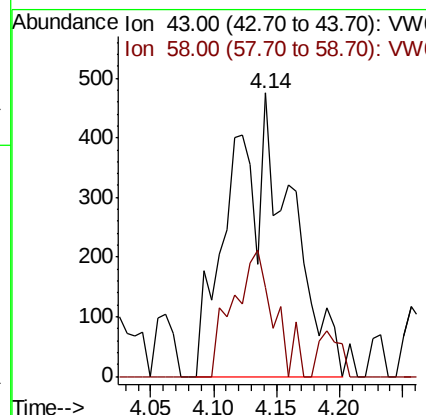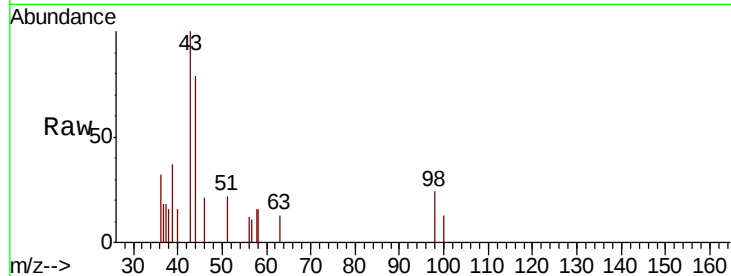

#16
Methylene chloride
Concen: 2.005 ug/L
RT: 4.92 min Scan# 494
Delta R.T. -0.00 min
Lab File: VW017848.D
Acq: 13 Jan 2021 15:31

Tgt Ion: 84 Resp: 10091
Ion Ratio Lower Upper
84 100
49 108.0 90.5 168.1
86 61.8 44.8 83.2

