

Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW011321\
 Data File : VW017867.D
 Acq On : 13 Jan 2021 22:58
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK

Manual Integrations
 APPROVED

MMDadoda
 1/15/2021 4:07:22 PM

Quant Time: Jan 14 15:17:47 2021
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122420S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 14 11:39:57 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	337315	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	317935	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	152230	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	117790	22.57	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.28%
7) Chloroethane-d5	2.89	69	98960	22.97	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.88%
10) 1,1-Dichloroethene-d2	4.02	63	155844	17.14	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.56%
20) 2-Butanone-d5	7.07	46	49900	58.99	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	117.98%
24) Chloroform-d	7.65	84	214345	24.32	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.28%
26) 1,2-Dichloroethane-d4	8.31	65	127091m	27.86	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	111.44%
29) Benzene-d6	8.27	84	429012	23.95	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.80%
33) 1,2-Dichloropropane-d6	9.27	67	124201	25.16	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	100.64%
37) Toluene-d8	10.32	98	387307	22.52	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.08%
38) trans-1,3-Dichloropropene-	10.58	79	47735	21.69	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	86.76%
39) 2-Hexanone-d5	10.93	63	34894	56.29	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	112.58%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	94429	25.77	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	103.08%
61) 1,2-Dichlorobenzene-d4	13.85	152	122868	23.18	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	92.72%

Target Compounds					Ovalue
16) Methylene chloride	4.91	84	8019	1.662 ug/L	80

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW011321\
Data File : VW017867.D
Acq On : 13 Jan 2021 22:58
Operator : SY/VA
Sample : VIBLK
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 24 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
VIBLK

Manual Integrations
APPROVED

MMDadoda
1/15/2021 4:07:22 PM

Quant Time: Jan 14 15:17:47 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122420S.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 14 11:39:57 2021
Response via : Initial Calibration

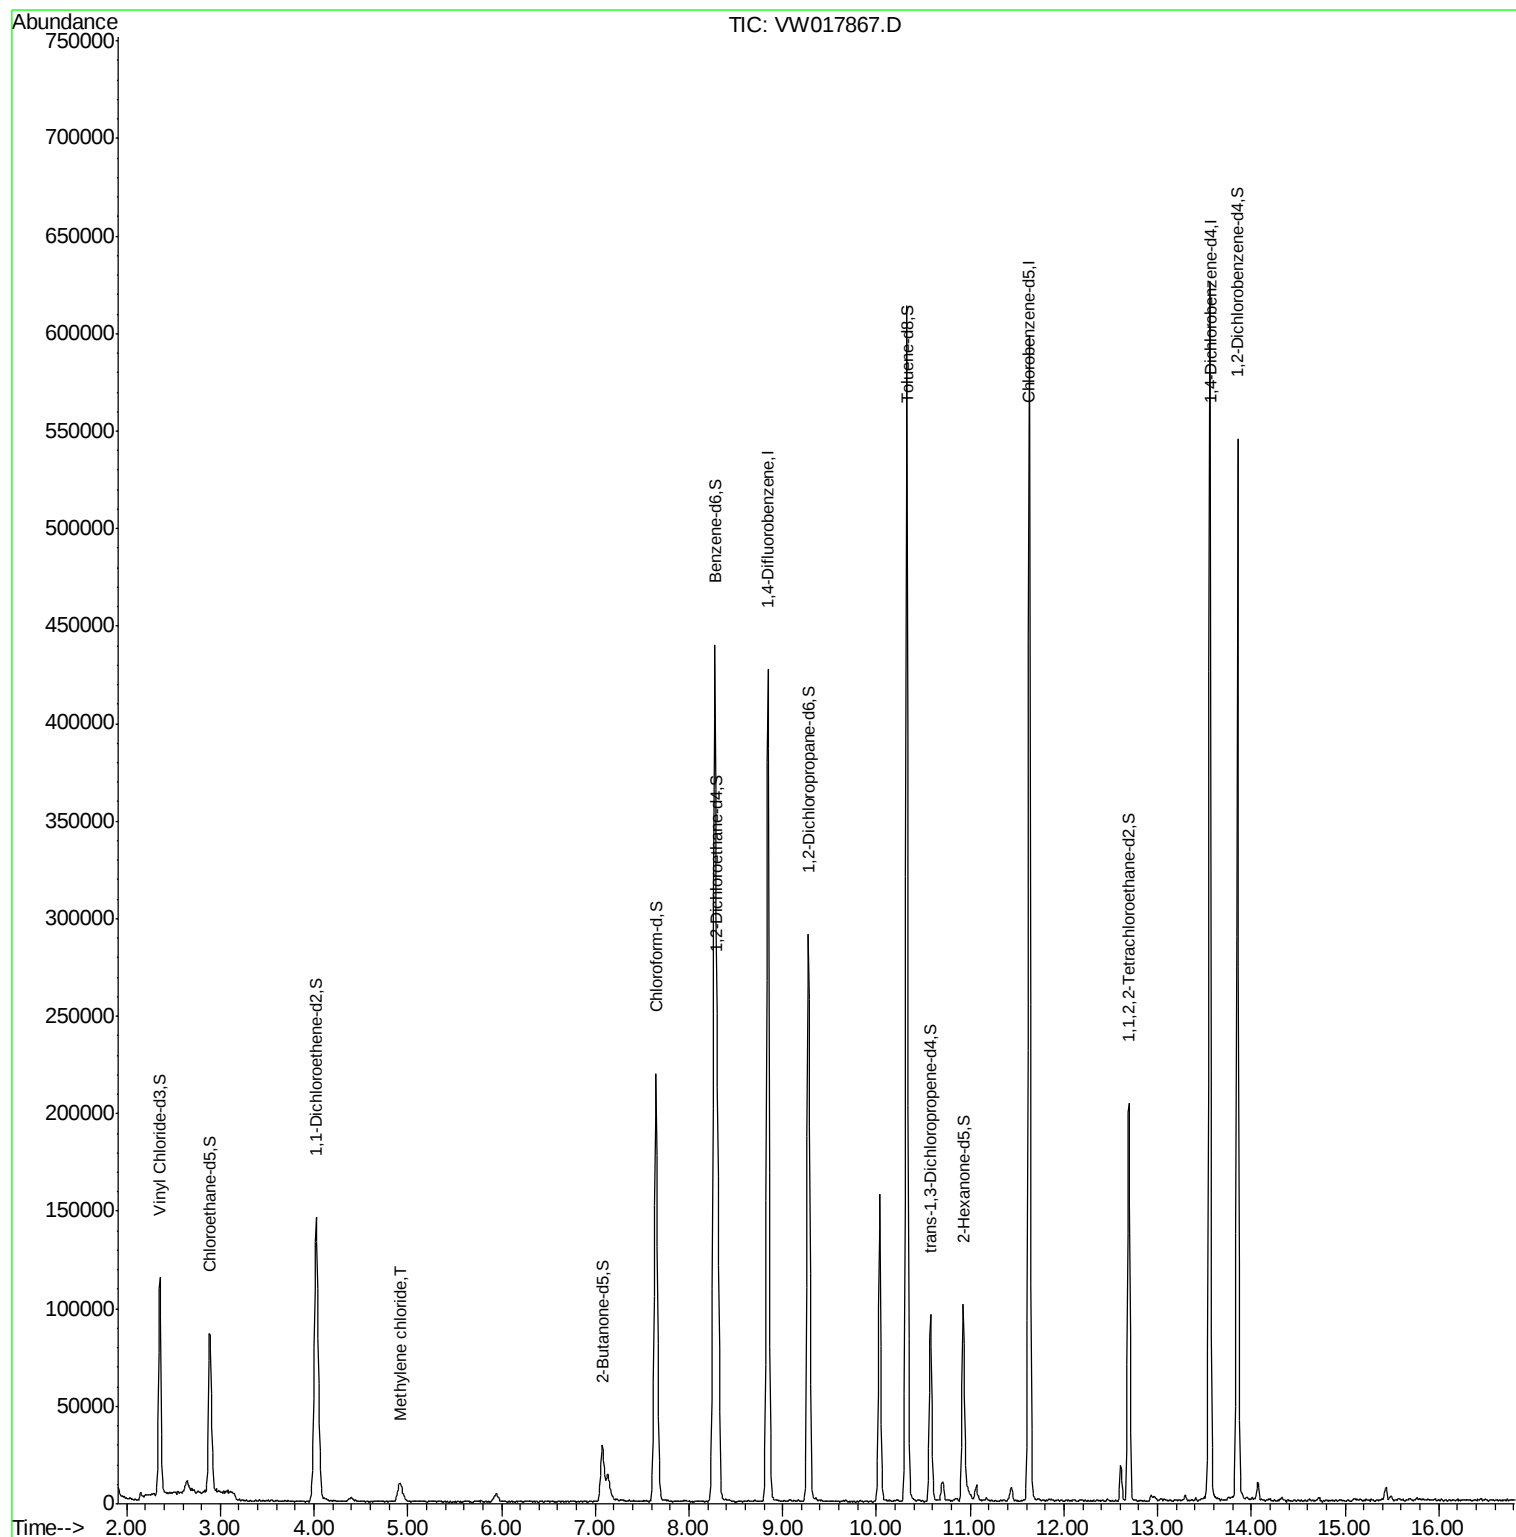

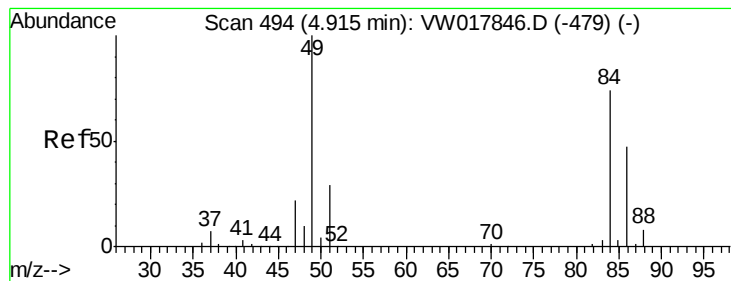

#16
 Methvlene chloride
 Concen: 1.662 ug/L
 RT: 4.91 min Scan# 493
 Delta R.T. -0.01 min
 Lab File: VW017867.D
 Acq: 13 Jan 2021 22:58

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK

Tot Ion	Ratio	Lower	Upper
84	100		
49	102.7	90.5	168.1
86	53.0	44.8	83.2

Manual Integrations
 APPROVED

MMDadoda
 1/15/2021 4:07:22 PM

