


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW011419\
Data File : VW008262.D
Acq On : 14 Jan 2019 23:14
Operator : SY/VA
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W010819S.M
Title : SW846 8260
Last Update : Wed Jan 09 04:40:48 2019

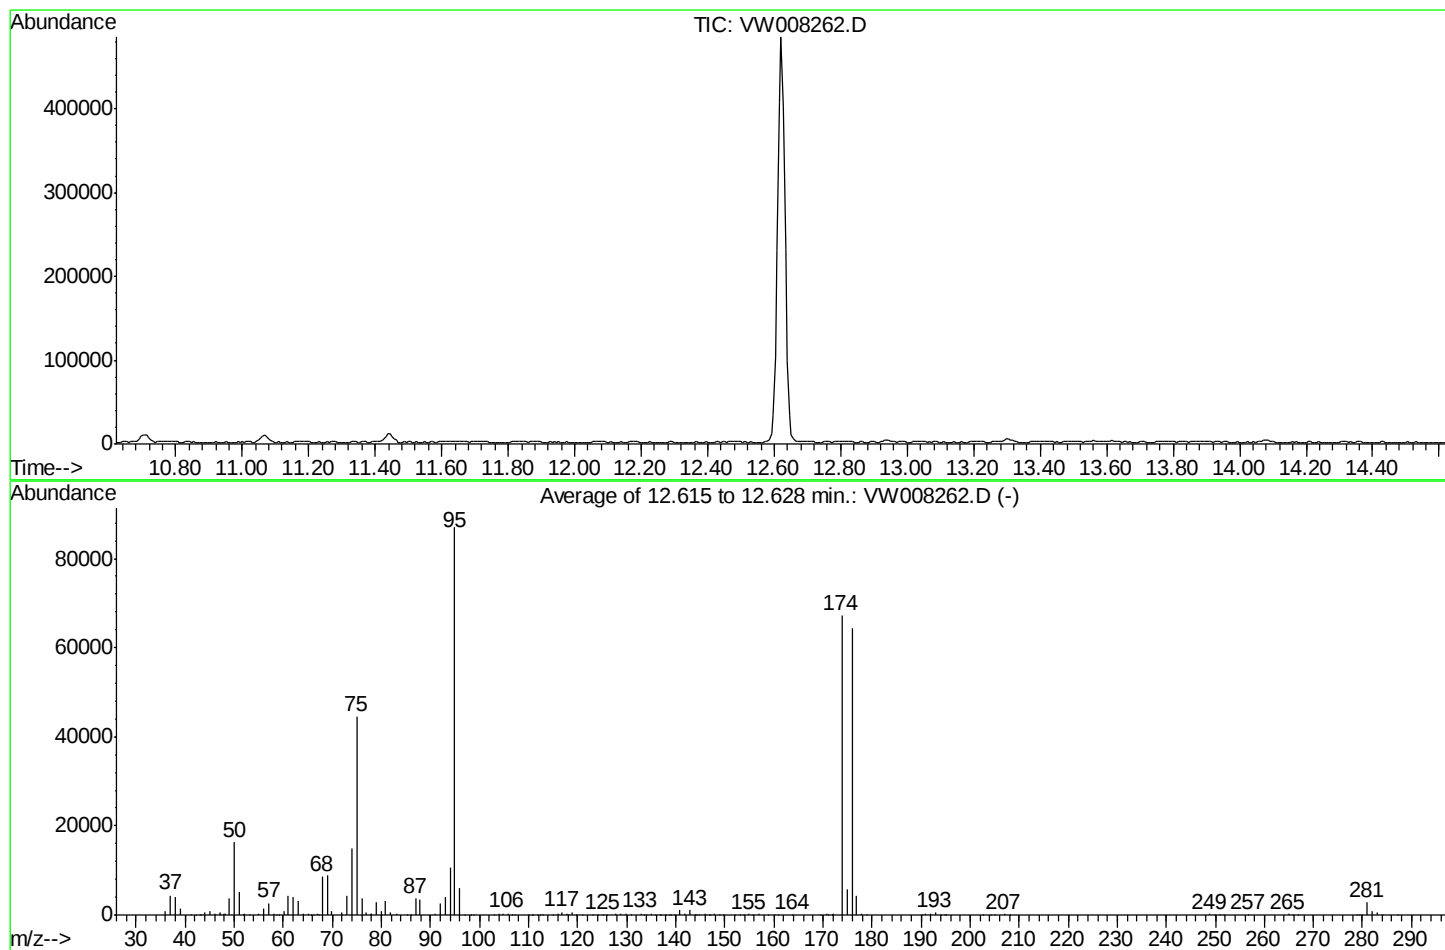

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.7	16310	PASS
75	95	30	60	51.1	44501	PASS
95	95	100	100	100.0	87005	PASS
96	95	5	9	7.0	6111	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	77.2	67154	PASS
175	174	5	9	8.7	5817	PASS
176	174	95	101	96.0	64464	PASS
177	176	5	9	6.6	4282	PASS