




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011422\
 Data File : VW021910.D
 Acq On : 14 Jan 2022 13:49
 Operator : SY/VA
 Sample : VIBLK588
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK588

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/17/2022
 Supervised By :Mahesh Dadoda 01/17/2022

Quant Time: Jan 17 00:46:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jan 17 00:44:09 2022
 Response via : Initial Calibration

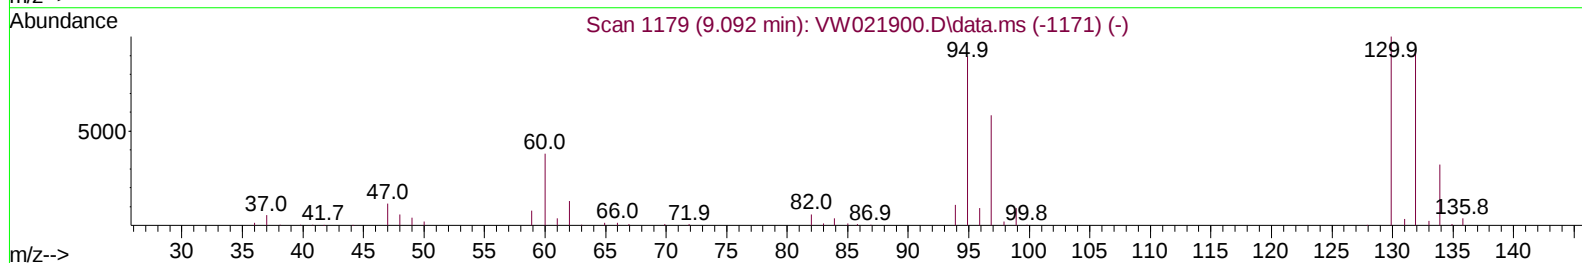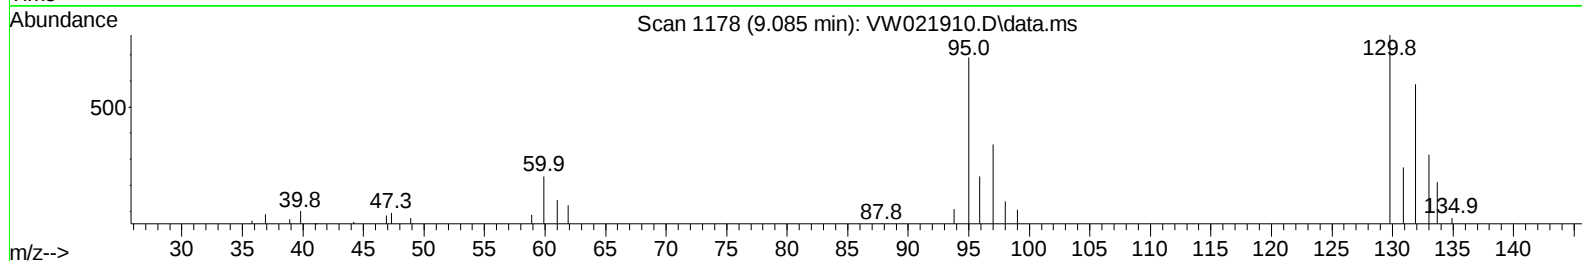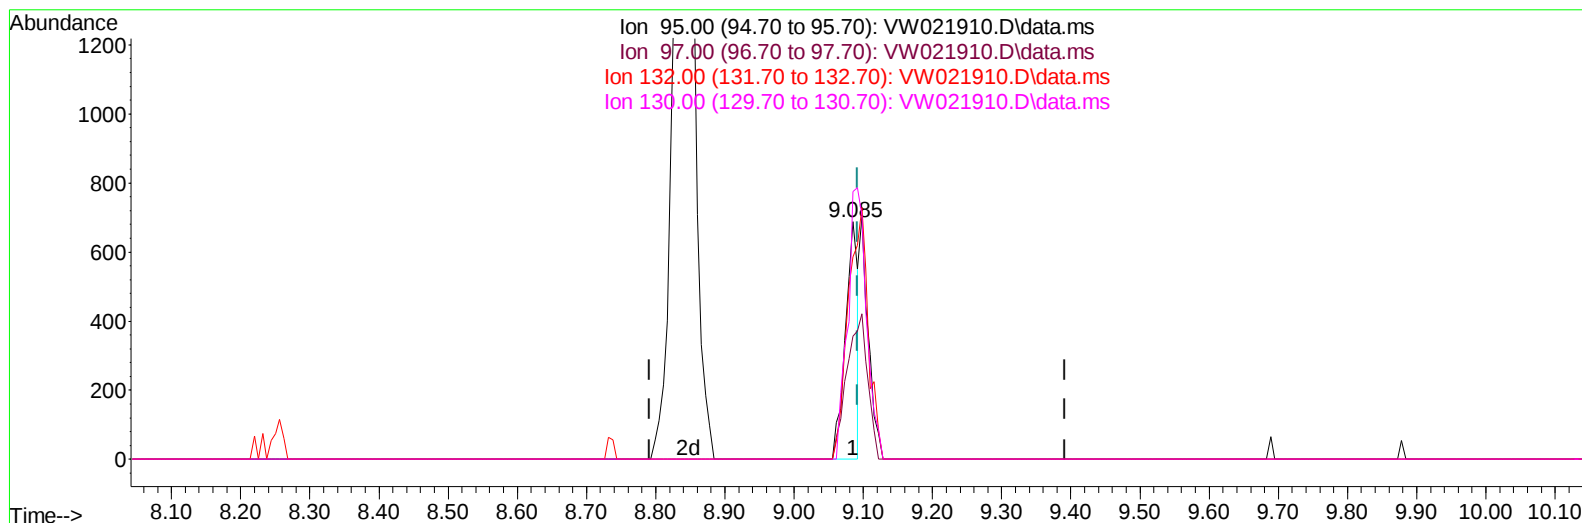

TIC: VW021910.D\data.ms

(34) Trichloroethene (T)

9.085min (-0.006) 0.31 ug/L

response 865

Ion	Exp%	Act%
95.00	100.00	100.00
97.00	67.10	51.81
132.00	93.50	85.05
130.00	99.10	112.48




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011422\
Data File : VW021910.D
Acq On : 14 Jan 2022 13:49
Operator : SY/VA
Sample : VIBLK588
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK588

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/17/2022
Supervised By :Mahesh Dadoda 01/17/2022

Quant Time: Jan 17 00:46:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Jan 17 00:44:09 2022
Response via : Initial Calibration

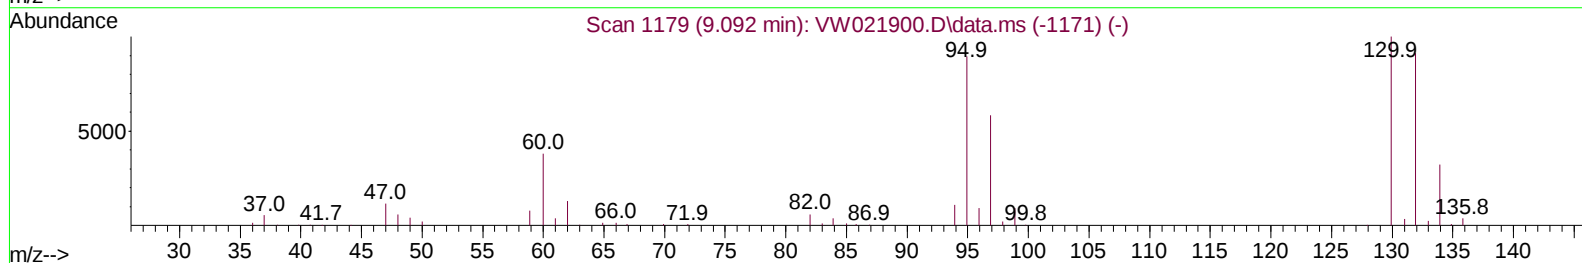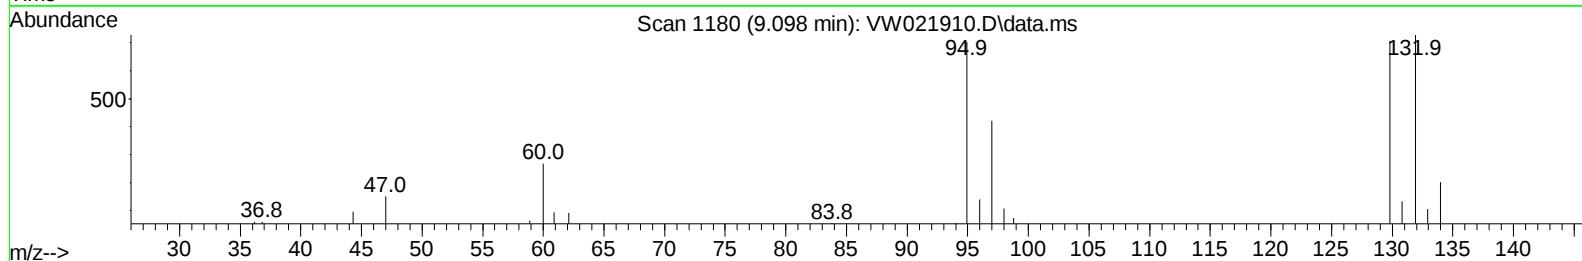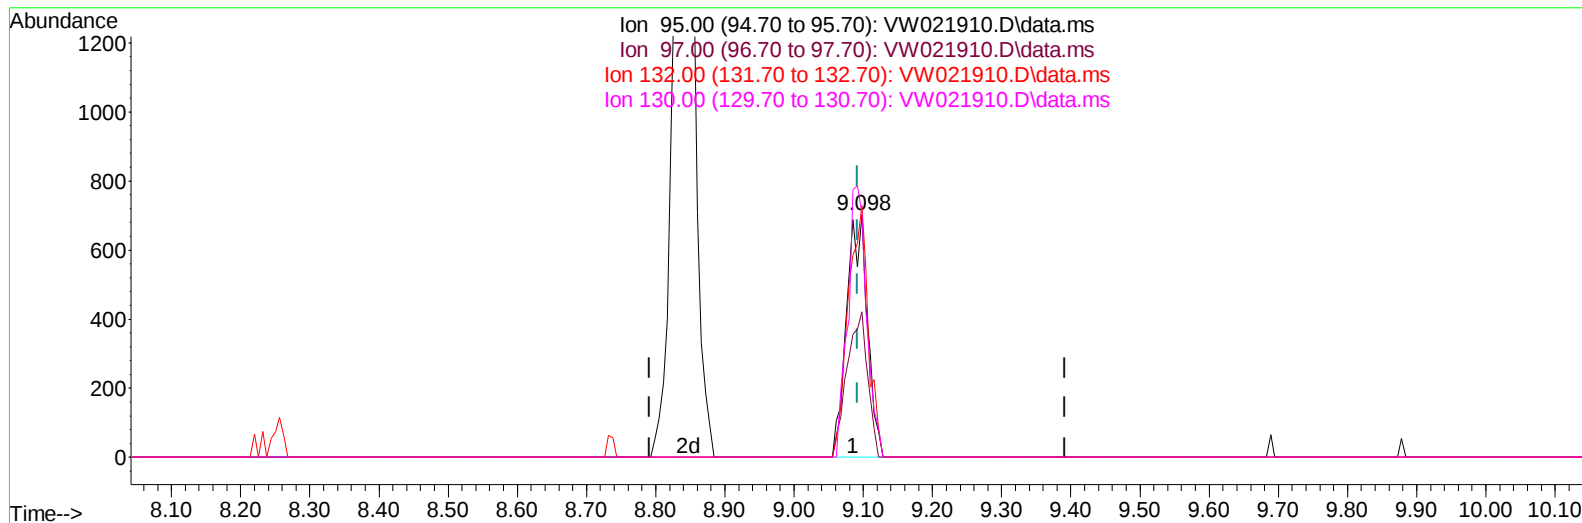

TIC: VW021910.D\data.ms

(34) Trichloroethene (T)

9.098min (+ 0.006) 0.52 ug/L m

response 1467

Ion	Exp%	Act%
95.00	100.00	100.00
97.00	67.10	59.97
132.00	93.50	103.70
130.00	99.10	100.71

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011422\
 Data File : VW021910.D
 Acq On : 14 Jan 2022 13:49
 Operator : SY/VA
 Sample : VIBLK588
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK588

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/17/2022
 Supervised By :Mahesh Dadoda 01/17/2022

Quant Time: Jan 17 00:46:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jan 17 00:44:09 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.842	114		163936	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.628	117		157631	25.000	ug/L	# 0.00
58) 1,4-Dichlorobenzene-d4	13.554	152		89298	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65		58548	19.215	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	76.840%		
7) Chloroethane-d5	2.879	69		40319	14.653	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	58.600%		
11) 1,1-Dichloroethene-d2	4.013	63		69693	14.488	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	57.960%		
21) 2-Butanone-d5	7.080	46		24405	56.746	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	113.500%		
24) Chloroform-d	7.647	84		101711	19.205	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	76.800%		
26) 1,2-Dichloroethane-d4	8.305	65		53828	21.047	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	84.200%		
32) Benzene-d6	8.275	84		211209	20.650	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	82.600%		
36) 1,2-Dichloropropane-d6	9.274	67		57072	21.170	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	84.680%		
41) Toluene-d8	10.323	98		206791	20.056	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	80.240%		
43) trans-1,3-Dichloroprop...	10.579	79		22259	19.447	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	77.800%		
47) 2-Hexanone-d5	10.921	63		21614	59.085	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	118.180%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84		48807	23.152	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	92.600%		
66) 1,2-Dichlorobenzene-d4	13.847	152		78067	21.261	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	85.040%		
Target Compounds							
34) Trichloroethene	9.098	95		1467m	0.523	ug/L	
46) Tetrachloroethene	10.866	164		6674	2.407	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011422\
Data File : VW021910.D
Acq On : 14 Jan 2022 13:49
Operator : SY/VA
Sample : VIBLK588
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK588

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/17/2022
Supervised By :Mahesh Dadoda 01/17/2022

Quant Time: Jan 17 00:46:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Jan 17 00:44:09 2022
Response via : Initial Calibration

