

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011422\
 Data File : VW021917.D
 Acq On : 14 Jan 2022 16:51
 Operator : SY/VA
 Sample : VIBLK590
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK590

Manual IntegrationsAPPROVED

Quant Time: Jan 17 00:47:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jan 17 00:44:09 2022
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

01/17/2022
 Supervised By :Mahesh
 Dadoda

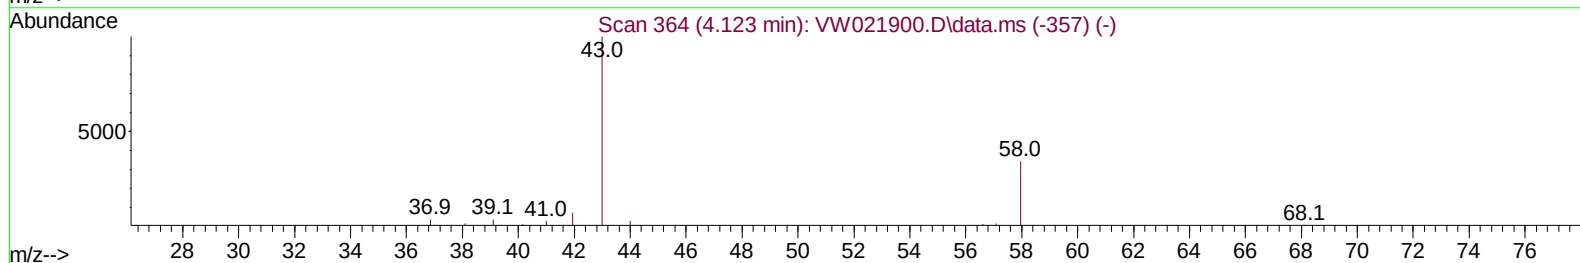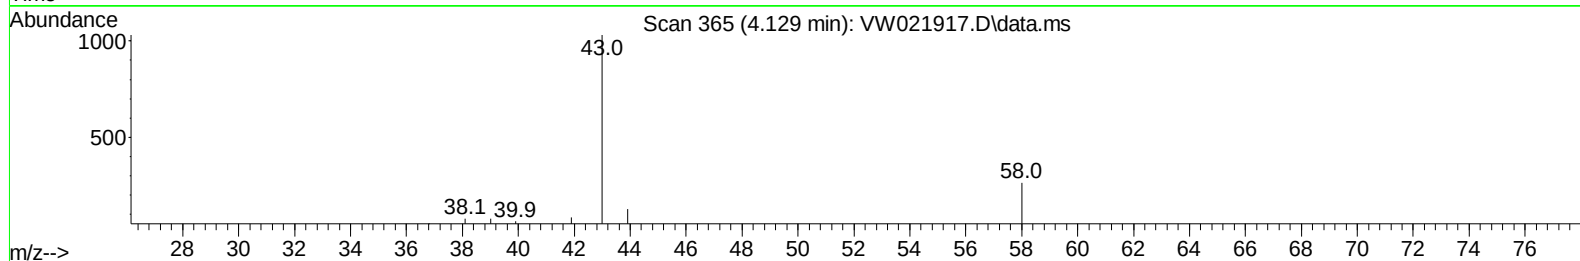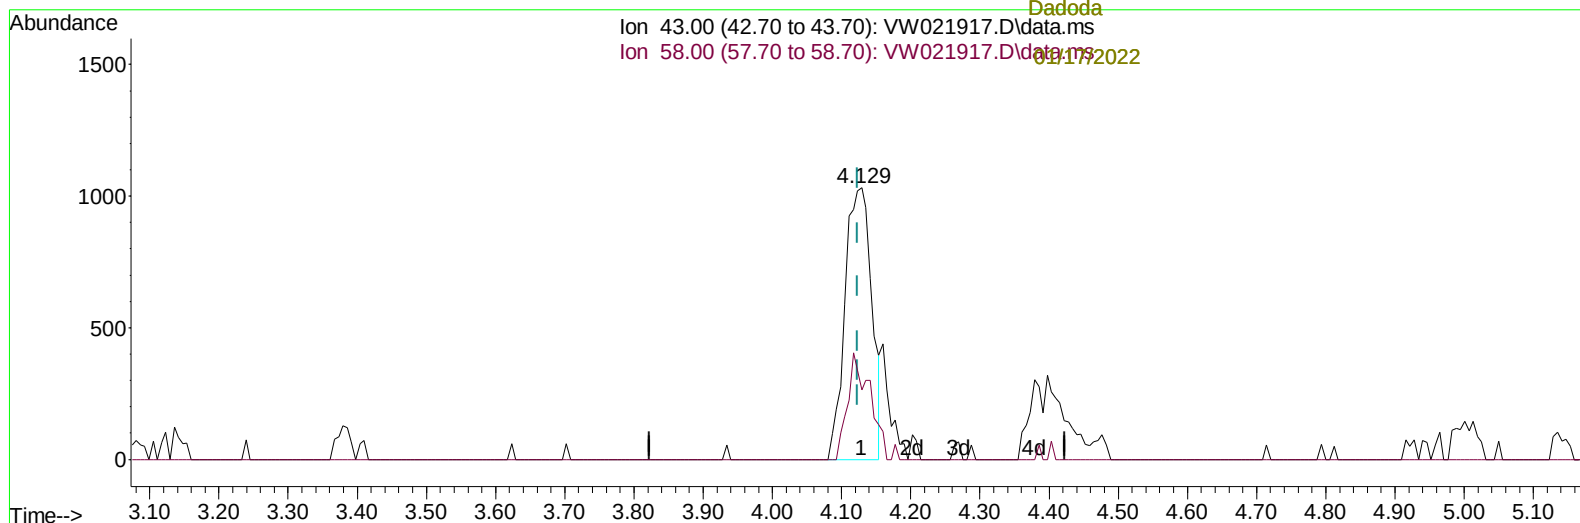

TIC: VW021917.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 8.79 ug/L

response 2774

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.40	13.12
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011422\
 Data File : VW021917.D
 Acq On : 14 Jan 2022 16:51
 Operator : SY/VA
 Sample : VIBLK590
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK590

Manual IntegrationsAPPROVED

Quant Time: Jan 17 00:47:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jan 17 00:44:09 2022
 Response via : Initial Calibration




Reviewed By :Semsettin
 Yesilyurt

01/17/2022

Supervised By :Mahesh

Dadoda

01/17/2022

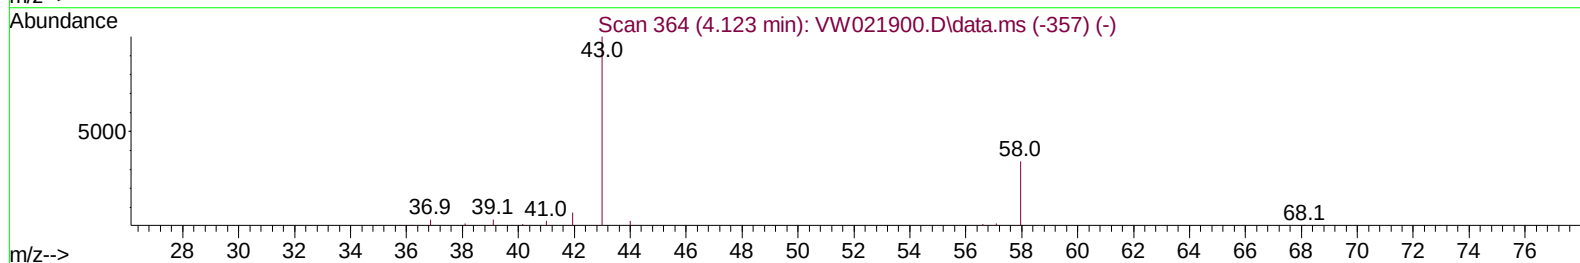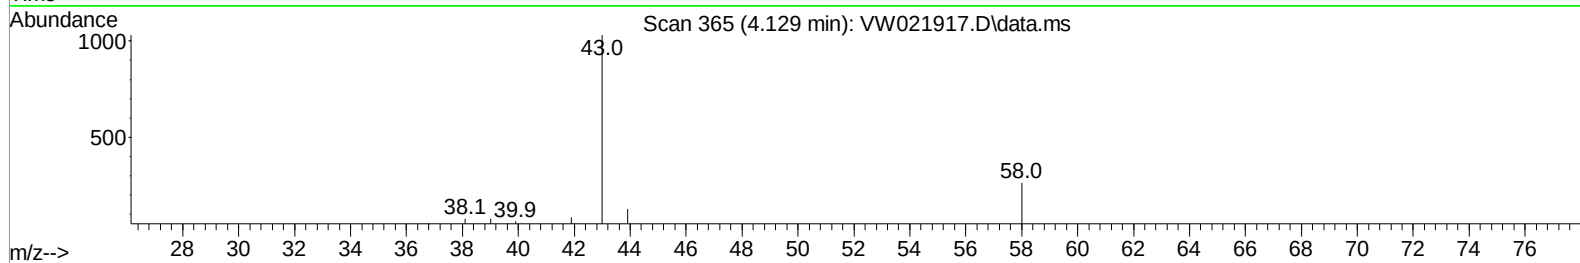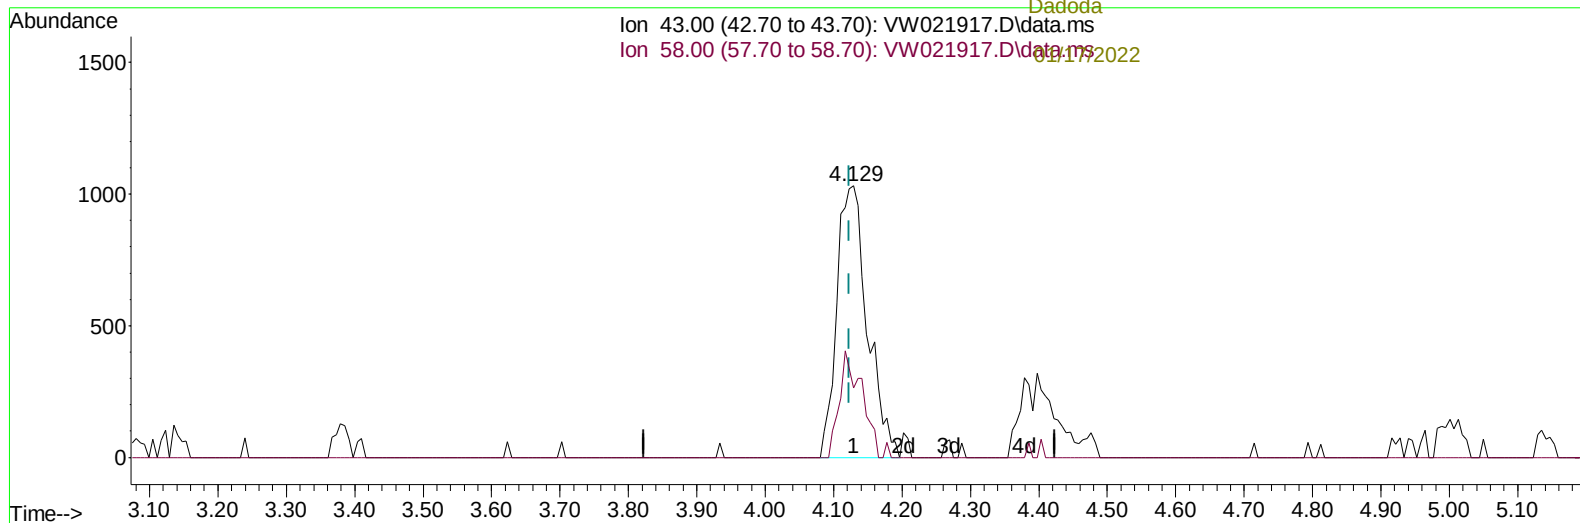

TIC: VW021917.D\data.ms

(13) Acetone (T)

4.129min (+ 0.006) 10.05 ug/L m

response 3174

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.40	11.47
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011422\
 Data File : VW021917.D
 Acq On : 14 Jan 2022 16:51
 Operator : SY/VA
 Sample : VIBLK590
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK590

Manual IntegrationsAPPROVED

Quant Time: Jan 17 00:47:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jan 17 00:44:09 2022
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

01/17/2022
 Supervised By :Mahesh
 Dadoda

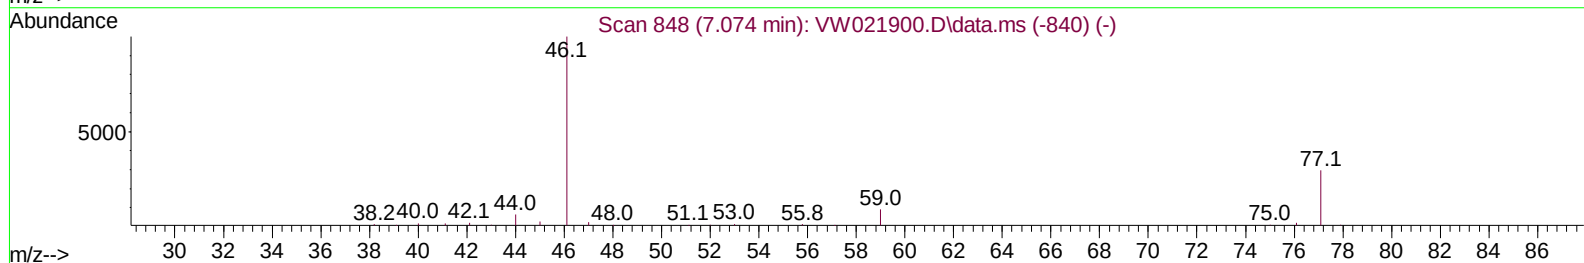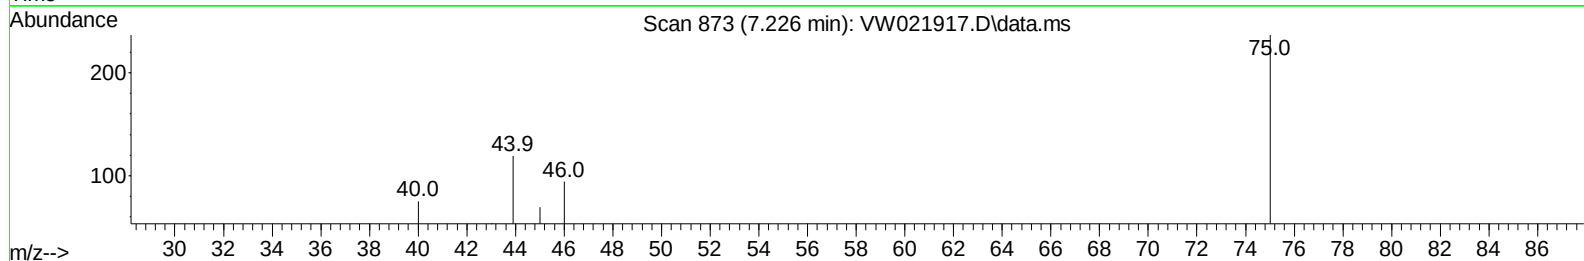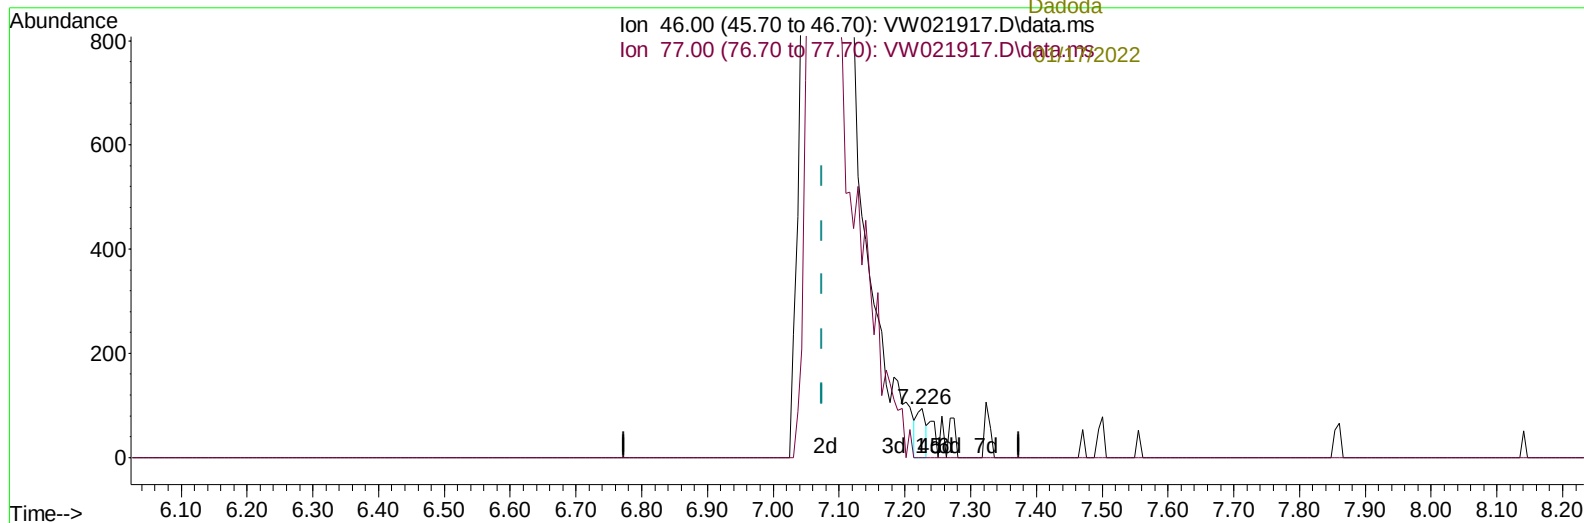

TIC: VW021917.D\data.ms

(21) 2-Butanone-d5 (S)

7.226min (+ 0.153) 0.23 ug/L

response 89

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	20.20	22.47
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011422\
 Data File : VW021917.D
 Acq On : 14 Jan 2022 16:51
 Operator : SY/VA
 Sample : VIBLK590
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1




Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK590

Manual IntegrationsAPPROVED

Quant Time: Jan 17 00:47:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jan 17 00:44:09 2022
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

01/17/2022
 Supervised By :Mahesh
 Dadoda

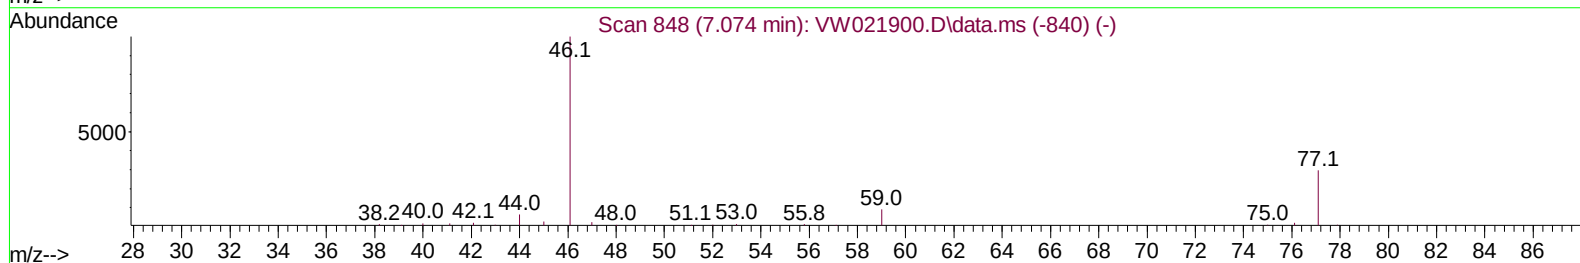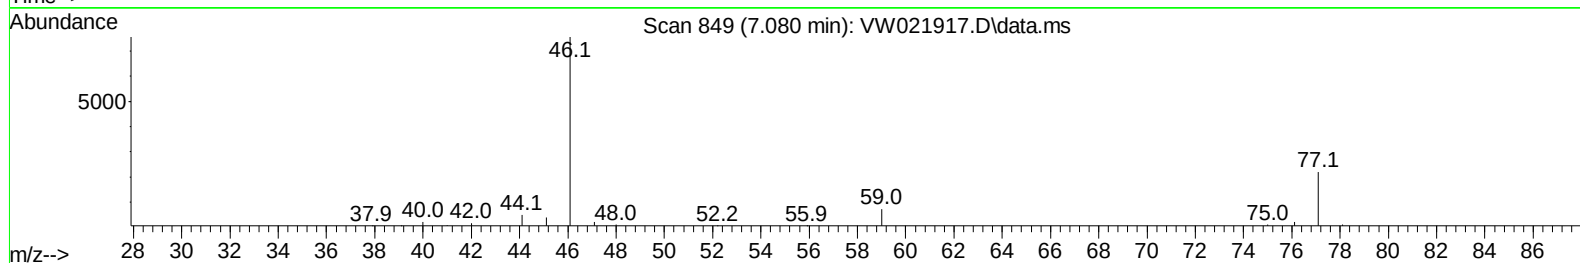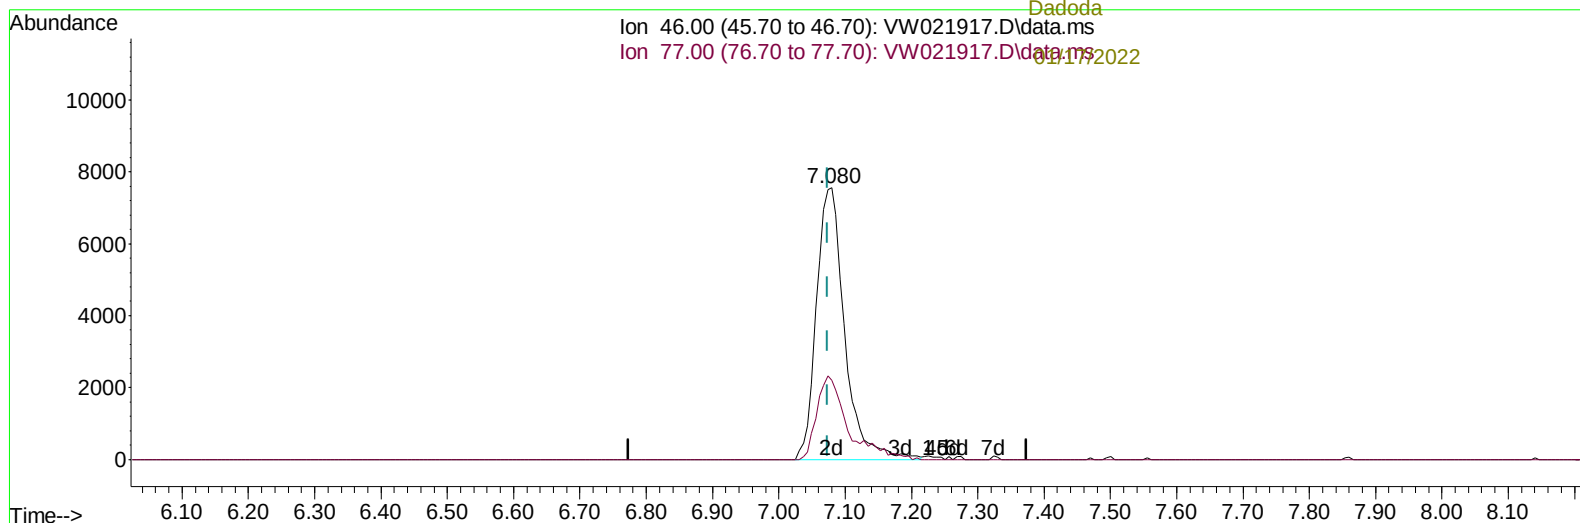

TIC: VW021917.D\data.ms

(21) 2-Butanone-d5 (S)

7.080min (+ 0.006) 58.16 ug/L m

response 22224

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	20.20	0.09#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011422\
 Data File : VW021917.D
 Acq On : 14 Jan 2022 16:51
 Operator : SY/VA
 Sample : VIBLK590
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK590

Manual IntegrationsAPPROVED

Quant Time: Jan 17 00:47:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jan 17 00:44:09 2022
 Response via : Initial Calibration

Reviewed By :Semsettin
 Yesilyurt

01/17/2022
 Supervised By :Mahesh
 Dadoda

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
-----01/17/2022							
Internal Standards							
1) 1,4-Difluorobenzene	8.842	114	145659	25.000	ug/L	#	0.00
28) Chlorobenzene-d5	11.628	117	147079	25.000	ug/L		0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	84952	25.000	ug/L		0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.349	65	55487	20.495	ug/L		0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	82.000%		
7) Chloroethane-d5	2.885	69	40491	16.562	ug/L		0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	66.240%		
11) 1,1-Dichloroethene-d2	4.013	63	64425	15.073	ug/L		0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	60.280%		
21) 2-Butanone-d5	7.080	46	22224m	58.159	ug/L		0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	116.320%		
24) Chloroform-d	7.647	84	96631	20.535	ug/L		0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	82.160%		
26) 1,2-Dichloroethane-d4	8.305	65	50831	22.369	ug/L		0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	89.480%		
32) Benzene-d6	8.275	84	197968	20.744	ug/L		0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	82.960%		
36) 1,2-Dichloropropane-d6	9.268	67	52750	20.971	ug/L		0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	83.880%		
41) Toluene-d8	10.323	98	194588	20.226	ug/L		0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	80.920%		
43) trans-1,3-Dichloroprop...	10.573	79	21625	20.248	ug/L		0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	81.000%		
47) 2-Hexanone-d5	10.921	63	19771	57.924	ug/L		0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	115.840%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84	43682	22.208	ug/L		0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	88.840%		
66) 1,2-Dichlorobenzene-d4	13.853	152	76669	21.949	ug/L		0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	87.800%		
Target Compounds							
13) Acetone	4.129	43	3174m	10.054	ug/L	Qvalue	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011422\
Data File : VW021917.D
Acq On : 14 Jan 2022 16:51
Operator : SY/VA
Sample : VIBLK590
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK590

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
Yesilyurt

01/17/2022
Supervised By :Mahesh
Dadoda

01/17/2022

