

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011422\
 Data File : VW021917.D
 Acq On : 14 Jan 2022 16:51
 Operator : SY/VA
 Sample : VIBLK590
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK590

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 01/17/2022
 Supervised By :Mahesh Dadoda 01/17/2022

Quant Time: Jan 17 00:47:43 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jan 17 00:44:09 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	145659	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.628	117	147079	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	84952	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	55487	20.495	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	82.000%		
7) Chloroethane-d5	2.885	69	40491	16.562	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	66.240%		
11) 1,1-Dichloroethene-d2	4.013	63	64425	15.073	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	60.280%		
21) 2-Butanone-d5	7.080	46	22224m	58.159	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	116.320%		
24) Chloroform-d	7.647	84	96631	20.535	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	82.160%		
26) 1,2-Dichloroethane-d4	8.305	65	50831	22.369	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	89.480%		
32) Benzene-d6	8.275	84	197968	20.744	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	82.960%		
36) 1,2-Dichloropropane-d6	9.268	67	52750	20.971	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	83.880%		
41) Toluene-d8	10.323	98	194588	20.226	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	80.920%		
43) trans-1,3-Dichloroprop...	10.573	79	21625	20.248	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	81.000%		
47) 2-Hexanone-d5	10.921	63	19771	57.924	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	115.840%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84	43682	22.208	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	88.840%		
66) 1,2-Dichlorobenzene-d4	13.853	152	76669	21.949	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	87.800%		
Target Compounds						Qvalue
13) Acetone	4.129	43	3174m	10.054	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011422\
Data File : VW021917.D
Acq On : 14 Jan 2022 16:51
Operator : SY/VA
Sample : VIBLK590
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
VIBLK590

Quant Time: Jan 17 00:47:43 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Jan 17 00:44:09 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 01/17/2022
Supervised By :Mahesh Dadoda 01/17/2022

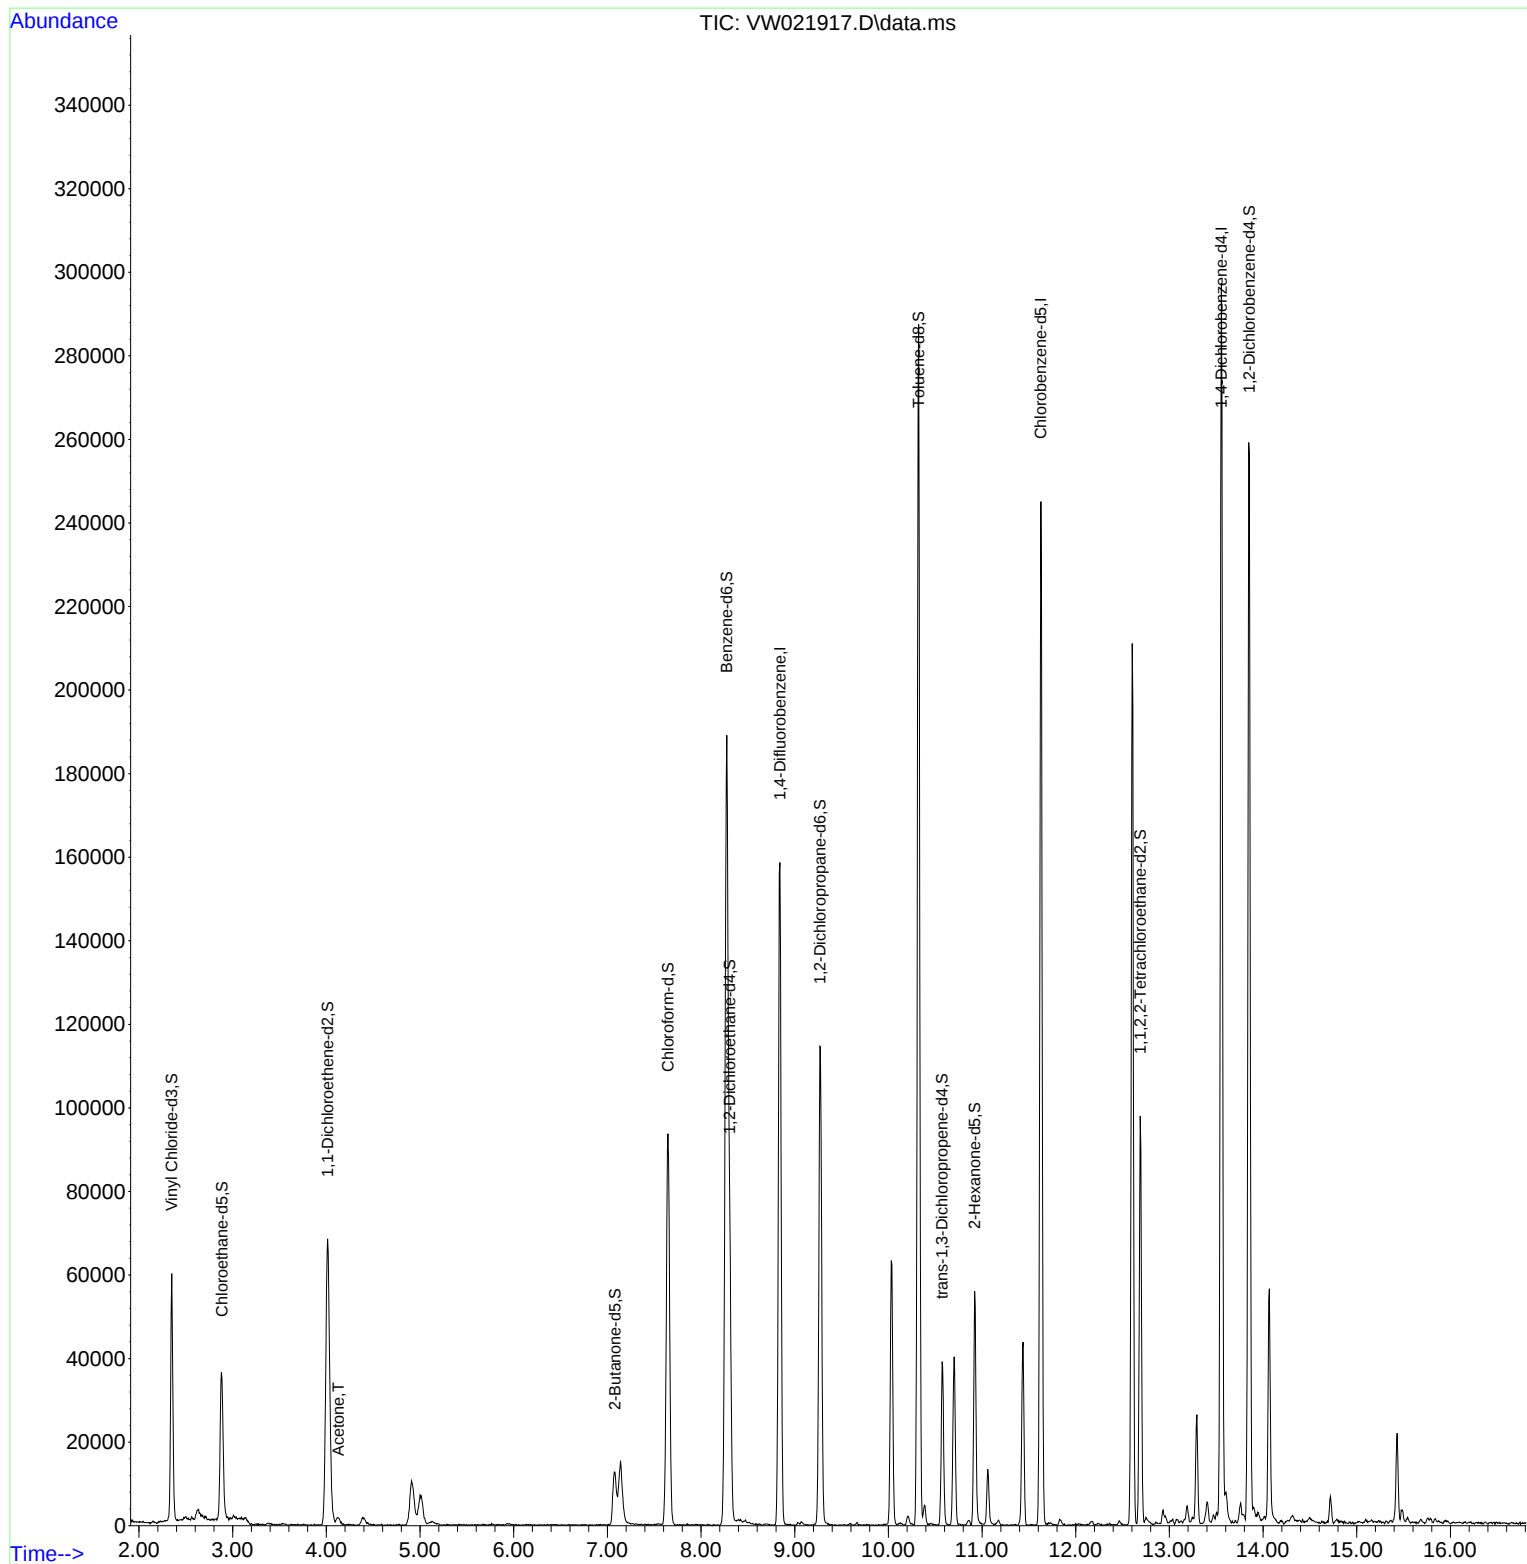

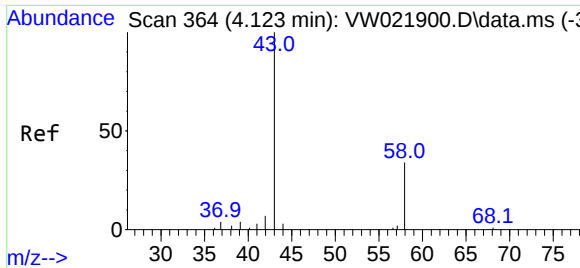

#13
 Acetone
 Concen: 10.054 ug/L m
 RT: 4.129 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW021917.D
 Acq: 14 Jan 2022 16:51

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK590

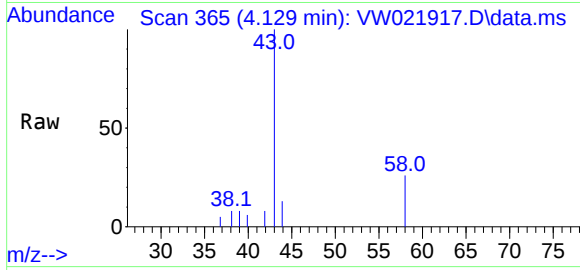

Tgt Ion: 43 Resp: 3174
 Ion Ratio Lower Upper
 43 100
 58 11.5 0.0 52.8

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 01/17/2022
 Supervised By :Mahesh Dadoda 01/17/2022

