

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW011520\
 Data File : VW014658.D
 Acq On : 15 Jan 2020 18:23
 Operator : SY/VA
 Sample : L1118-02
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GASJ5

Manual Integrations
 APPROVED

MMDadoda
 1/16/2020 5:41:41 PM

Quant Time: Jan 16 04:44:33 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122719S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 16 01:18:54 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	1301785	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	1137261	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	522451	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	383540	20.90	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.60%
7) Chloroethane-d5	2.89	69	300210	22.20	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.80%
10) 1,1-Dichloroethene-d2	4.01	63	549483	16.37	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	65.48%
20) 2-Butanone-d5	7.07	46	196983	45.11	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.22%
24) Chloroform-d	7.65	84	658686	21.99	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	87.96%
26) 1,2-Dichloroethane-d4	8.31	65	340601m	21.91	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	87.64%
29) Benzene-d6	8.27	84	1464659	24.22	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	96.88%
33) 1,2-Dichloropropane-d6	9.27	67	436482	24.00	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.00%
37) Toluene-d8	10.32	98	1331720	24.29	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	97.16%
38) trans-1,3-Dichloropropene-	10.57	79	173418	23.09	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	92.36%
39) 2-Hexanone-d5	10.92	63	156108	50.21	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	100.42%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	325049	23.81	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.24%
61) 1,2-Dichlorobenzene-d4	13.85	152	435662	25.31	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	101.24%

Target Compounds					Ovalue
13) Acetone	4.12	43	26028	4.305 ug/L	100

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW011520\
Data File : VW014658.D
Acq On : 15 Jan 2020 18:23
Operator : SY/VA
Sample : L1118-02
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
GASJ5

Manual Integrations
APPROVED

MMDadoda
1/16/2020 5:41:41 PM

Quant Time: Jan 16 04:44:33 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122719S.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 16 01:18:54 2020
Response via : Initial Calibration

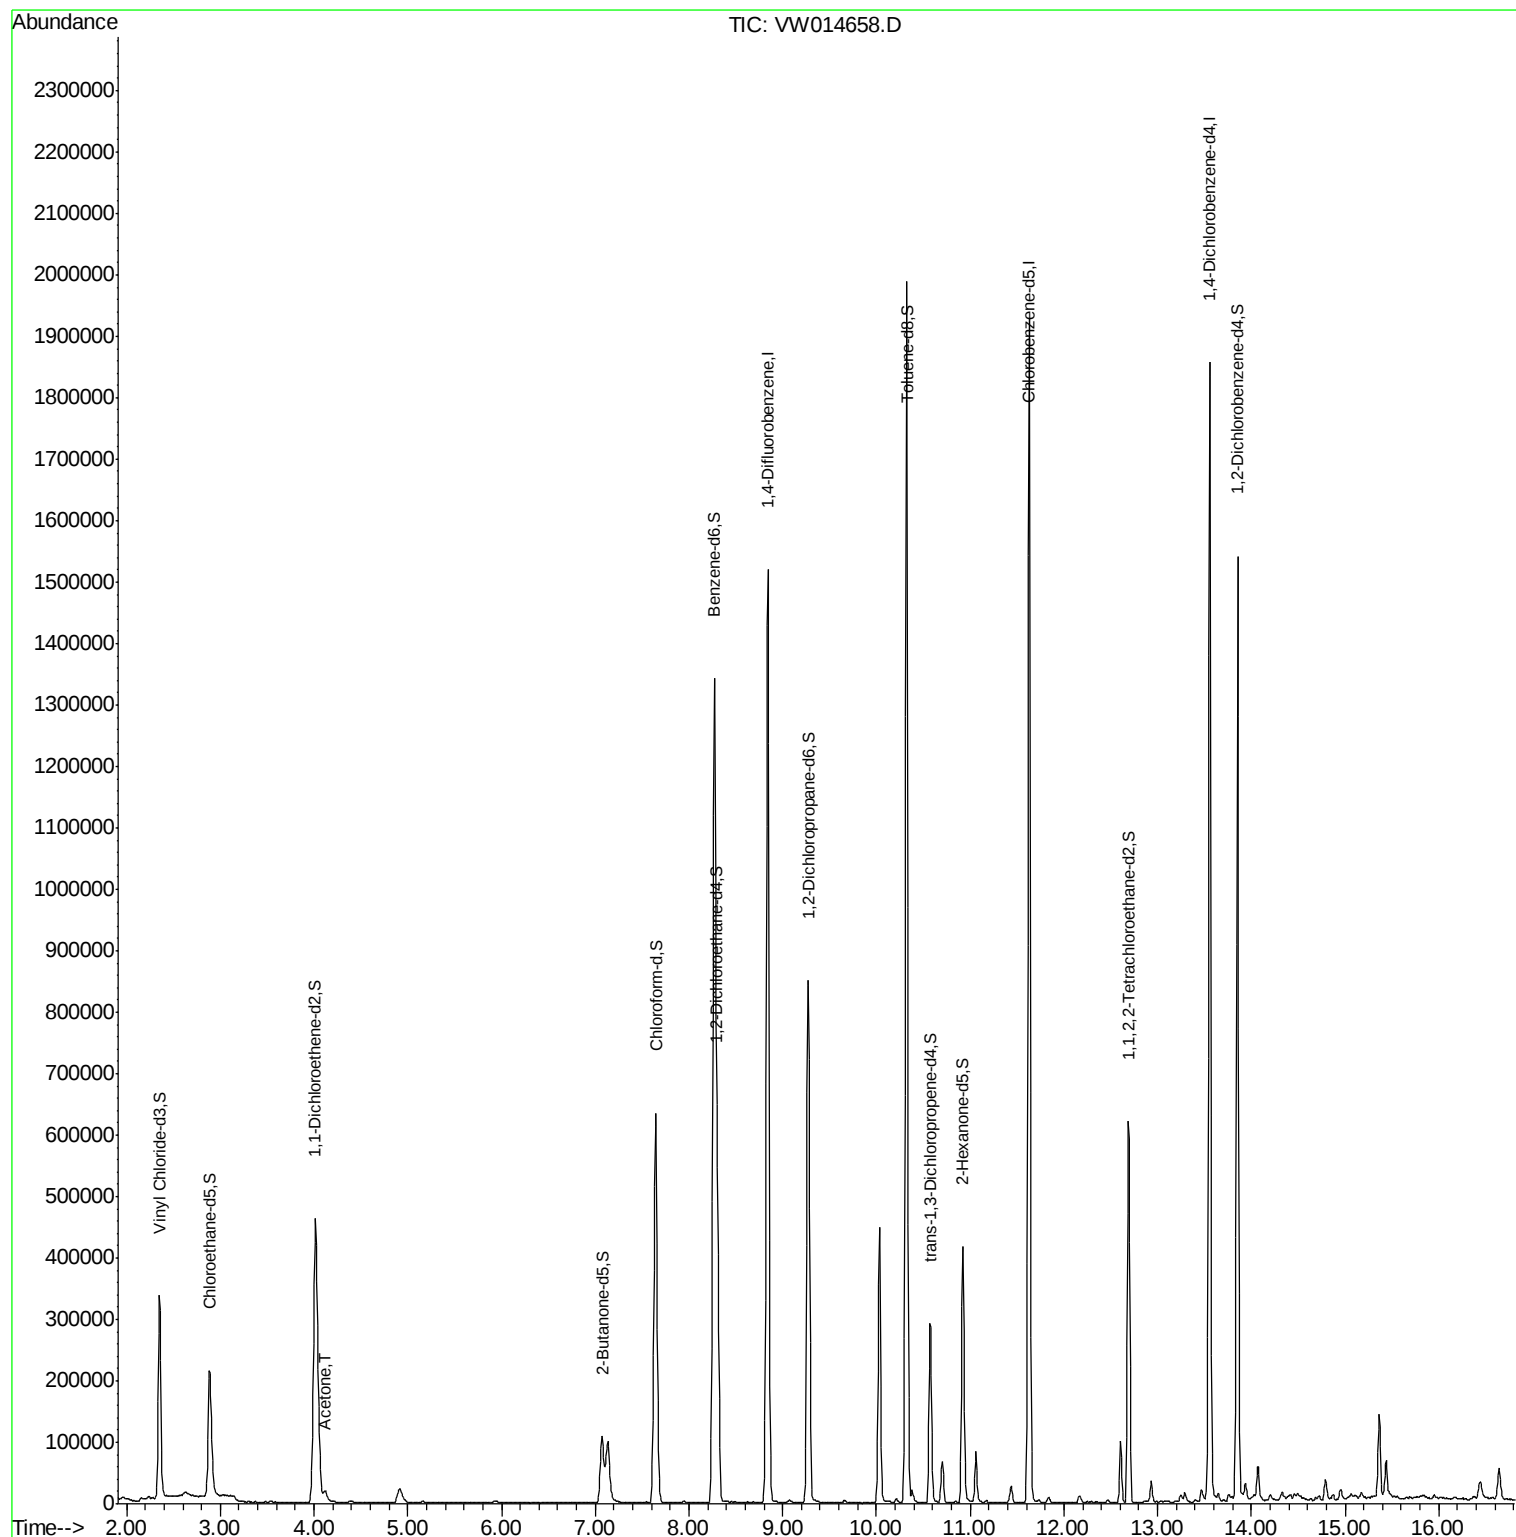

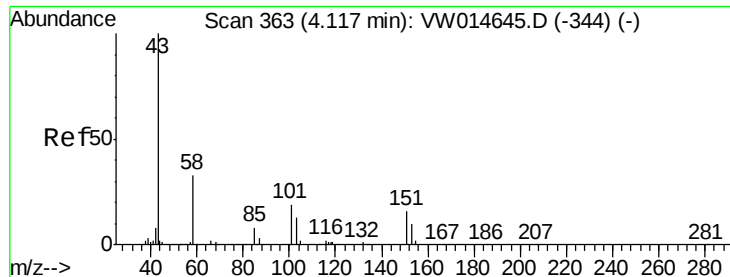

#13
 Acetone
 Concen: 4.305 ug/L
 RT: 4.12 min Scan# 364
 Delta R.T. 0.01 min
 Lab File: VW014658.D
 Acq: 15 Jan 2020 18:23

Instrument :
 MSVOA_W
 ClientSampleId :
 GASJ5

Tot Ion	Ratio	Lower	Upper
43	100		
58	32.3	0.0	64.0

Manual Integrations
 APPROVED

MMDadoda
 1/16/2020 5:41:41 PM

