




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011522\
Data File : VW021925.D
Acq On : 15 Jan 2022 00:07
Operator : SY/VA
Sample : N1155-08
Misc : 5.55g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLW2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/17/2022
Supervised By :Mahesh Dadoda 01/17/2022

Quant Time: Jan 17 03:24:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Jan 17 03:23:20 2022
Response via : Initial Calibration

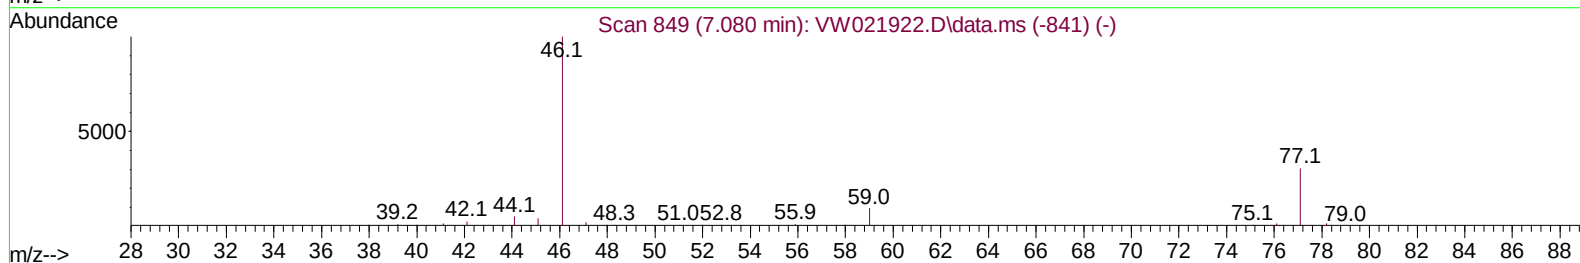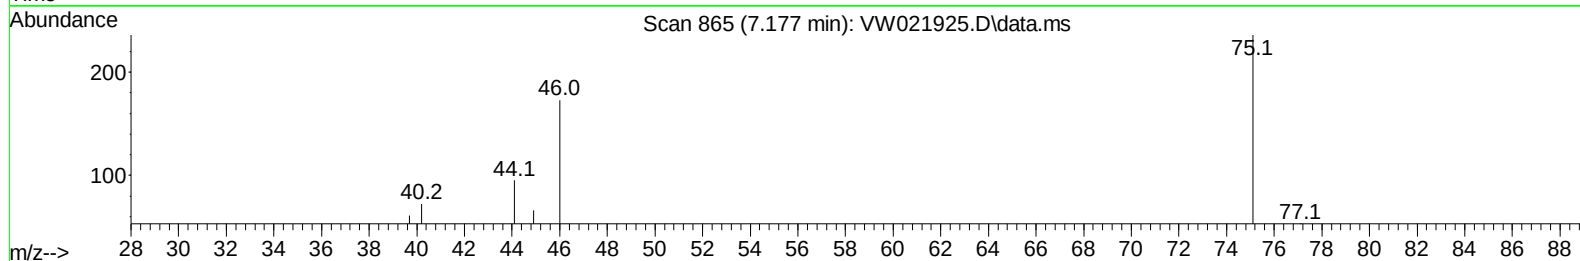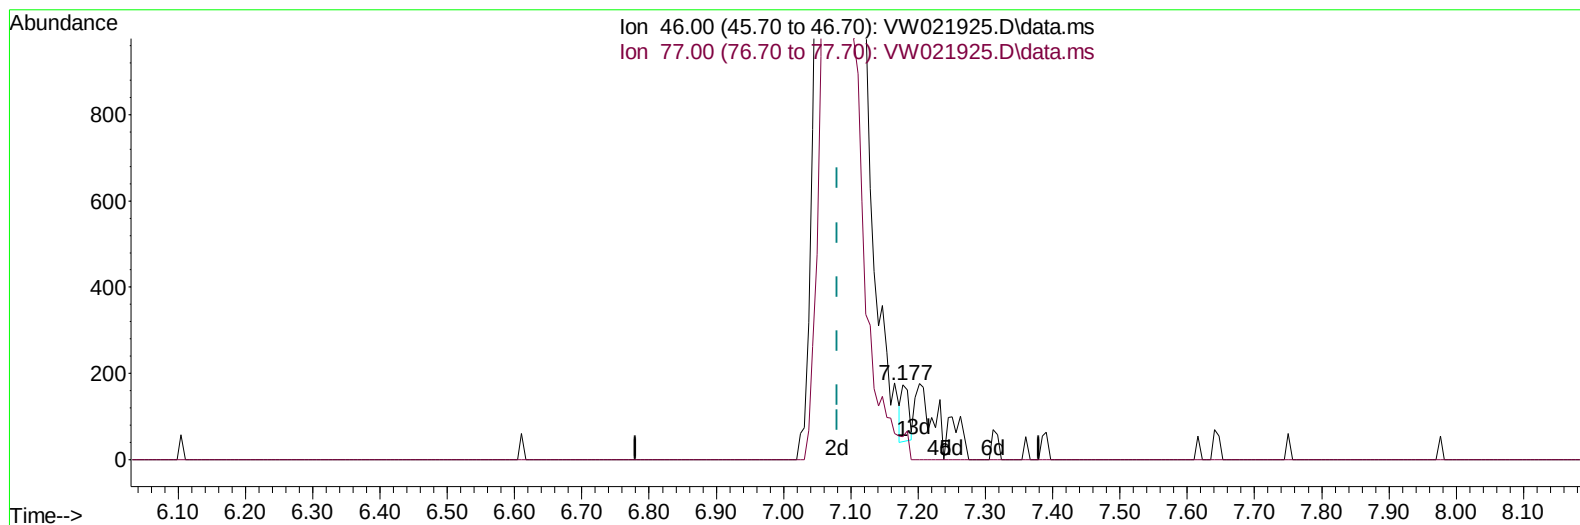

TIC: VW021925.D\data.ms

(21) 2-Butanone-d5 (S)

7.177min (+ 0.098) 0.22 ug/L

response 99

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	20.20	25.25
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011522\
 Data File : VW021925.D
 Acq On : 15 Jan 2022 00:07
 Operator : SY/VA
 Sample : N1155-08
 Misc : 5.55g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLW2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/17/2022
 Supervised By :Mahesh Dadoda 01/17/2022

Quant Time: Jan 17 03:24:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jan 17 03:23:20 2022
 Response via : Initial Calibration

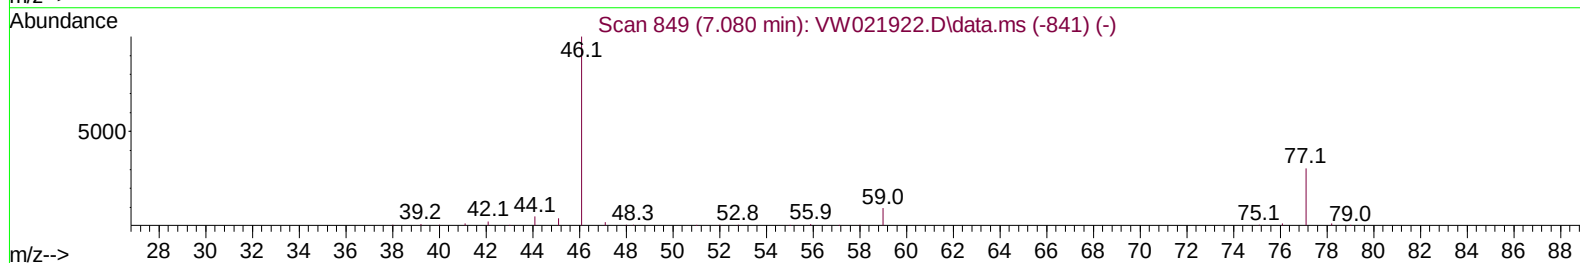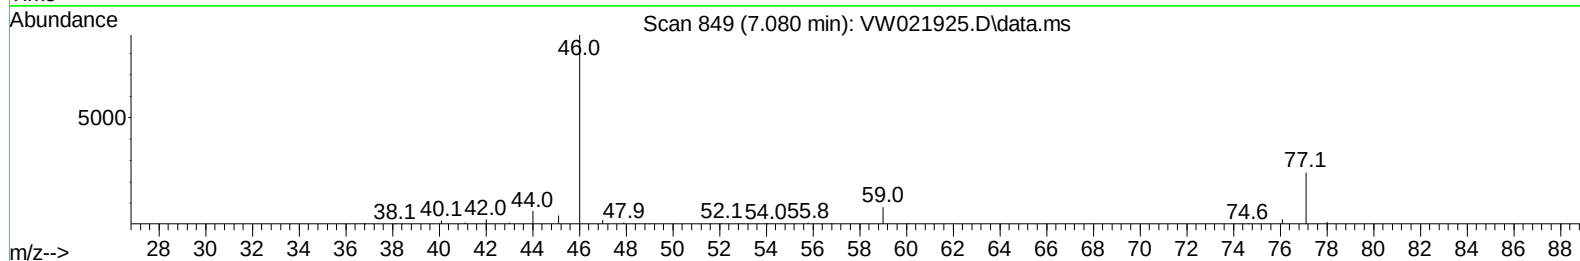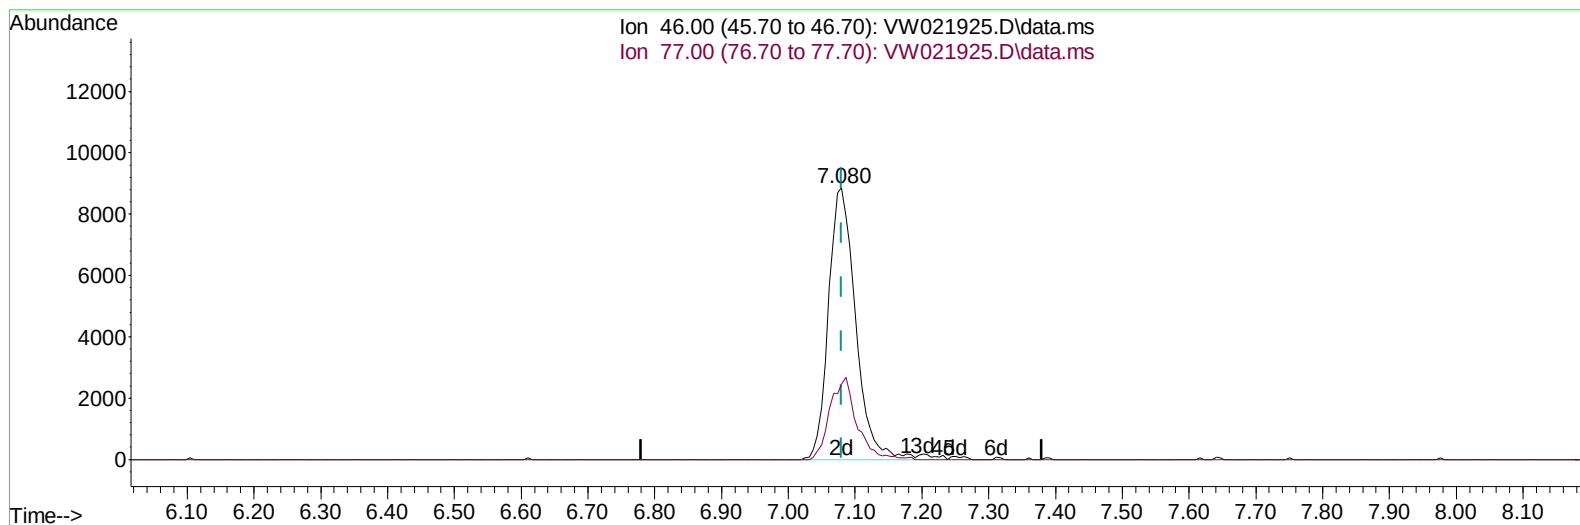

TIC: VW021925.D\data.ms

(21) 2-Butanone-d5 (S)

7.080min (+ 0.000) 56.21 ug/L m

response 24834

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	20.20	0.10#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011522\
 Data File : VW021925.D
 Acq On : 15 Jan 2022 00:07
 Operator : SY/VA
 Sample : N1155-08
 Misc : 5.55g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLW2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/17/2022
 Supervised By :Mahesh Dadoda 01/17/2022

Quant Time: Jan 17 03:24:18 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jan 17 03:23:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	168406	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.628	117	167269	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	95105	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	45935	14.675	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	58.720%	
7) Chloroethane-d5	2.879	69	35285	12.483	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	49.920%	
11) 1,1-Dichloroethene-d2	4.013	63	58285	11.795	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	47.160%	
21) 2-Butanone-d5	7.080	46	24834m	56.211	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	112.420%	
24) Chloroform-d	7.647	84	104136	19.141	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	76.560%	
26) 1,2-Dichloroethane-d4	8.305	65	55050	20.953	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	83.800%	
32) Benzene-d6	8.275	84	200831	18.504	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	74.000%	
36) 1,2-Dichloropropane-d6	9.275	67	57353	20.048	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	80.200%	
41) Toluene-d8	10.323	98	192813	17.623	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	70.480%	
43) trans-1,3-Dichloroprop...	10.579	79	22967	18.909	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	75.640%	
47) 2-Hexanone-d5	10.921	63	20737	53.421	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	106.840%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	51660	23.094	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	92.360%	
66) 1,2-Dichlorobenzene-d4	13.853	152	84262	21.547	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	86.200%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011522\
Data File : VW021925.D
Acq On : 15 Jan 2022 00:07
Operator : SY/VA
Sample : N1155-08
Misc : 5.55g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLW2

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 01/17/2022
Supervised By :Mahesh Dadoda 01/17/2022

Quant Time: Jan 17 03:24:18 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Jan 17 03:23:20 2022
Response via : Initial Calibration

