




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011522\
 Data File : VW021932.D
 Acq On : 15 Jan 2022 02:55
 Operator : SY/VA
 Sample : N1155-03
 Misc : 5.25g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLT6

Manual IntegrationsAPPROVED

Quant Time: Jan 17 03:25:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jan 17 03:23:20 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/17/2022
 Supervised By :Mahesh Dadoda 01/17/2022

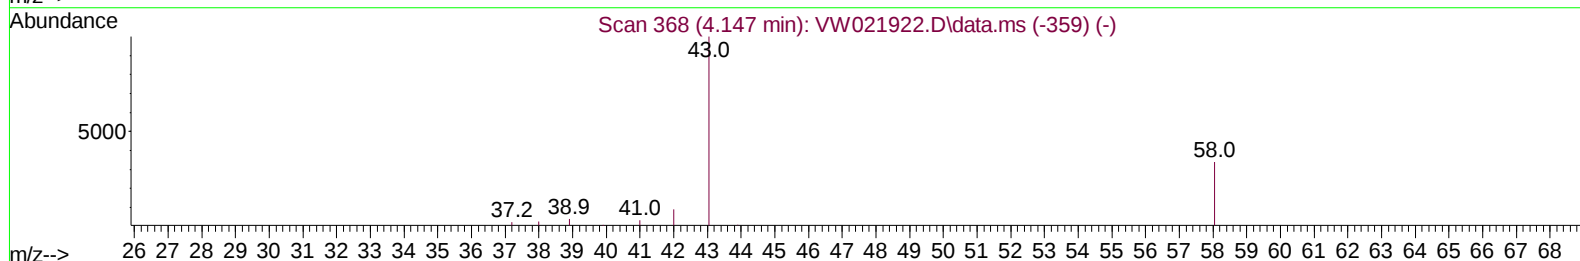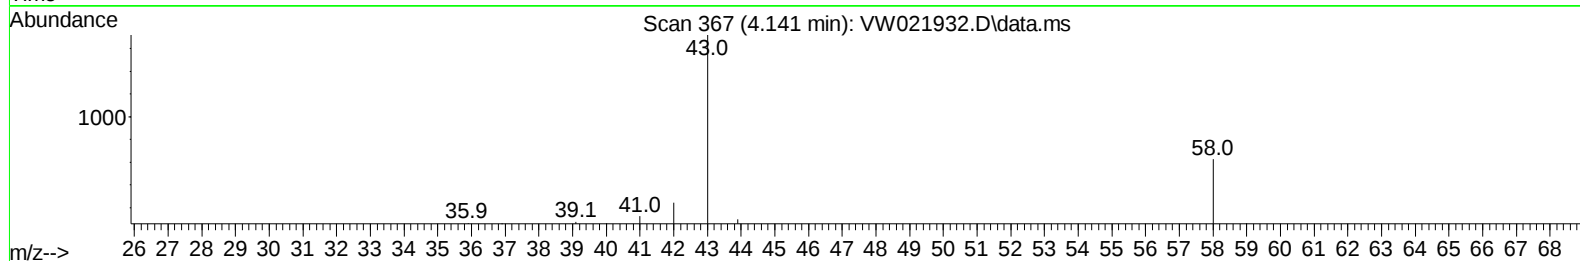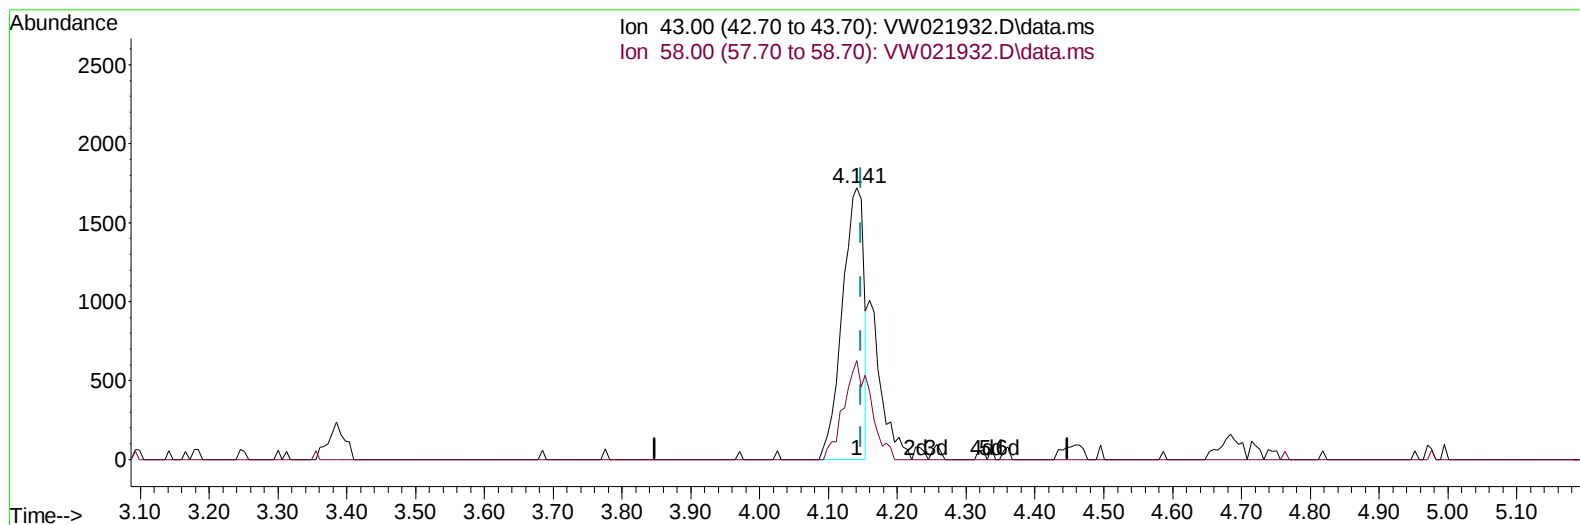

TIC: VW021932.D\data.ms

(13) Acetone (T)

4.141min (-0.006) 10.65 ug/L

response 3763

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.40	20.14
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011522\
 Data File : VW021932.D
 Acq On : 15 Jan 2022 02:55
 Operator : SY/VA
 Sample : N1155-03
 Misc : 5.25g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLT6

Manual IntegrationsAPPROVED

Quant Time: Jan 17 03:25:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jan 17 03:23:20 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/17/2022
 Supervised By :Mahesh Dadoda 01/17/2022

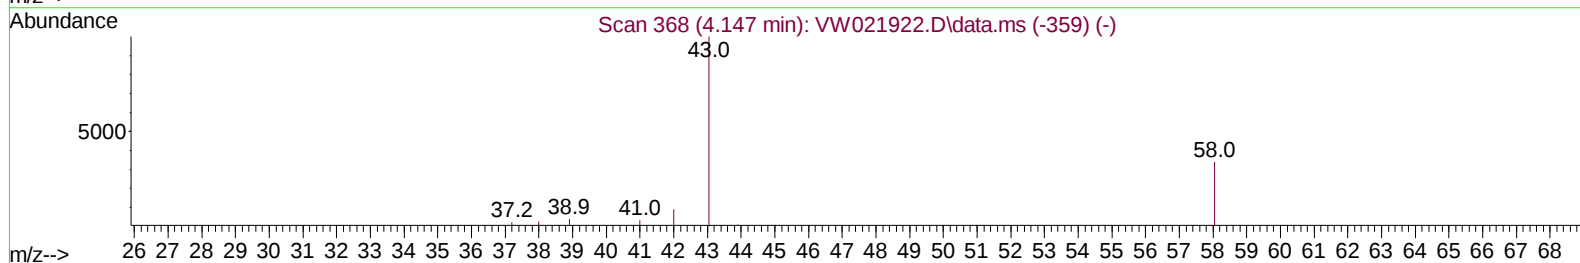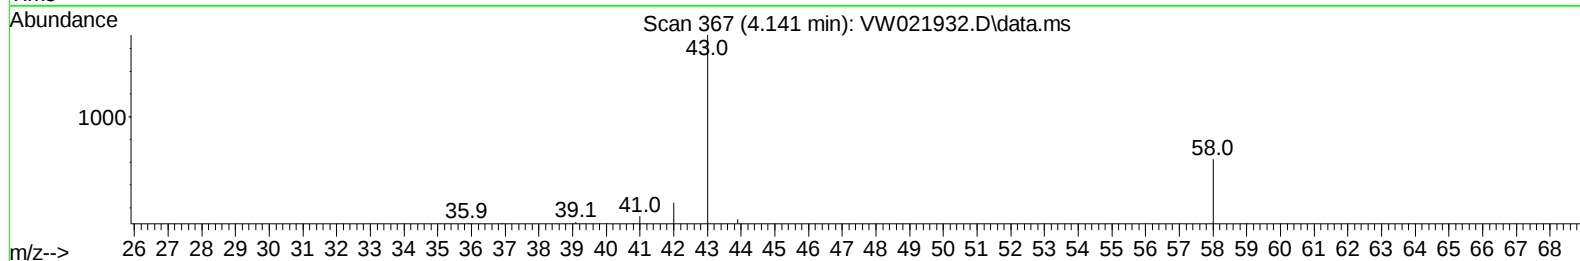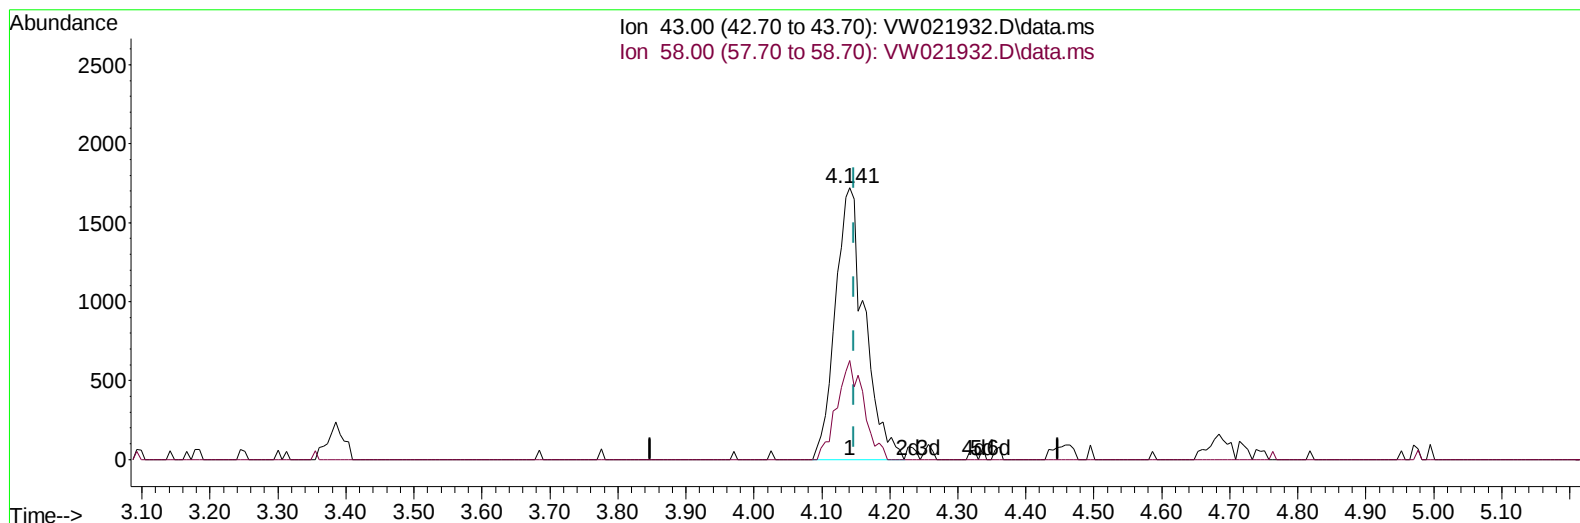

TIC: VW021932.D\data.ms

(13) Acetone (T)

4.141min (-0.006) 14.53 ug/L m

response 5134

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.40	14.76
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011522\
 Data File : VW021932.D
 Acq On : 15 Jan 2022 02:55
 Operator : SY/VA
 Sample : N1155-03
 Misc : 5.25g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLT6

Manual IntegrationsAPPROVED

Quant Time: Jan 17 03:25:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jan 17 03:23:20 2022
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/17/2022
 Supervised By :Mahesh Dadoda 01/17/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	163071	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.628	117	149926	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	77996	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	33775	11.143	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	44.560%	
7) Chloroethane-d5	2.885	69	35072	12.814	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	51.240%	
11) 1,1-Dichloroethene-d2	4.019	63	57637	12.045	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	48.200%	
21) 2-Butanone-d5	7.086	46	14311	33.452	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	66.900%	
24) Chloroform-d	7.653	84	100157	19.012	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	76.040%	
26) 1,2-Dichloroethane-d4	8.305	65	52533	20.650	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	82.600%	
32) Benzene-d6	8.275	84	188644	19.391	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	77.560%	
36) 1,2-Dichloropropane-d6	9.275	67	54149	21.118	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	84.480%	
41) Toluene-d8	10.323	98	170000	17.335	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	69.320%	
43) trans-1,3-Dichloroprop...	10.579	79	19426	17.844	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	71.360%	
47) 2-Hexanone-d5	10.921	63	12376	35.570	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	71.140%	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	44206	22.047	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	88.200%	
66) 1,2-Dichlorobenzene-d4	13.853	152	62206	19.396	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	77.600%	
Target Compounds						
13) Acetone	4.141	43	5134m	14.526	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011522\
Data File : VW021932.D
Acq On : 15 Jan 2022 02:55
Operator : SY/VA
Sample : N1155-03
Misc : 5.25g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGLT6

Manual IntegrationsAPPROVED

Quant Time: Jan 17 03:25:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Jan 17 03:23:20 2022
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 01/17/2022
Supervised By :Mahesh Dadoda 01/17/2022

