

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011522\
 Data File : VW021928.D
 Acq On : 15 Jan 2022 01:19
 Operator : SY/VA
 Sample : VIBLK591
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK591

Quant Time: Jan 17 03:24:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jan 17 03:23:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	127211	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.628	117	130416	25.000	ug/L	# 0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	71910	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	49761	21.046	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.200%
7) Chloroethane-d5	2.885	69	36001	16.861	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	67.440%
11) 1,1-Dichloroethene-d2	4.019	63	59837	16.030	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	64.120%
21) 2-Butanone-d5	7.080	46	21332	63.920	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	127.840%
24) Chloroform-d	7.647	84	94763	23.058	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.240%
26) 1,2-Dichloroethane-d4	8.305	65	50685	25.539	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	102.160%
32) Benzene-d6	8.275	84	188818	22.313	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	89.240%
36) 1,2-Dichloropropane-d6	9.275	67	51723	23.190	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.760%
41) Toluene-d8	10.323	98	179738	21.070	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	84.280%
43) trans-1,3-Dichloroprop...	10.579	79	20778	21.941	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	87.760%
47) 2-Hexanone-d5	10.921	63	18699	61.783	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	123.560%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	43879	25.158	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.640%
66) 1,2-Dichlorobenzene-d4	13.847	152	68703	23.235	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	92.960%
Target Compounds					Qvalue	
13) Acetone	4.129	43	1380	5.005	ug/L	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011522\
Data File : VW021928.D
Acq On : 15 Jan 2022 01:19
Operator : SY/VA
Sample : VIBLK591
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK591

Quant Time: Jan 17 03:24:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Jan 17 03:23:20 2022
Response via : Initial Calibration

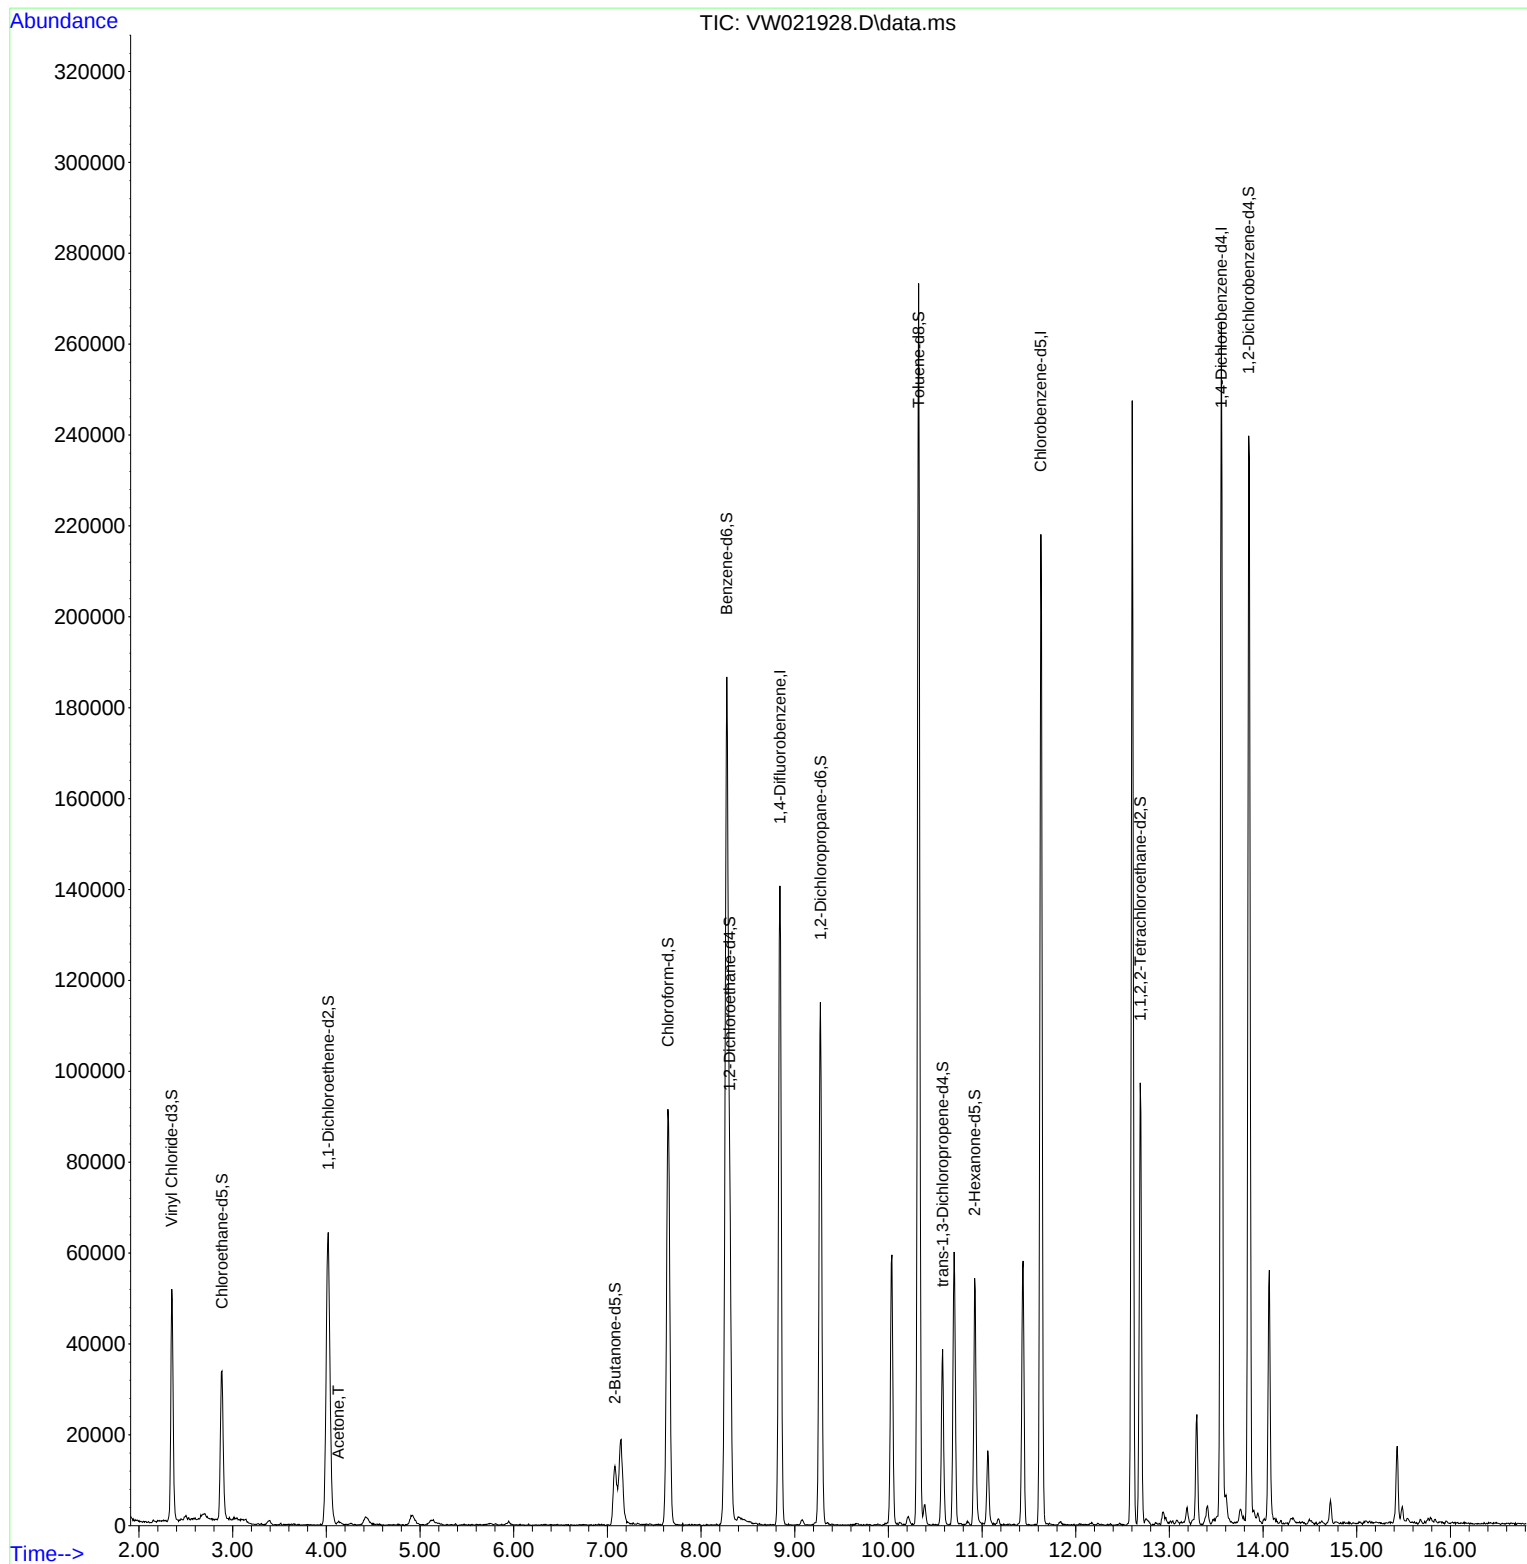

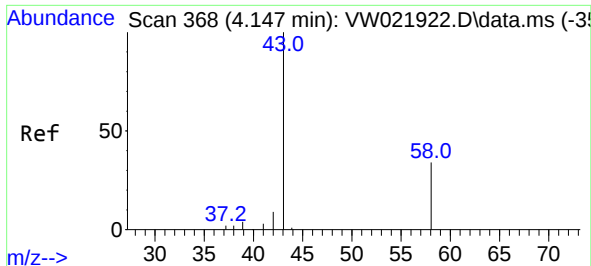

#13
 Acetone
 Concen: 5.005 ug/L
 RT: 4.129 min Scan# 3
 Delta R.T. -0.018 min
 Lab File: VW021928.D
 Acq: 15 Jan 2022 01:19

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK591

Tgt Ion: 43 Resp: 1380
 Ion Ratio Lower Upper
 43 100
 58 15.1 0.0 52.8

