

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011522\
 Data File : VW021931.D
 Acq On : 15 Jan 2022 02:31
 Operator : SY/VA
 Sample : N1155-12
 Misc : 7.03g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLW6

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 01/17/2022
 Supervised By :Mahesh Dadoda 01/17/2022

Quant Time: Jan 17 03:25:22 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jan 17 03:23:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	152813	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.628	117	152500	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	81630	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	41139	14.484	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	57.920%		
7) Chloroethane-d5	2.879	69	33149	12.924	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	51.680%		
11) 1,1-Dichloroethene-d2	4.019	63	53192	11.862	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	47.440%		
21) 2-Butanone-d5	7.080	46	19285	48.105	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	96.220%		
24) Chloroform-d	7.647	84	96489	19.545	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	78.160%		
26) 1,2-Dichloroethane-d4	8.305	65	49213	20.643	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	82.560%		
32) Benzene-d6	8.275	84	184155	18.610	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	74.440%		
36) 1,2-Dichloropropane-d6	9.274	67	51871	19.888	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	79.560%		
41) Toluene-d8	10.323	98	175694	17.613	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	70.440%		
43) trans-1,3-Dichloroprop...	10.579	79	19573	17.675	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	70.720%		
47) 2-Hexanone-d5	10.920	63	16306	46.075	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	92.140%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	43016	21.092	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	84.360%		
66) 1,2-Dichlorobenzene-d4	13.847	152	68151	20.304	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	81.200%		
Target Compounds					Qvalue	
13) Acetone	4.129	43	2124m	6.413	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011522\
Data File : VW021931.D
Acq On : 15 Jan 2022 02:31
Operator : SY/VA
Sample : N1155-12
Misc : 7.03g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
BGLW6

Quant Time: Jan 17 03:25:22 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Jan 17 03:23:20 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 01/17/2022
Supervised By :Mahesh Dadoda 01/17/2022

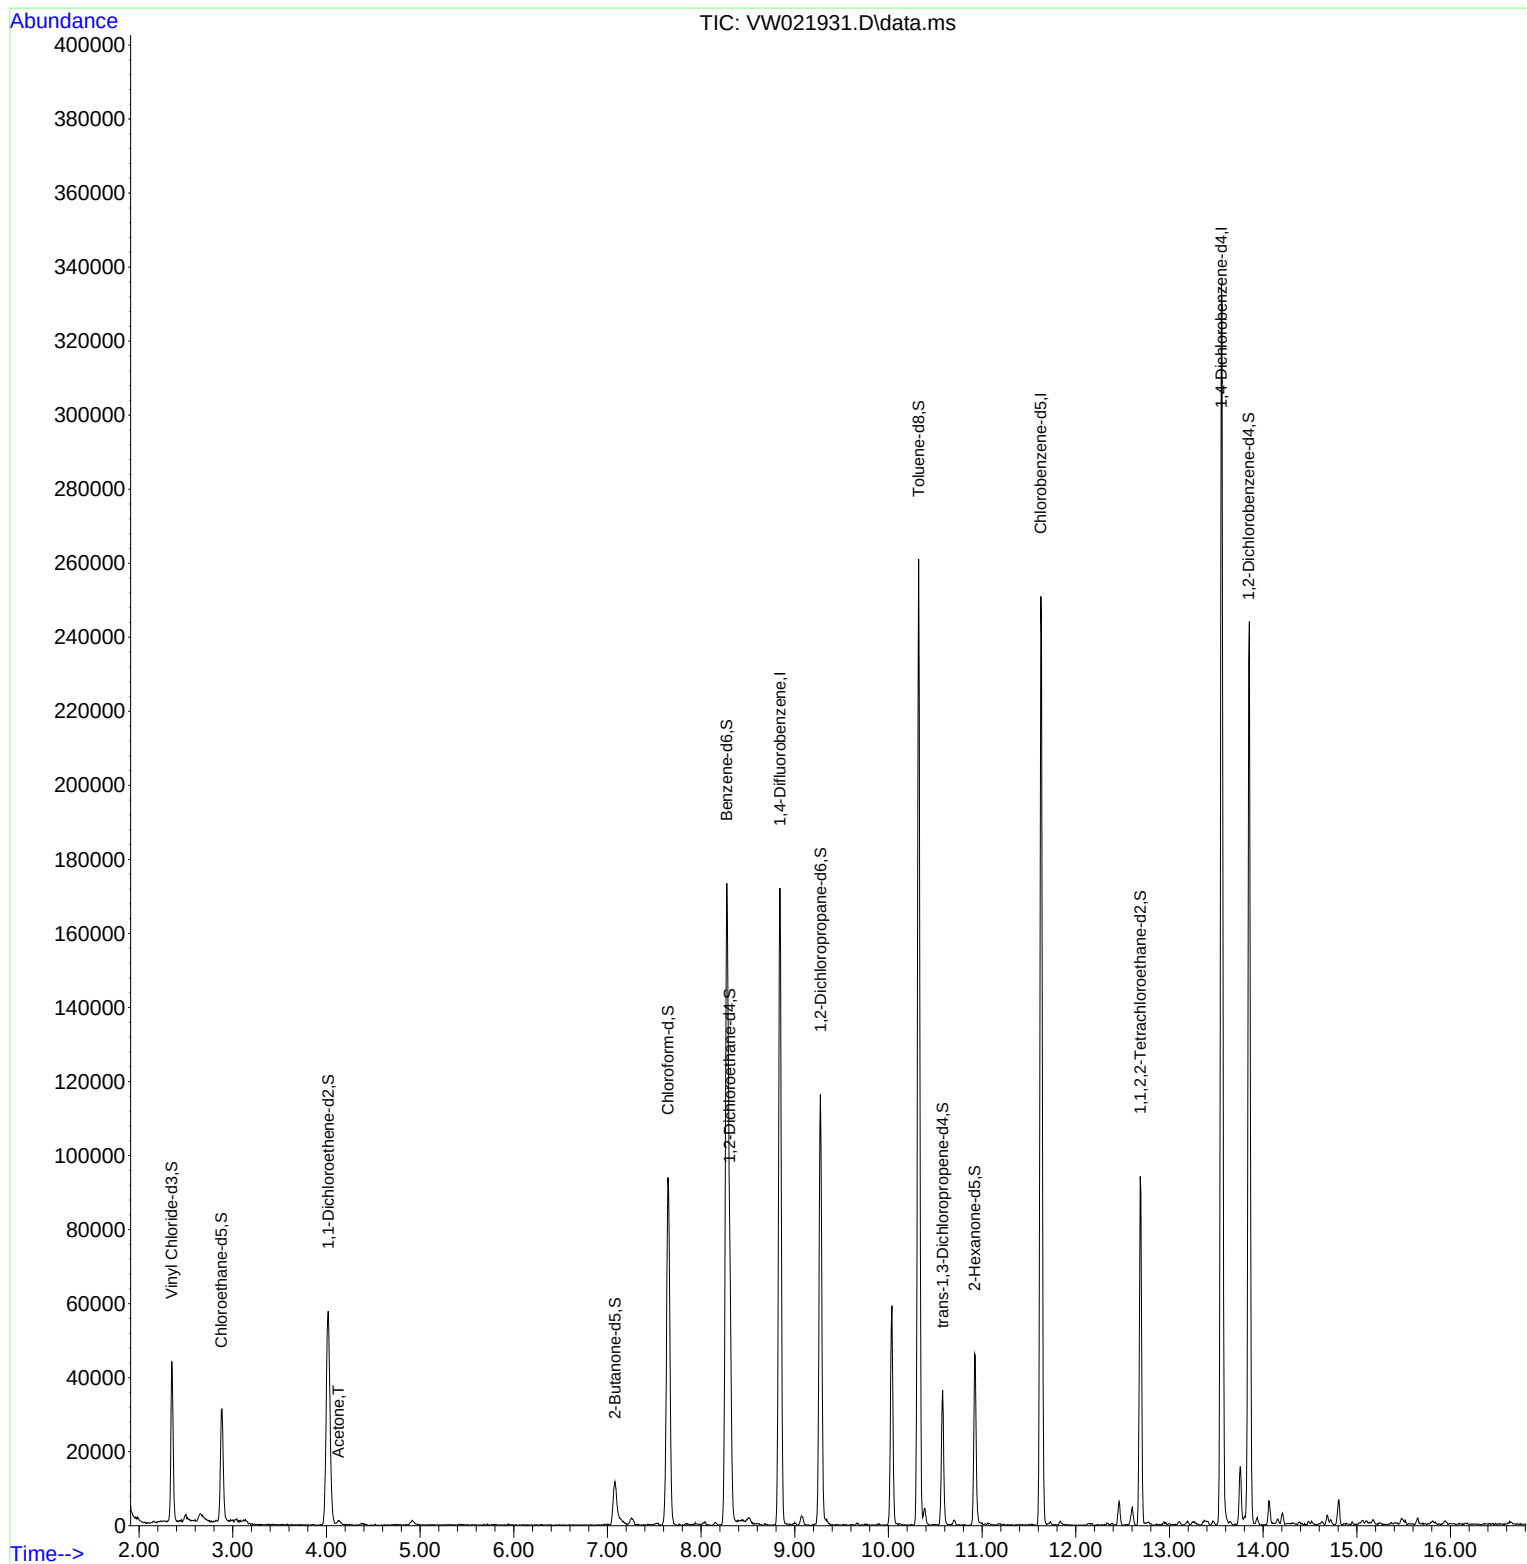

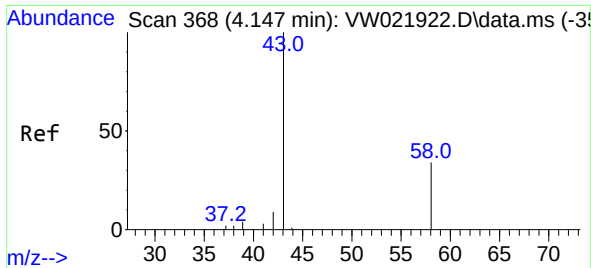

#13
 Acetone
 Concen: 6.413 ug/L m
 RT: 4.129 min Scan# 30
 Delta R.T. -0.019 min
 Lab File: VW021931.D
 Acq: 15 Jan 2022 02:31

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLW6

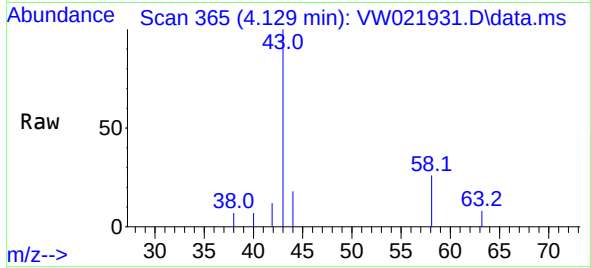

Tgt Ion: 43 Resp: 2124

Ion	Ratio	Lower	Upper
43	100		
58	25.3	0.0	52.8

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 01/17/2022
 Supervised By :Mahesh Dadoda 01/17/2022

