

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011522\
 Data File : VW021932.D
 Acq On : 15 Jan 2022 02:55
 Operator : SY/VA
 Sample : N1155-03
 Misc : 5.25g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLT6

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 01/17/2022
 Supervised By :Mahesh Dadoda 01/17/2022

Quant Time: Jan 17 03:25:32 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
 Quant Title : SFAM01.0
 QLast Update : Mon Jan 17 03:23:20 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	163071	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.628	117	149926	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	77996	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	33775	11.143	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	44.560%		
7) Chloroethane-d5	2.885	69	35072	12.814	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	51.240%		
11) 1,1-Dichloroethene-d2	4.019	63	57637	12.045	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	48.200%		
21) 2-Butanone-d5	7.086	46	14311	33.452	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	66.900%		
24) Chloroform-d	7.653	84	100157	19.012	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	76.040%		
26) 1,2-Dichloroethane-d4	8.305	65	52533	20.650	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	82.600%		
32) Benzene-d6	8.275	84	188644	19.391	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	77.560%		
36) 1,2-Dichloropropane-d6	9.275	67	54149	21.118	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	84.480%		
41) Toluene-d8	10.323	98	170000	17.335	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	69.320%		
43) trans-1,3-Dichloroprop...	10.579	79	19426	17.844	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	71.360%		
47) 2-Hexanone-d5	10.921	63	12376	35.570	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	71.140%		
56) 1,1,2,2-Tetrachloroeth...	12.689	84	44206	22.047	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	88.200%		
66) 1,2-Dichlorobenzene-d4	13.853	152	62206	19.396	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	77.600%		
Target Compounds					Qvalue	
13) Acetone	4.141	43	5134m	14.526	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011522\
Data File : VW021932.D
Acq On : 15 Jan 2022 02:55
Operator : SY/VA
Sample : N1155-03
Misc : 5.25g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
BGLT6

Quant Time: Jan 17 03:25:32 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011122SMA.M
Quant Title : SFAM01.0
QLast Update : Mon Jan 17 03:23:20 2022
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 01/17/2022
Supervised By :Mahesh Dadoda 01/17/2022

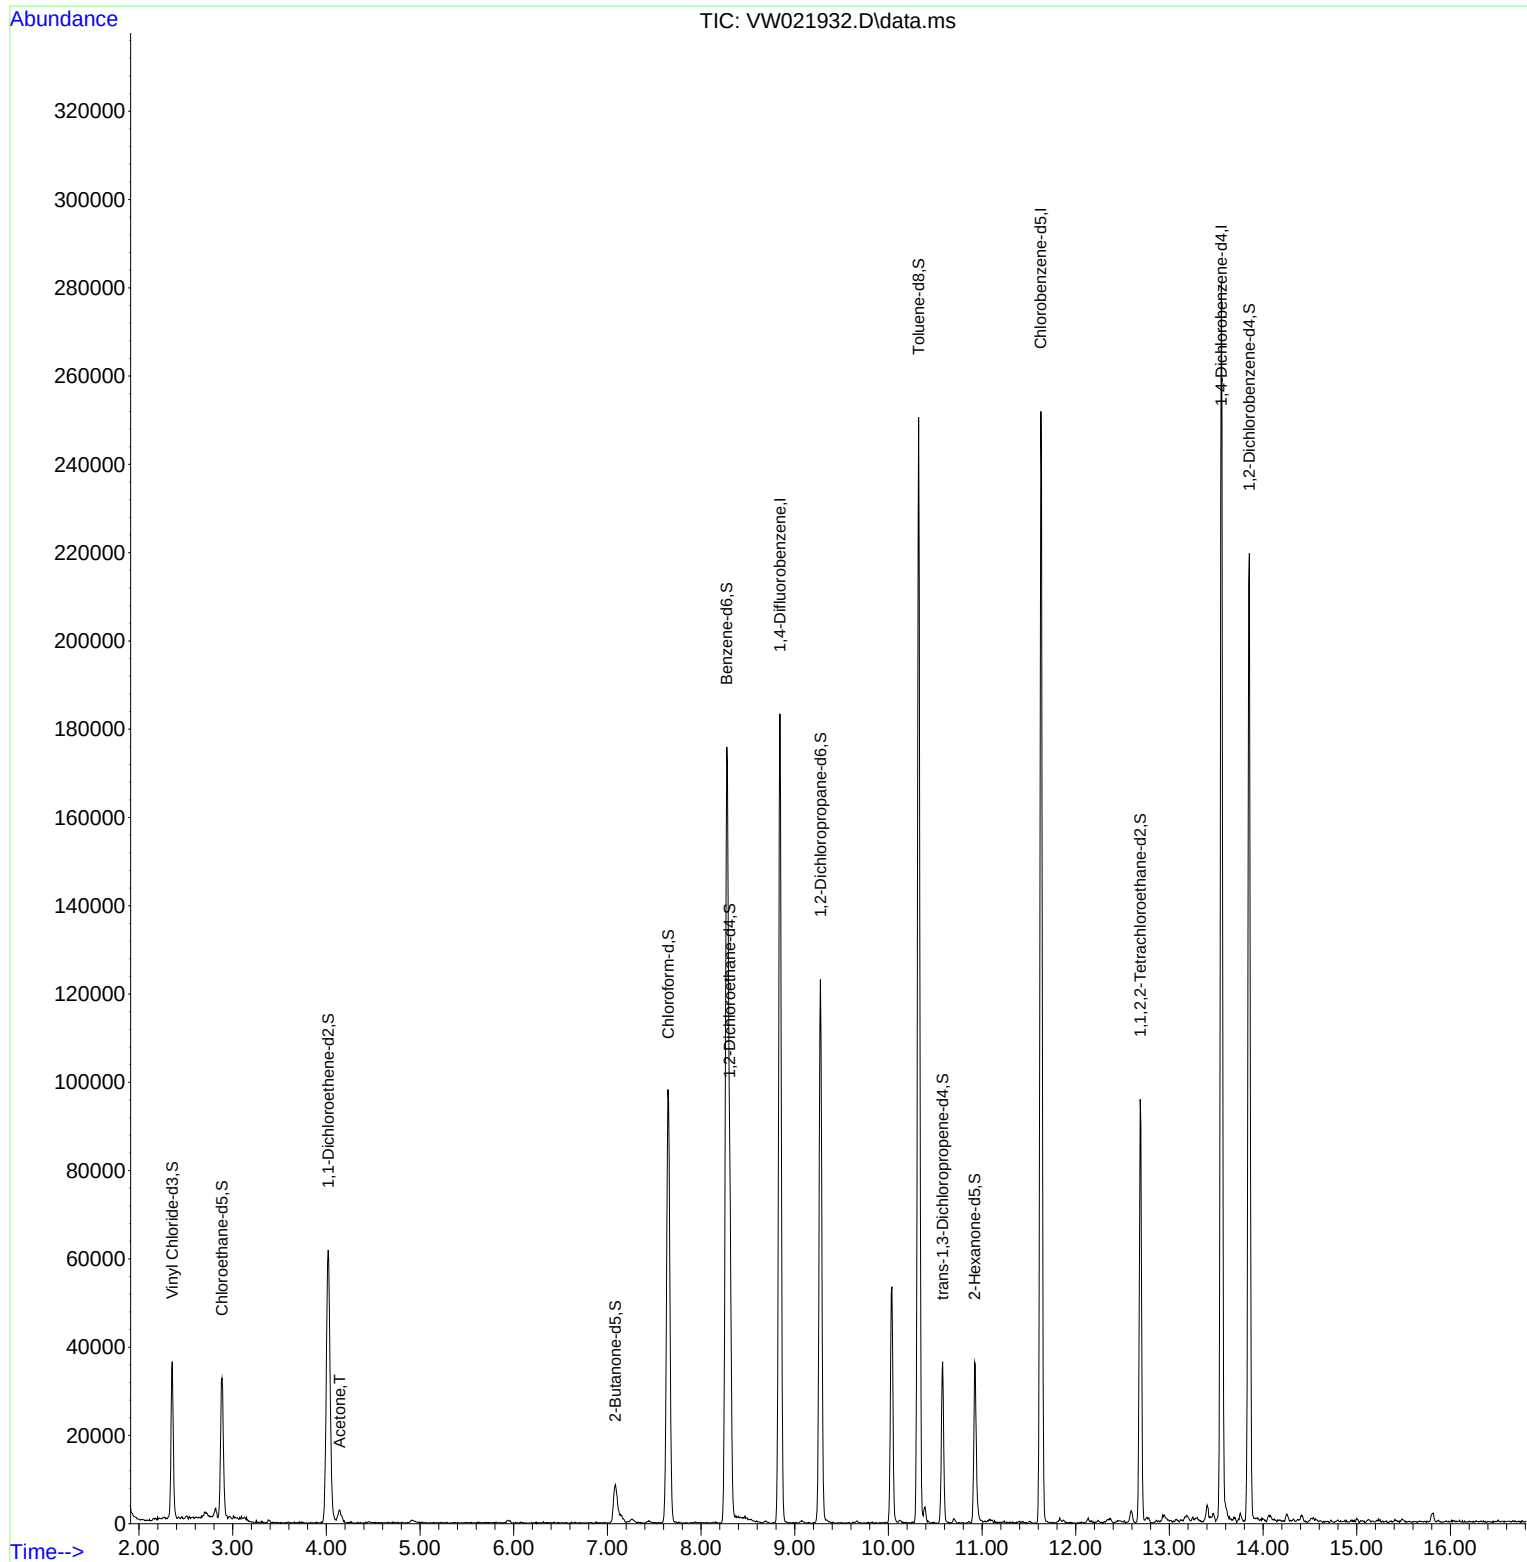

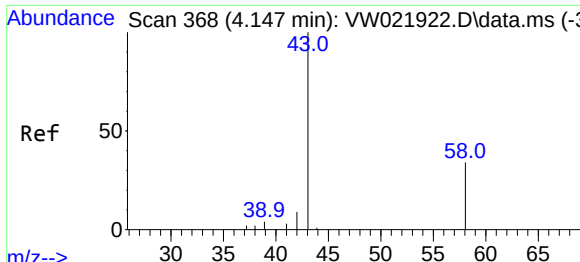

#13
 Acetone
 Concen: 14.526 ug/L m
 RT: 4.141 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: VW021932.D
 Acq: 15 Jan 2022 02:55

Instrument :
 MSVOA_W
 ClientSampleId :
 BGLT6

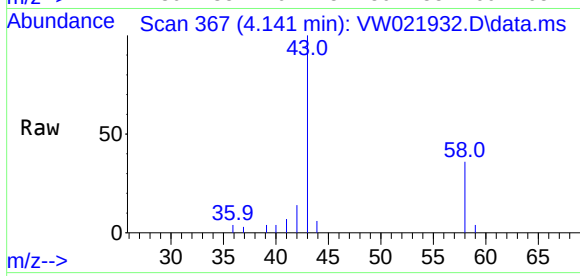

Tgt Ion: 43 Resp: 5134

Ion	Ratio	Lower	Upper
43	100		
58	14.8	0.0	52.8

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 01/17/2022
 Supervised By :Mahesh Dadoda 01/17/2022

