

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW011619\
 Data File : VW008301.D
 Acq On : 16 Jan 2019 11:53
 Operator : SY/VA
 Sample : VW0116SBL01
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VW0116SBL01

Quant Time: Jan 17 05:42:05 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W010819S.M
 Quant Title : SW846 8260
 QLast Update : Wed Jan 09 04:40:48 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	86585	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	158763	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	145670	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	64897	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.30	65	51031	52.44	ug/l	0.00
Spiked Amount	50.000		Recovery	=	104.88%	
35) Dibromofluoromethane	7.88	113	50285	54.31	ug/l	0.00
Spiked Amount	50.000		Recovery	=	108.62%	
50) Toluene-d8	10.32	98	199698	51.39	ug/l	0.00
Spiked Amount	50.000		Recovery	=	102.78%	
62) 4-Bromofluorobenzene	12.62	95	67108	48.17	ug/l	0.00
Spiked Amount	50.000		Recovery	=	96.34%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW011619\
Data File : VW008301.D
Acq On : 16 Jan 2019 11:53
Operator : SY/VA
Sample : VW0116SBL01
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VW0116SBL01

Quant Time: Jan 17 05:42:05 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W010819S.M
Quant Title : SW846 8260
QLast Update : Wed Jan 09 04:40:48 2019
Response via : Initial Calibration

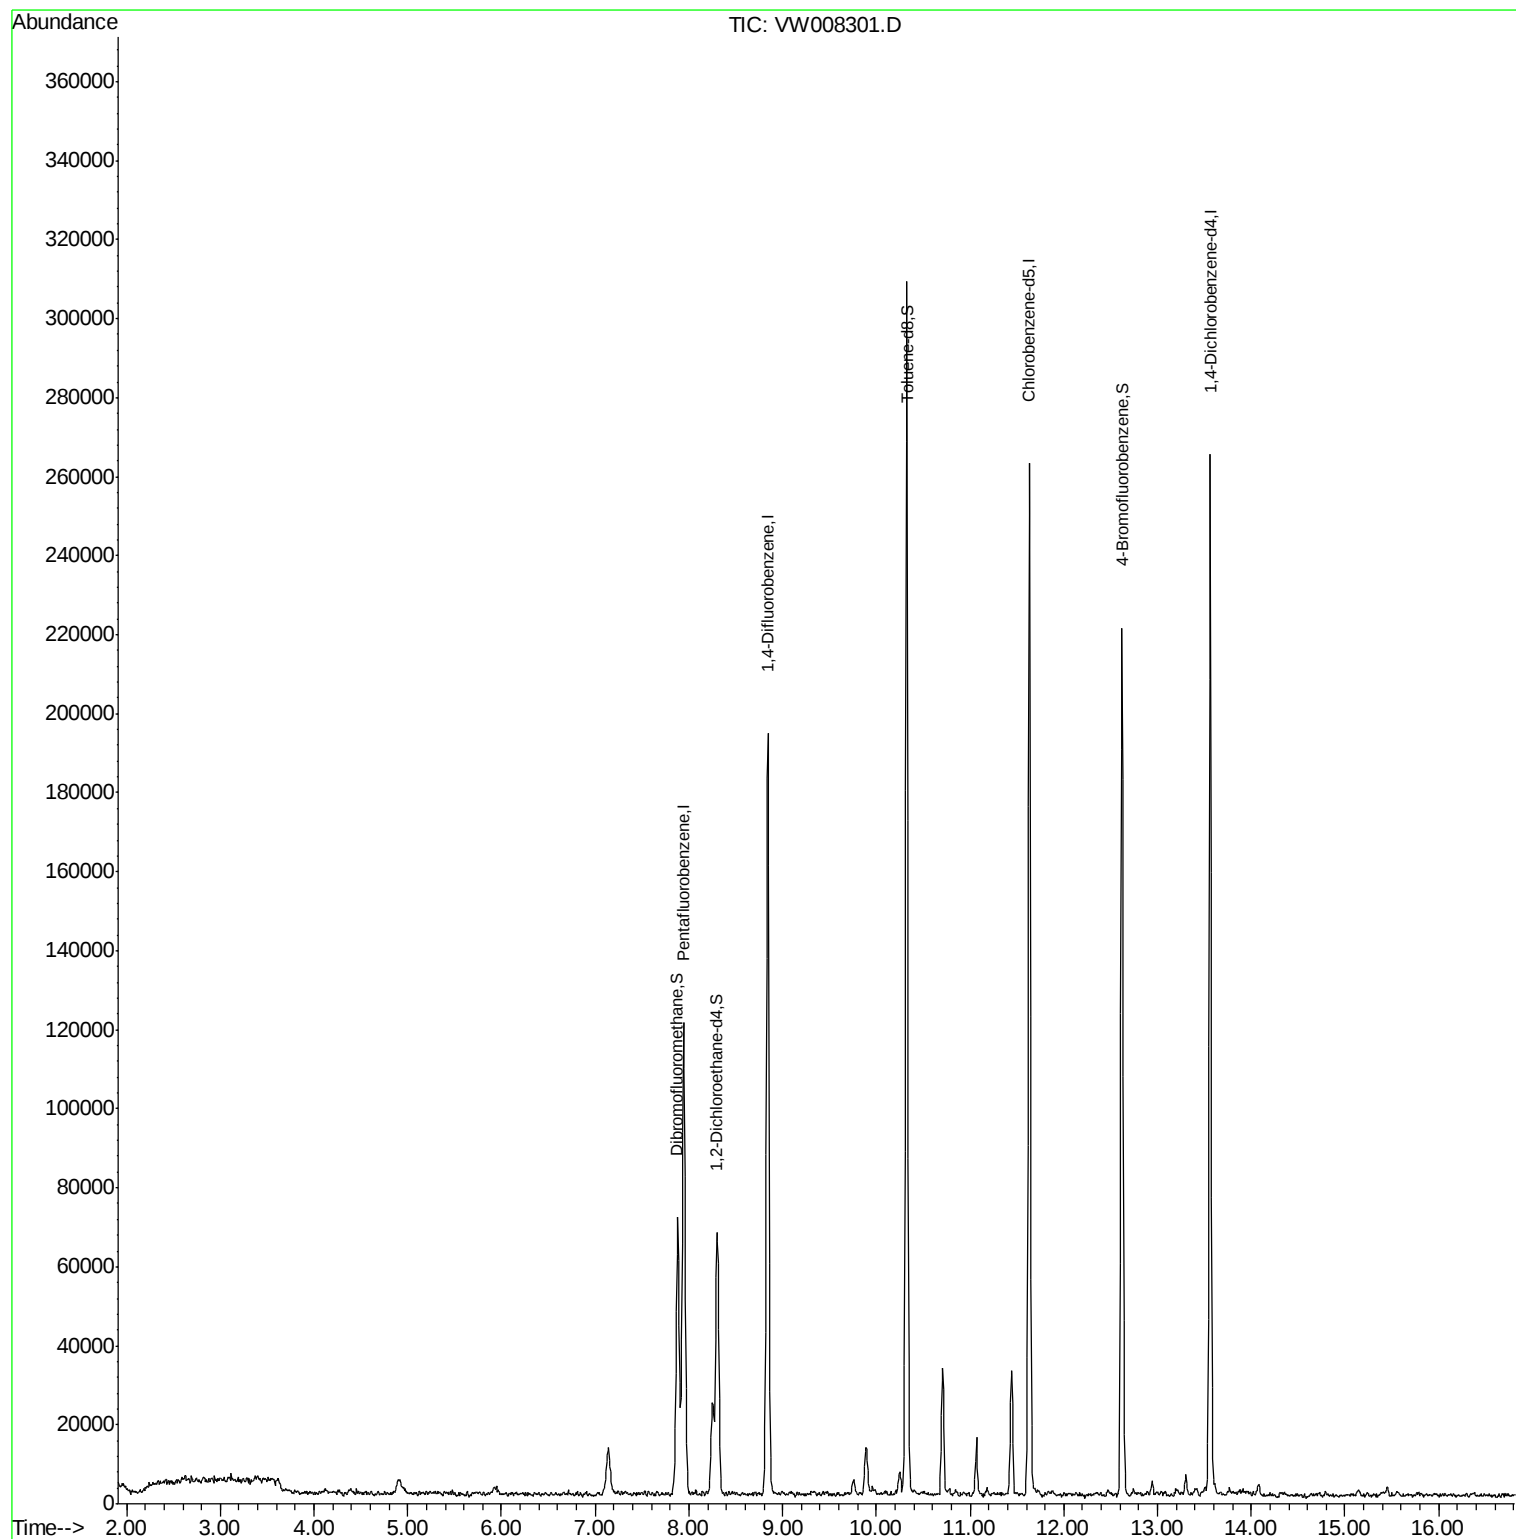

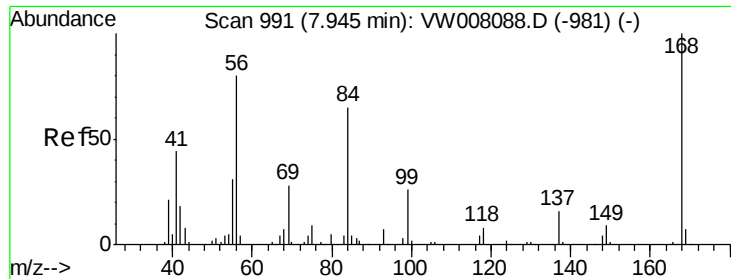

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 991

Delta R.T. 0.00 min

Lab File: VW008301.D

Acq: 16 Jan 2019 11:53

Instrument :

MSVOA_W

ClientSampleId :


VW0116SBL01

Tot Ion:168 Resp: 86585

Ion Ratio Lower Upper




168 100

99 60.9 52.6 78.8

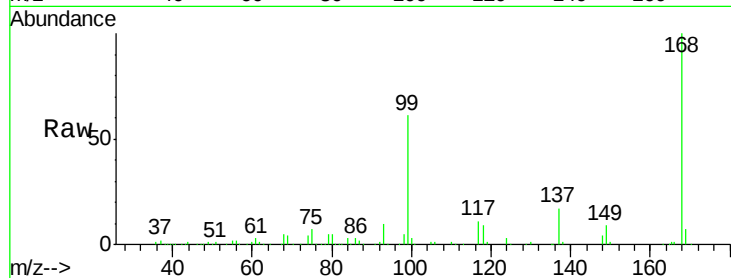

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

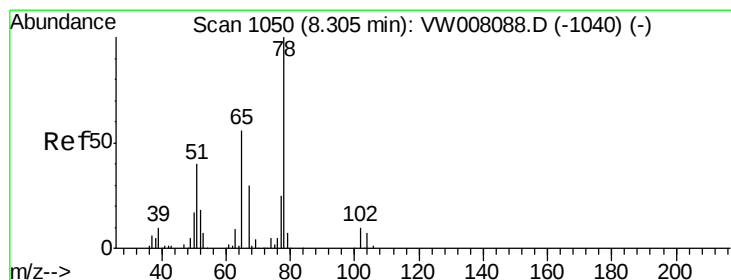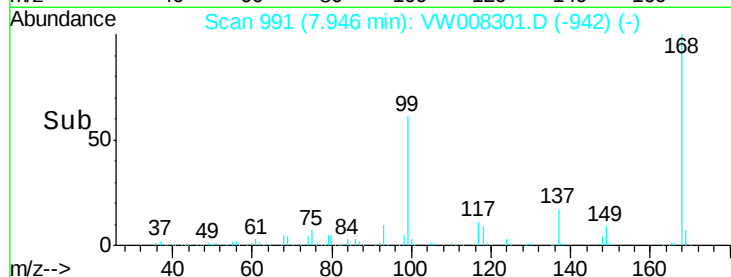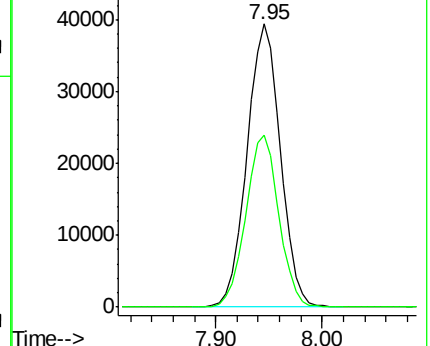

#33

1,2-Dichloroethane-d4

Concen: 52.440 ug/l

RT: 8.30 min Scan# 1049

Delta R.T. -0.01 min

Lab File: VW008301.D


Acq: 16 Jan 2019 11:53

Tgt Ion: 65 Resp: 51031

Ion Ratio Lower Upper



65 100


67 54.2 0.0 106.8

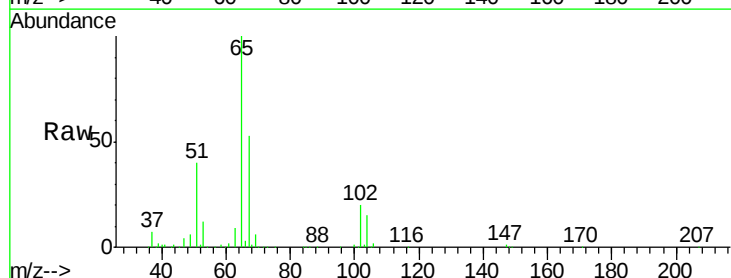

Abundance Ion 64.90 (64.60 to 65.60): VW

Ion 66.90 (66.60 to 67.60): VW

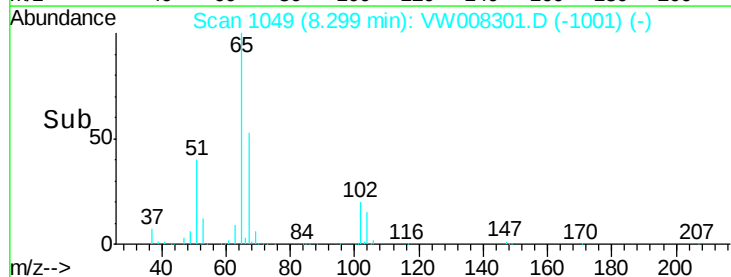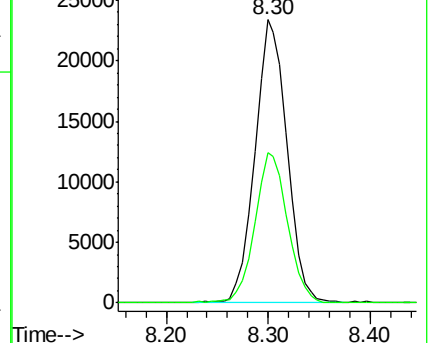


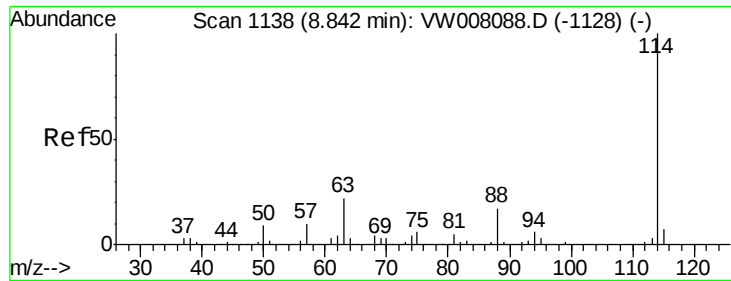




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.84 min Scan# 1138
 Delta R.T. 0.00 min
 Lab File: VW008301.D
 Acq: 16 Jan 2019 11:53

Instrument :
 MSVOA_W
 ClientSampleId :
 VW0116SBL01

Tot Ion:114 Resp: 158763
 Ion Ratio Lower Upper
 114 100
 63 21.5 0.0 43.4
 88 16.2 0.0 33.4

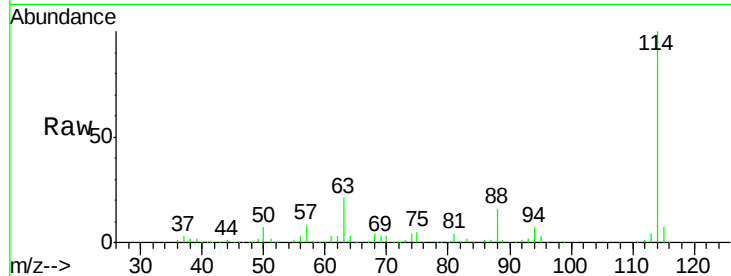


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VW
 Ion 87.90 (87.60 to 88.60): VW

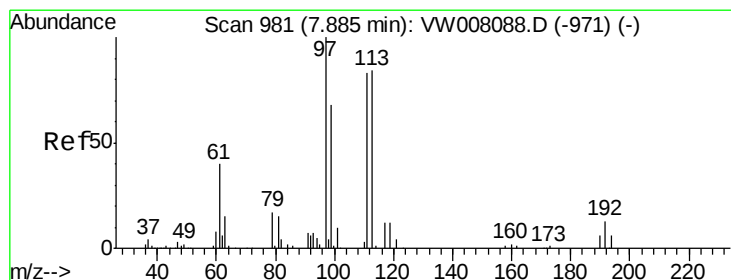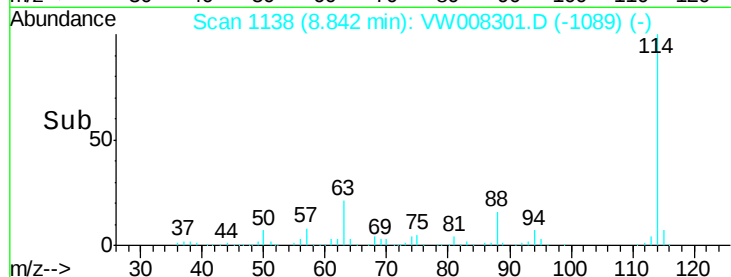
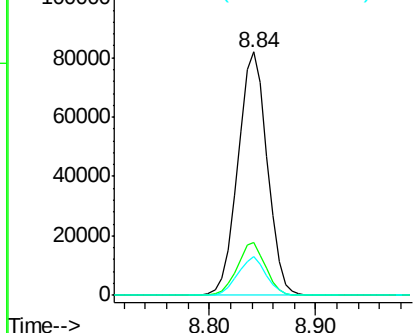



#35
 Dibromofluoromethane
 Concen: 54.305 ug/l
 RT: 7.88 min Scan# 980
 Delta R.T. -0.01 min
 Lab File: VW008301.D
 Acq: 16 Jan 2019 11:53

Tgt Ion:113 Resp: 50285
 Ion Ratio Lower Upper
 113 100
 111 102.7 81.8 122.8
 192 17.6 12.8 19.2

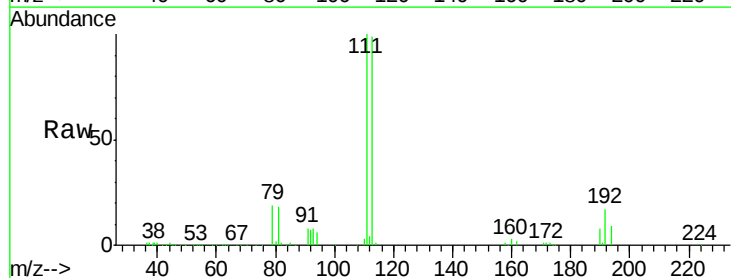

Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

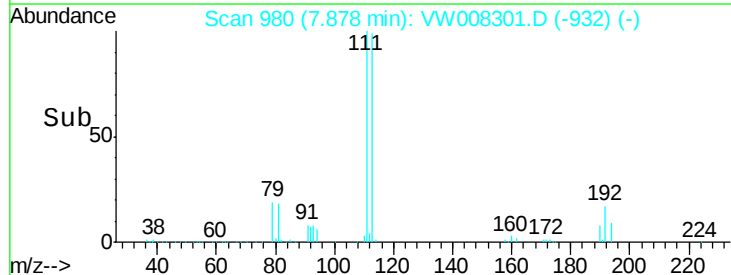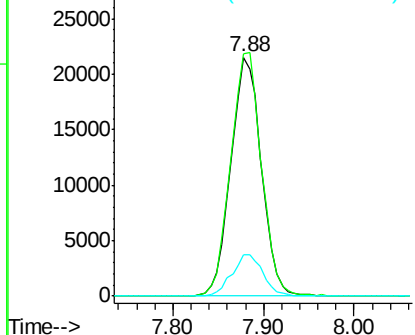

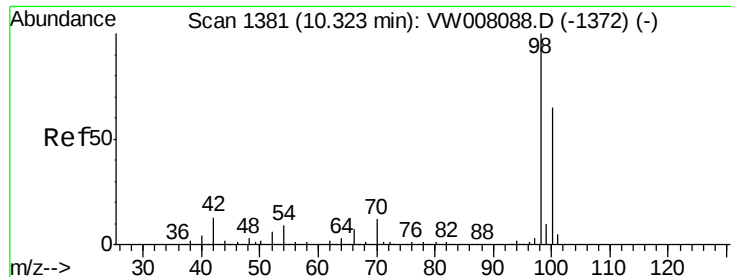

#50

Toluene-d8

Concen: 51.393 ug/l

RT: 10.32 min Scan# 1381

Delta R.T. 0.00 min

Lab File: VW008301.D

Acq: 16 Jan 2019 11:53

Instrument :

MSVOA_W

ClientSampleId :





VW0116SBL01

Tot Ion: 98 Resp: 199698

Ion Ratio Lower Upper

98 100

100 64.6 51.7 77.5

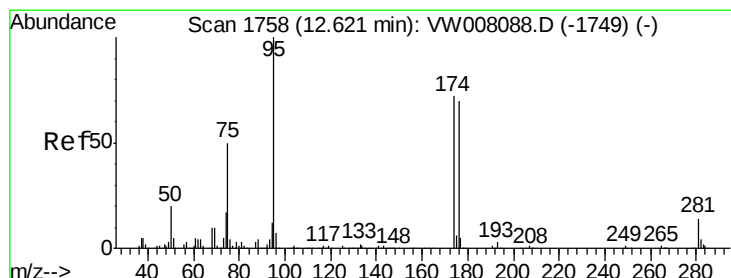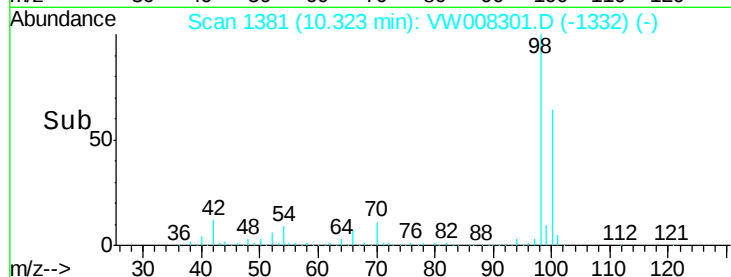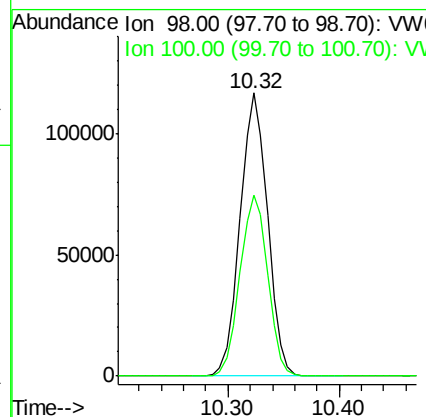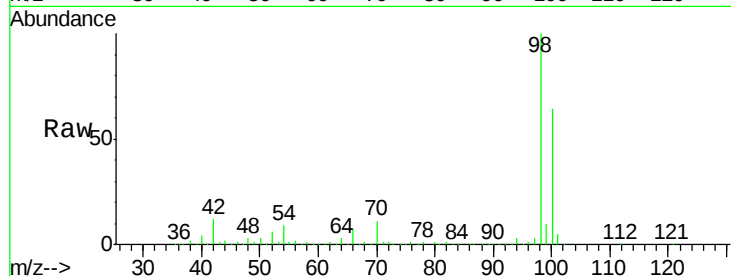

#62

4-Bromofluorobenzene

Concen: 48.174 ug/l

RT: 12.62 min Scan# 1758

Delta R.T. 0.00 min

Lab File: VW008301.D

Acq: 16 Jan 2019 11:53




Tgt Ion: 95 Resp: 67108


Ion Ratio Lower Upper

95 100

174 77.4 0.0 143.0

176 72.6 0.0 140.2

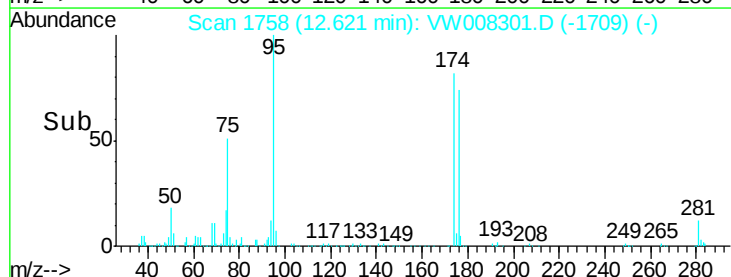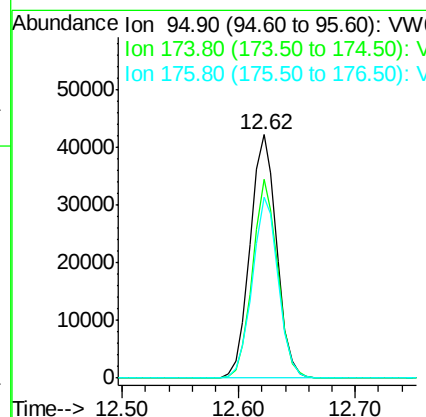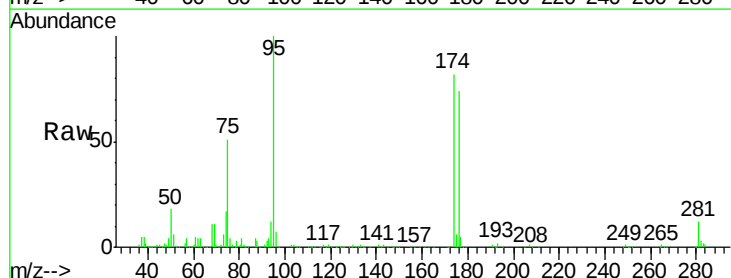


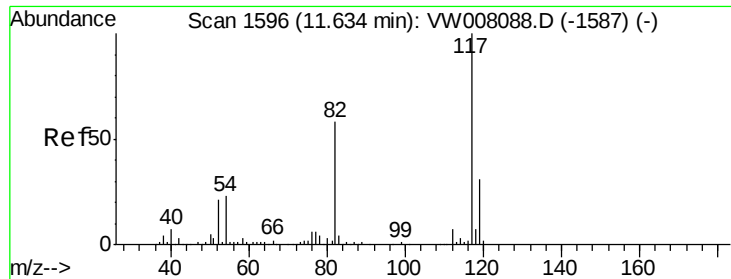




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.63 min Scan# 1596
Delta R.T. 0.00 min
Lab File: VW008301.D
Acq: 16 Jan 2019 11:53

Instrument :
MSVOA_W
ClientSampleId :
VW0116SBL01

Tot Ion:117 Resp: 145670
Ion Ratio Lower Upper
117 100
82 54.6 46.4 69.6
119 31.7 24.7 37.1

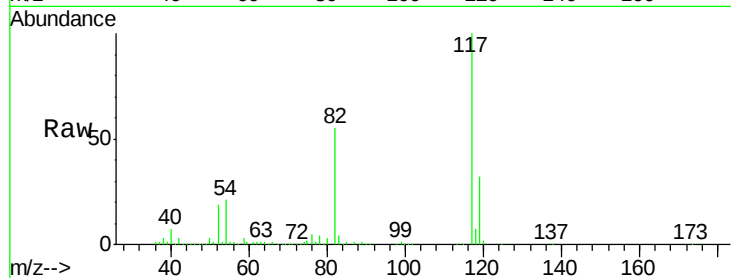


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

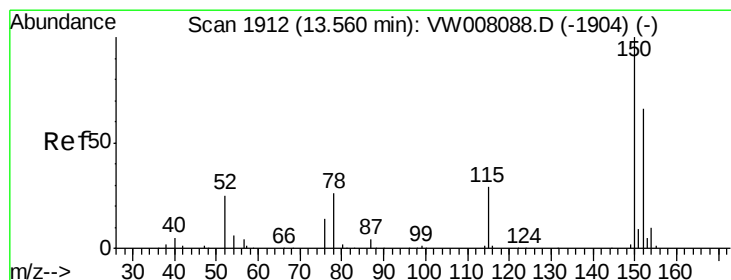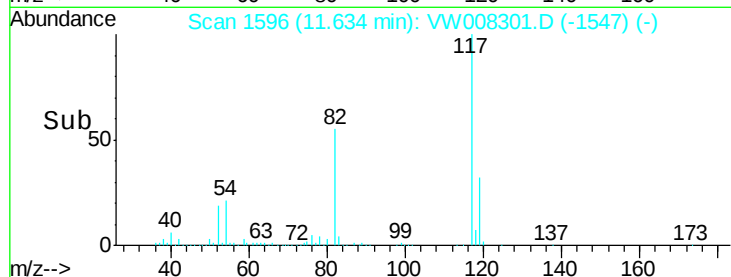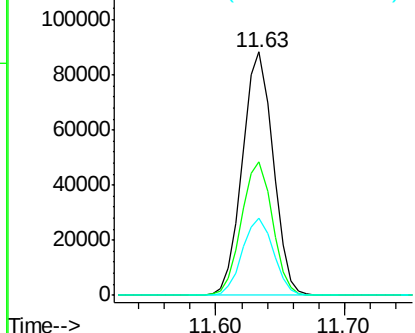

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.56 min Scan# 1912
Delta R.T. 0.00 min
Lab File: VW008301.D
Acq: 16 Jan 2019 11:53

Tgt Ion:152 Resp: 64897
Ion Ratio Lower Upper
152 100
115 61.2 30.8 92.4
150 161.1 0.0 350.2

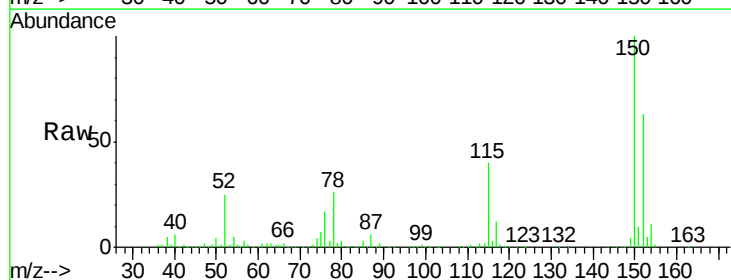

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

