


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW011619\
 Data File : VW008299.D
 Acq On : 16 Jan 2019 09:56
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W010819S.M
 Title : SW846 8260
 Last Update : Wed Jan 09 04:40:48 2019

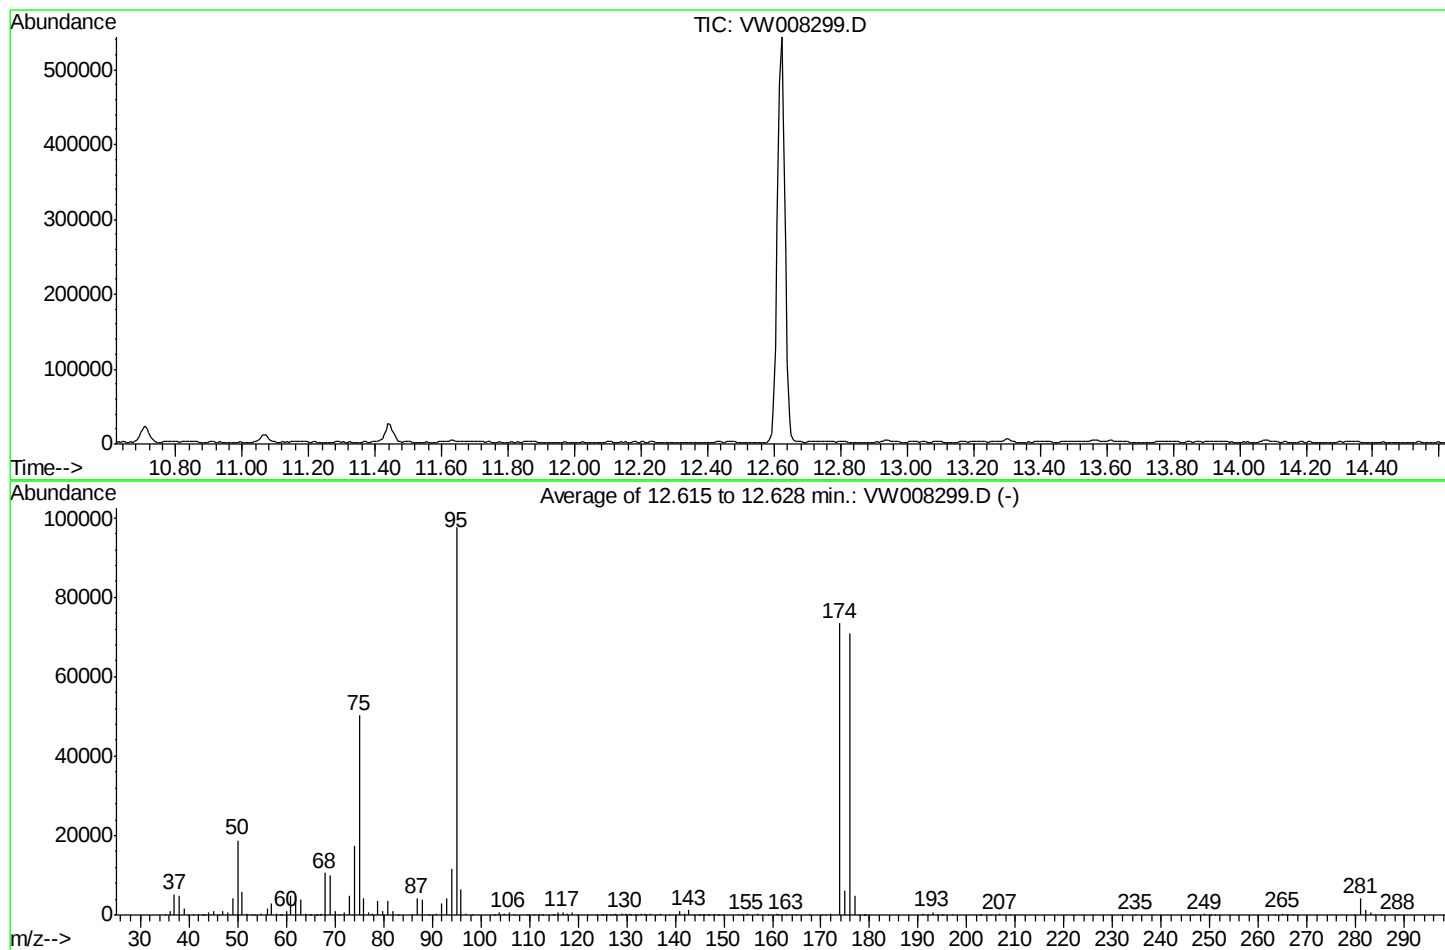

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1747

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	18853	PASS
75	95	30	60	51.4	50186	PASS
95	95	100	100	100.0	97586	PASS
96	95	5	9	6.6	6423	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	75.3	73445	PASS
175	174	5	9	8.4	6147	PASS
176	174	95	101	96.6	70914	PASS
177	176	5	9	6.7	4764	PASS