

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW011720\
 Data File : VW014682.D
 Acq On : 17 Jan 2020 13:08
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampled :
 VIBLK

Manual Integrations
APPROVED

MMDadoda
 1/17/2020 4:58:11 PM

Quant Time: Jan 17 14:43:12 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122719S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jan 17 14:29:33 2020
 Response via : Initial Calibration

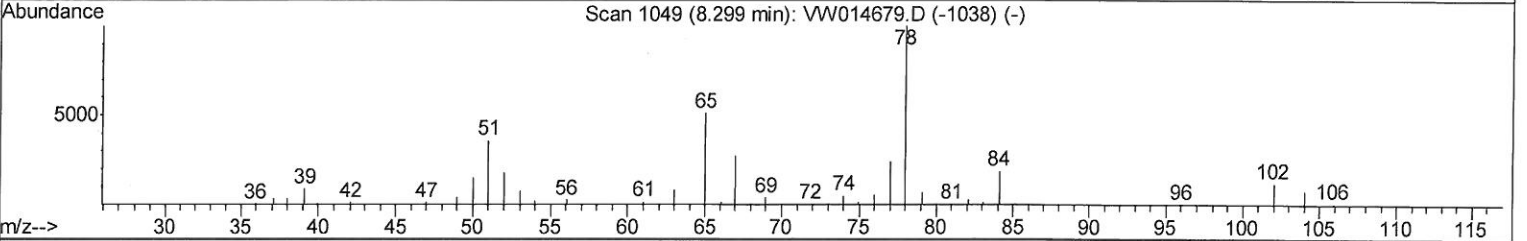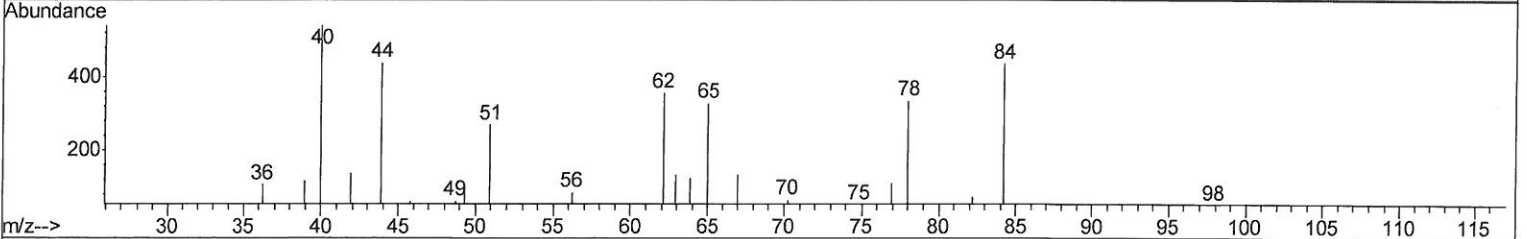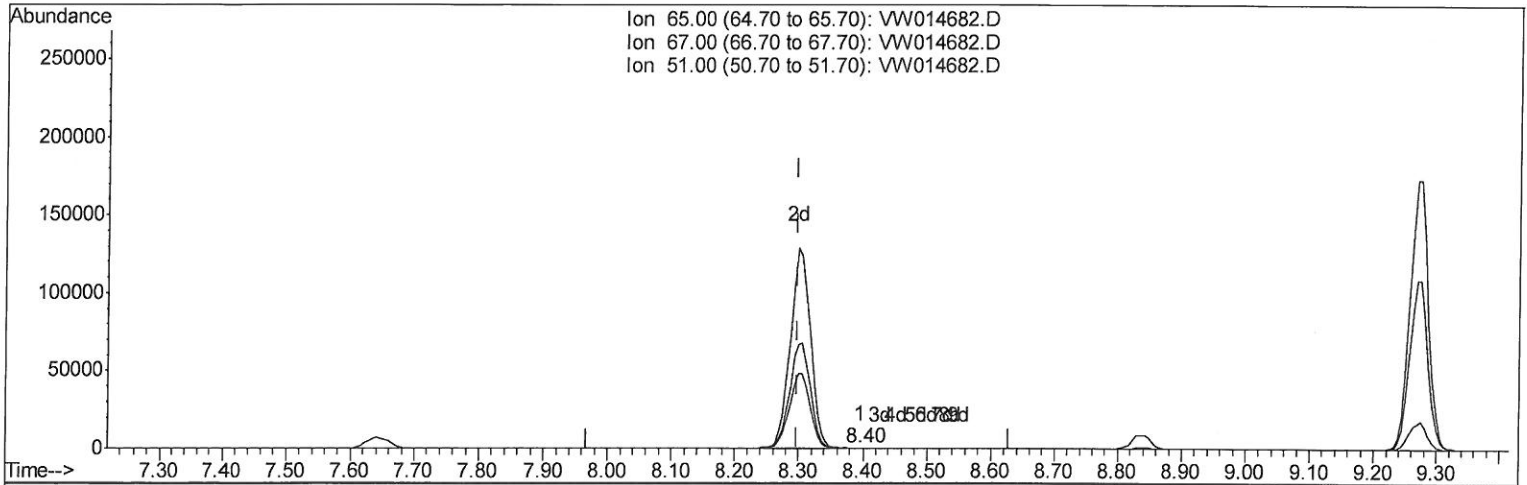

TIC: VW014682.D

(26) 1,2-Dichloroethane-d4 (S)

8.397min (+0.098) 0.02ug/L

response 300

Ion	Exp%	Act%
65.00	100	100
67.00	54.90	49.33
51.00	114.80	107.33
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW011720\
 Data File : VW014682.D
 Acq On : 17 Jan 2020 13:08
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK

Manual Integrations
 APPROVED

MMDadoda
 1/17/2020 4:58:11 PM

Quant Time: Jan 17 14:43:12 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122719S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jan 17 14:29:33 2020
 Response via : Initial Calibration

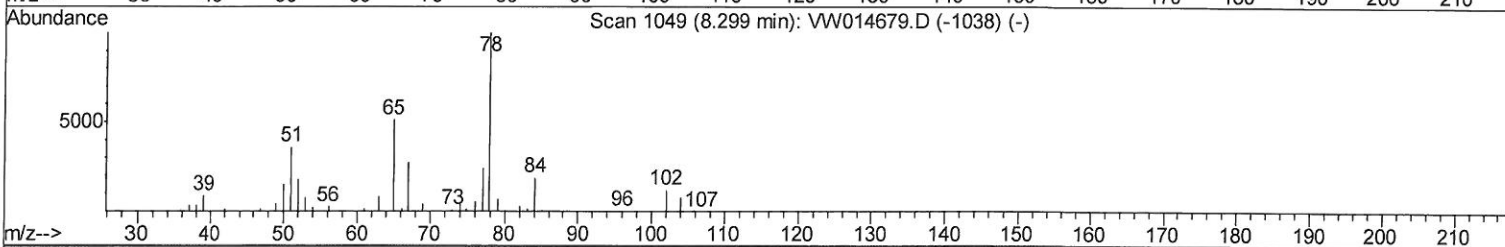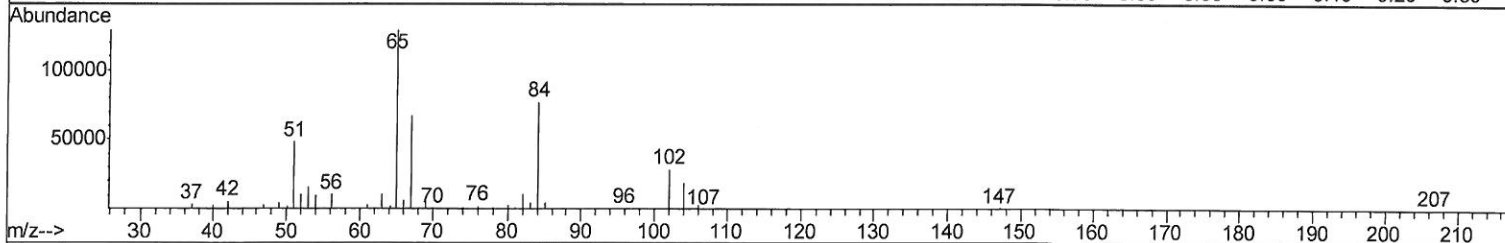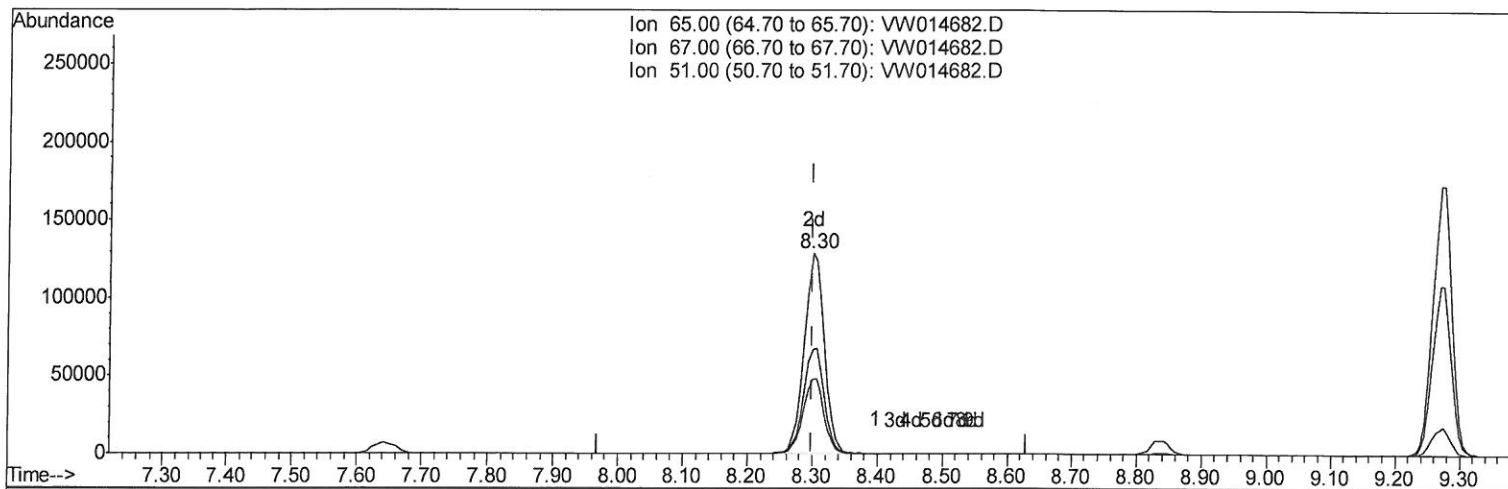

TIC: VW014682.D

(26) 1,2-Dichloroethane-d4 (S)

8.299min (+0.000) 21.14ug/L m

response 279422

Ion	Exp%	Act%
65.00	100	100
67.00	54.90	0.05#
51.00	114.80	0.12#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW011720\
 Data File : VW014682.D
 Acq On : 17 Jan 2020 13:08
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK

Manual Integrations
 APPROVED

MMDadoda
 1/17/2020 4:58:11 PM

Quant Time: Jan 17 15:03:49 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122719S.M
 Quant Title : VOC Analysis
 QLast Update : Fri Jan 17 14:29:33 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	1107067	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	974860	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	475290	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	274474	17.59	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	70.36%		
7) Chloroethane-d5	2.89	69	223316	19.42	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	77.68%		
10) 1,1-Dichloroethene-d2	4.01	63	408485	14.31	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	57.24%		
20) 2-Butanone-d5	7.07	46	176422	47.51	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	95.02%		
24) Chloroform-d	7.65	84	523737	20.56	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	82.24%		
26) 1,2-Dichloroethane-d4	8.30	65	279422m	21.14	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	84.56%		
29) Benzene-d6	8.27	84	1142945	22.05	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	88.20%		
33) 1,2-Dichloropropane-d6	9.27	67	349918	22.45	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	89.80%		
37) Toluene-d8	10.32	98	1027089	21.85	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	87.40%		
38) trans-1,3-Dichloropropene-	10.57	79	136460	21.20	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	84.80%		
39) 2-Hexanone-d5	10.92	63	139428	52.31	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	104.62%		
48) 1,1,2,2-Tetrachloroethane-	12.69	84	281627	24.06	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	96.24%		
61) 1,2-Dichlorobenzene-d4	13.85	152	364590	23.28	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	93.12%		

01/17/2020

Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW011720\
Data File : VW014682.D
Acq On : 17 Jan 2020 13:08
Operator : SY/VA
Sample : VIBLK
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
VIBLK

Manual Integrations
APPROVED

MMDadoda
1/17/2020 4:58:11 PM

Quant Time: Jan 17 15:03:49 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122719S.M
Quant Title : VOC Analysis
QLast Update : Fri Jan 17 14:29:33 2020
Response via : Initial Calibration

