
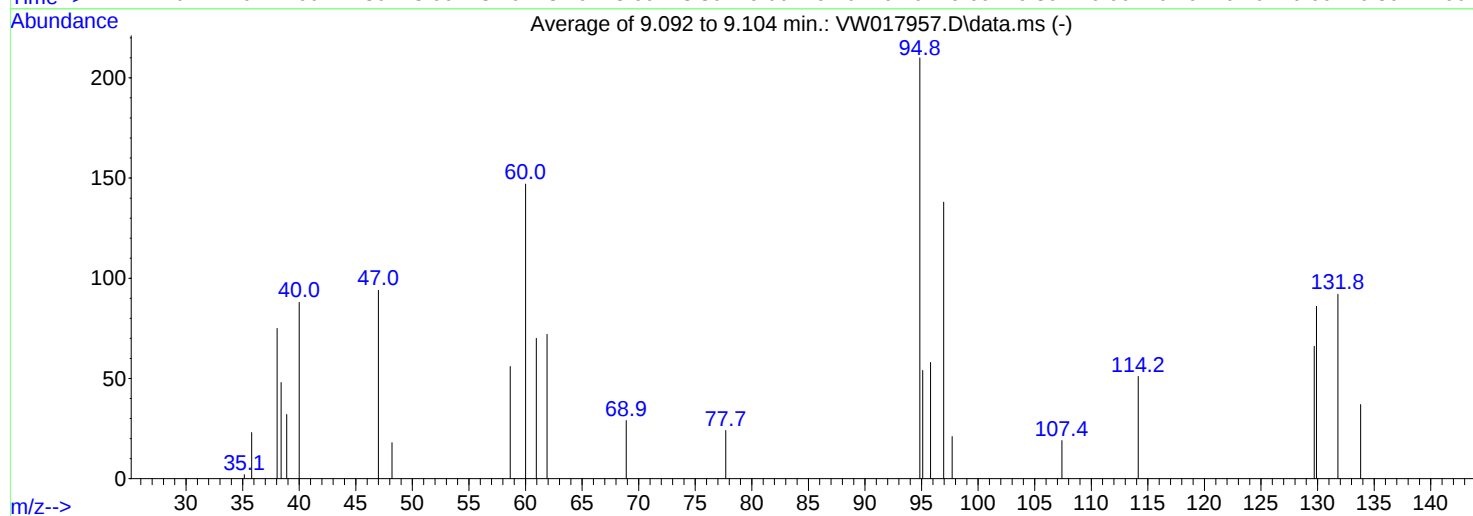


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW011921\
 Data File : VW017957.D
 Acq On : 19 Jan 2021 14:59
 Operator : SY/VA
 Sample : M1170-05
 Misc : 4.96G/10ML/MSVOA_W/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SOM2WLM011821S.M
 Title : VOC Analysis
 Last Update : Wed Jan 20 04:48:23 2021

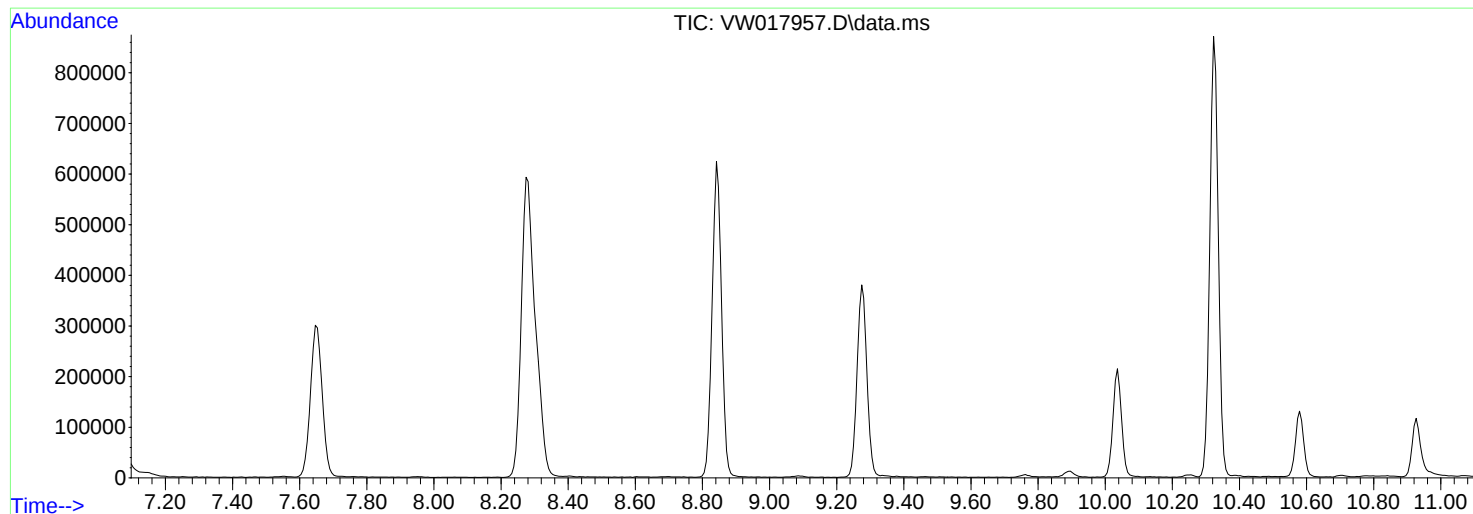

AutoFind: Scans 1179, 1180, 1181; Background Corrected with Scan 1176

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	0.0	0	FAIL*
75	95	30	80	0.0	0	FAIL*
95	95	100	100	100.0	210	PASS
96	95	5	9	27.6	58	FAIL*
173.00	174.00	COMPARISON MASS IS NOT PRESENT!!!				
174	95	50	120	0.0	0	FAIL*
175.00	174.00	COMPARISON MASS IS NOT PRESENT!!!				
176.00	174.00	COMPARISON MASS IS NOT PRESENT!!!				
177.00	176.00	COMPARISON MASS IS NOT PRESENT!!!				