

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW012020\
 Data File : VW014692.D
 Acq On : 20 Jan 2020 13:53
 Operator : SY/VA
 Sample : L1118-20
 Misc : 4.99G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GASN5

Manual Integrations
 APPROVED

MMDadoda
 1/21/2020 2:20:15 PM

Quant Time: Jan 21 04:00:37 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122719S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jan 21 03:38:42 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	1185362	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	1065803	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	465630	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	340505	20.38	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.52%
7) Chloroethane-d5	2.89	69	276848	22.49	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.96%
10) 1,1-Dichloroethene-d2	4.01	63	510885	16.71	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.84%
20) 2-Butanone-d5	7.07	46	194472	48.91	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.82%
24) Chloroform-d	7.64	84	679777	24.93	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	99.72%
26) 1,2-Dichloroethane-d4	8.30	65	362166m	25.59	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	102.36%
29) Benzene-d6	8.27	84	1431560	25.26	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	101.04%
33) 1,2-Dichloropropane-d6	9.27	67	447241	26.24	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	104.96%
37) Toluene-d8	10.32	98	1286035	25.03	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	100.12%
38) trans-1,3-Dichloropropene-	10.57	79	172425	24.50	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	98.00%
39) 2-Hexanone-d5	10.92	63	150291	51.58	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.16%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	332182	25.96	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	103.84%
61) 1,2-Dichlorobenzene-d4	13.85	152	425191	27.71	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	110.84%

Target Compounds					Ovalue
13) Acetone	4.12	43	17018	3.091 ug/L	100
44) Toluene	10.38	91	28143	0.420 ug/L	89

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW012020\
Data File : VW014692.D
Acq On : 20 Jan 2020 13:53
Operator : SY/VA
Sample : L1118-20
Misc : 4.99G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
GASN5

Manual Integrations
APPROVED

MMDadoda
1/21/2020 2:20:15 PM

Quant Time: Jan 21 04:00:37 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM122719S.M
Quant Title : VOC Analysis
QLast Update : Tue Jan 21 03:38:42 2020
Response via : Initial Calibration

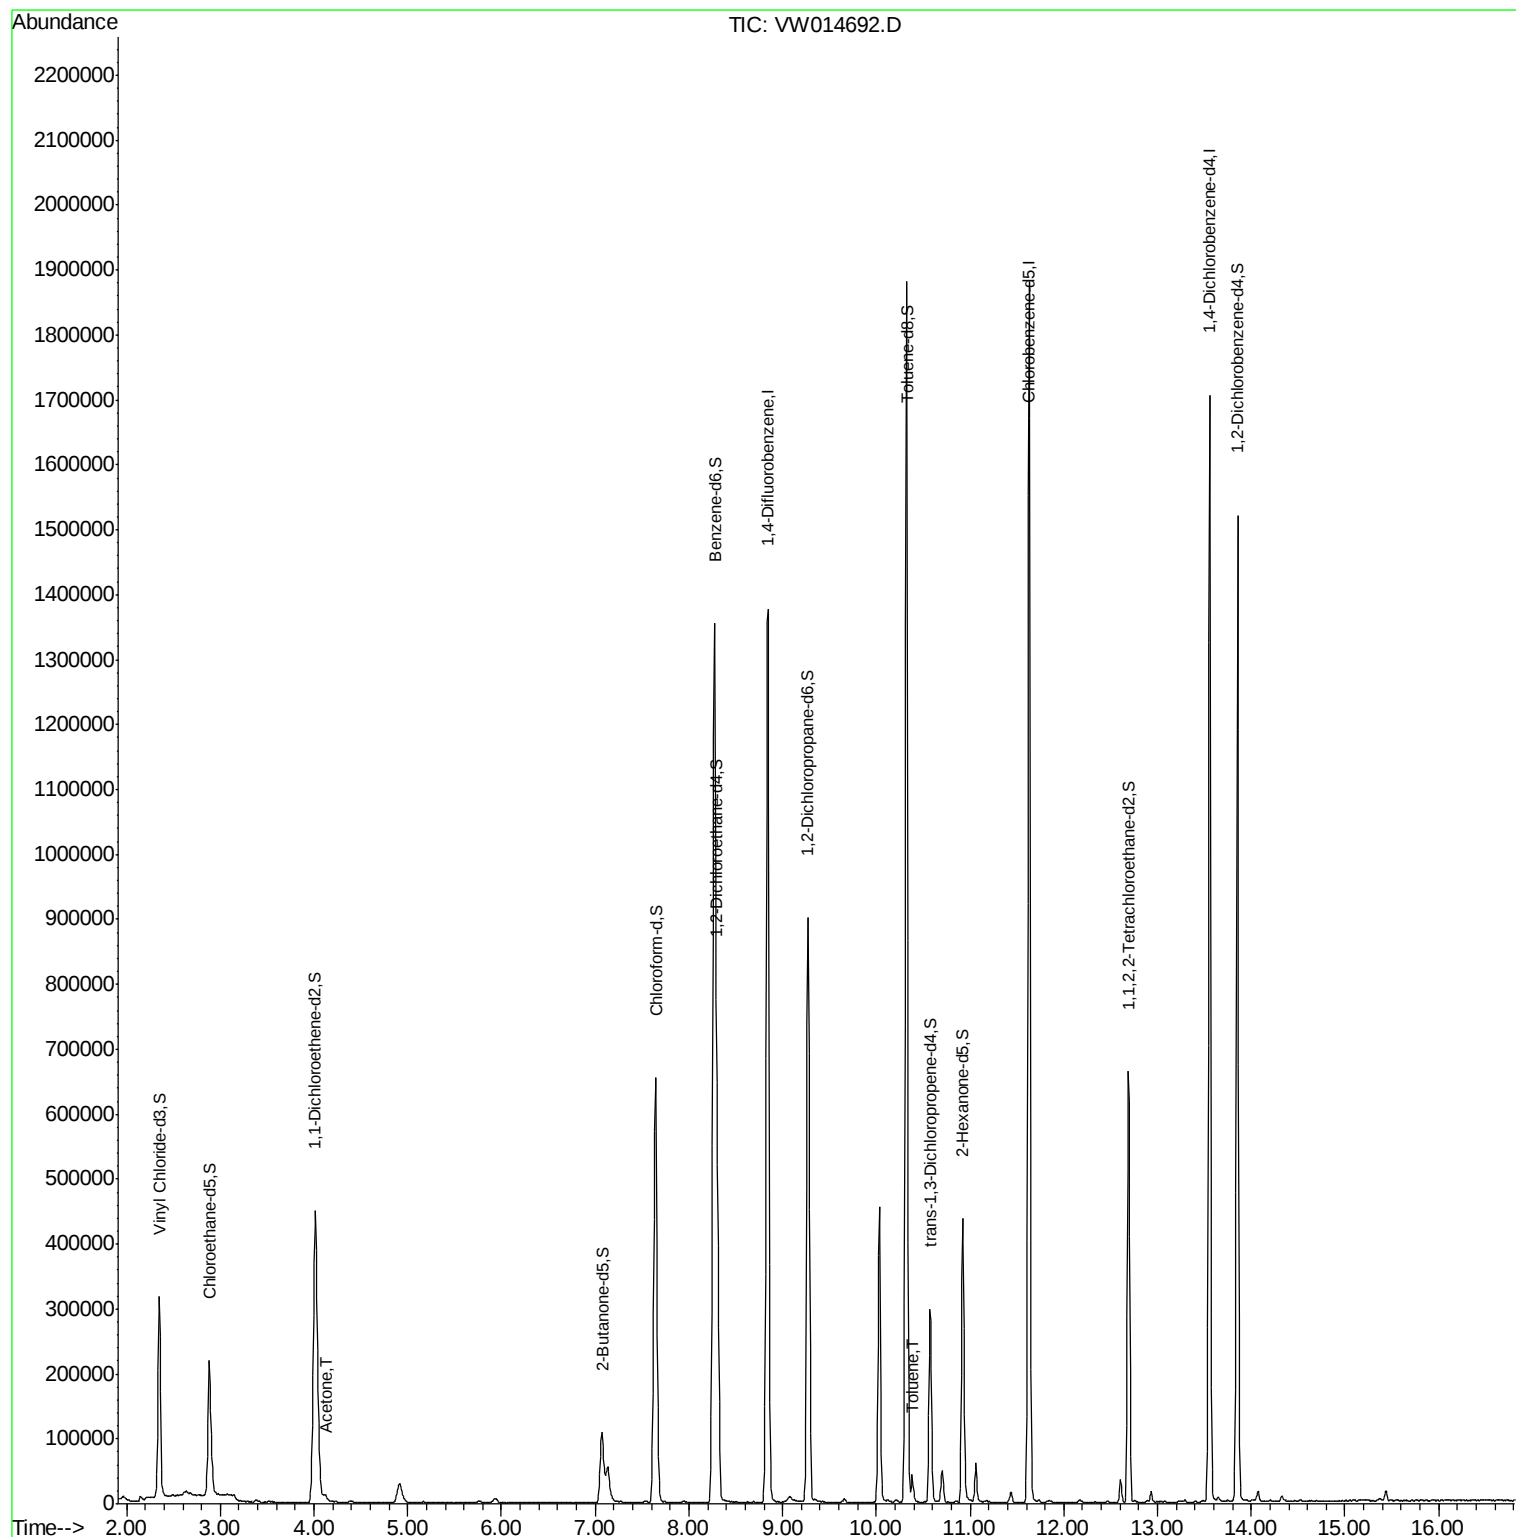

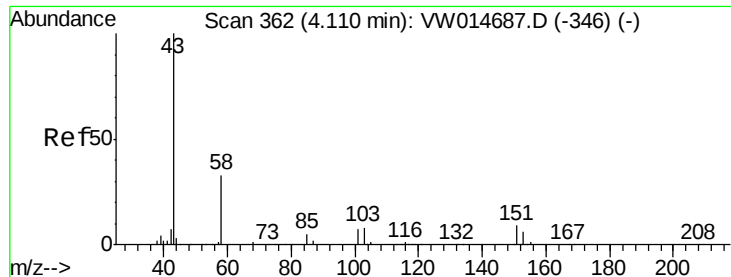





#13
Acetone
Concen: 3.091 ug/L
RT: 4.12 min Scan# 364
Delta R.T. 0.01 min
Lab File: VW014692.D
Acq: 20 Jan 2020 13:53

Instrument :
MSVOA_W
ClientSampled :
GASN5

Tot Ion: 43 Resp: 17018
Ion Ratio Lower Upper
43 100
58 32.2 0.0 64.0

Manual Integrations
APPROVED

MMDadoda
1/21/2020 2:20:15 PM

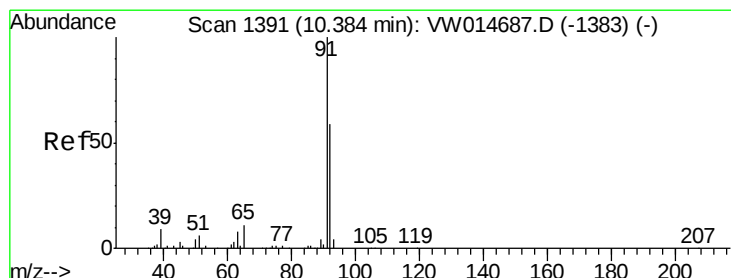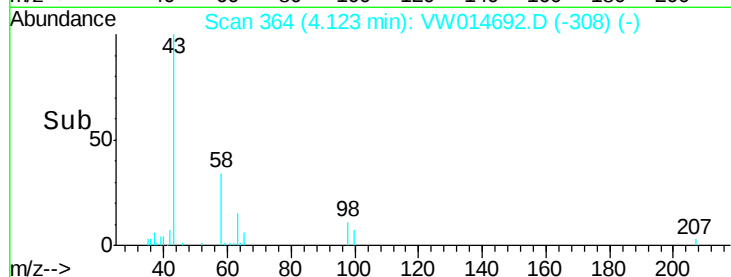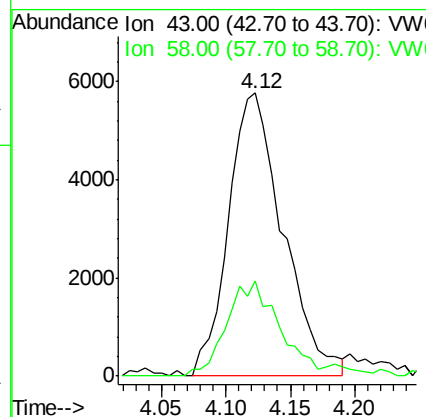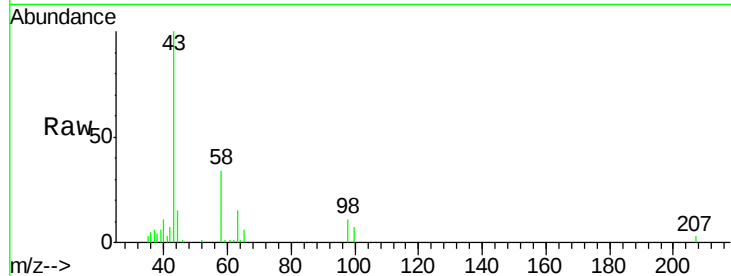

#44
Toluene
Concen: 0.420 ug/L
RT: 10.38 min Scan# 1391
Delta R.T. 0.00 min
Lab File: VW014692.D
Acq: 20 Jan 2020 13:53

Tgt Ion: 91 Resp: 28143
Ion Ratio Lower Upper
91 100
92 65.6 40.2 74.6

