

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW012025\
 Data File : VW031580.D
 Acq On : 20 Jan 2025 13:54
 Operator : SY/MD
 Sample : Q1108-16
 Misc : 5.78g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jan 21 01:00:51 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011025SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jan 18 00:35:19 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	938896	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	807102	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	358169	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	349141	23.698	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	94.800%
7) Chloroethane-d5	2.899	69	242030	23.003	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	92.000%
11) 1,1-Dichloroethene-d2	4.015	65	154463	23.564	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	94.240%
21) 2-Butanone-d5	7.094	46	100444	42.411	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	84.820%
24) Chloroform-d	7.648	84	545495	22.450	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.800%
26) 1,2-Dichloroethane-d4	8.301	65	271178	22.674	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	90.680%
32) Benzene-d6	8.270	84	1191106	23.494	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	93.960%
36) 1,2-Dichloropropane-d6	9.270	67	336811	22.501	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	90.000%
41) Toluene-d8	10.319	98	1054877	23.049	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	92.200%
43) trans-1,3-Dichloroprop...	10.575	79	132078	21.487	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	85.960%
47) 2-Hexanone-d5	10.922	63	67092	43.921	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.840%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	199127	21.753	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	87.000%
66) 1,2-Dichlorobenzene-d4	13.848	152	286255	22.787	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	91.160%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	9308	0.426	ug/L	# 77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW012025\
Data File : VW031580.D
Acq On : 20 Jan 2025 13:54
Operator : SY/MD
Sample : Q1108-16
Misc : 5.78g/10mL/MSVOA_W/SOIL/A
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Jan 21 01:00:51 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM011025SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jan 18 00:35:19 2025
Response via : Initial Calibration

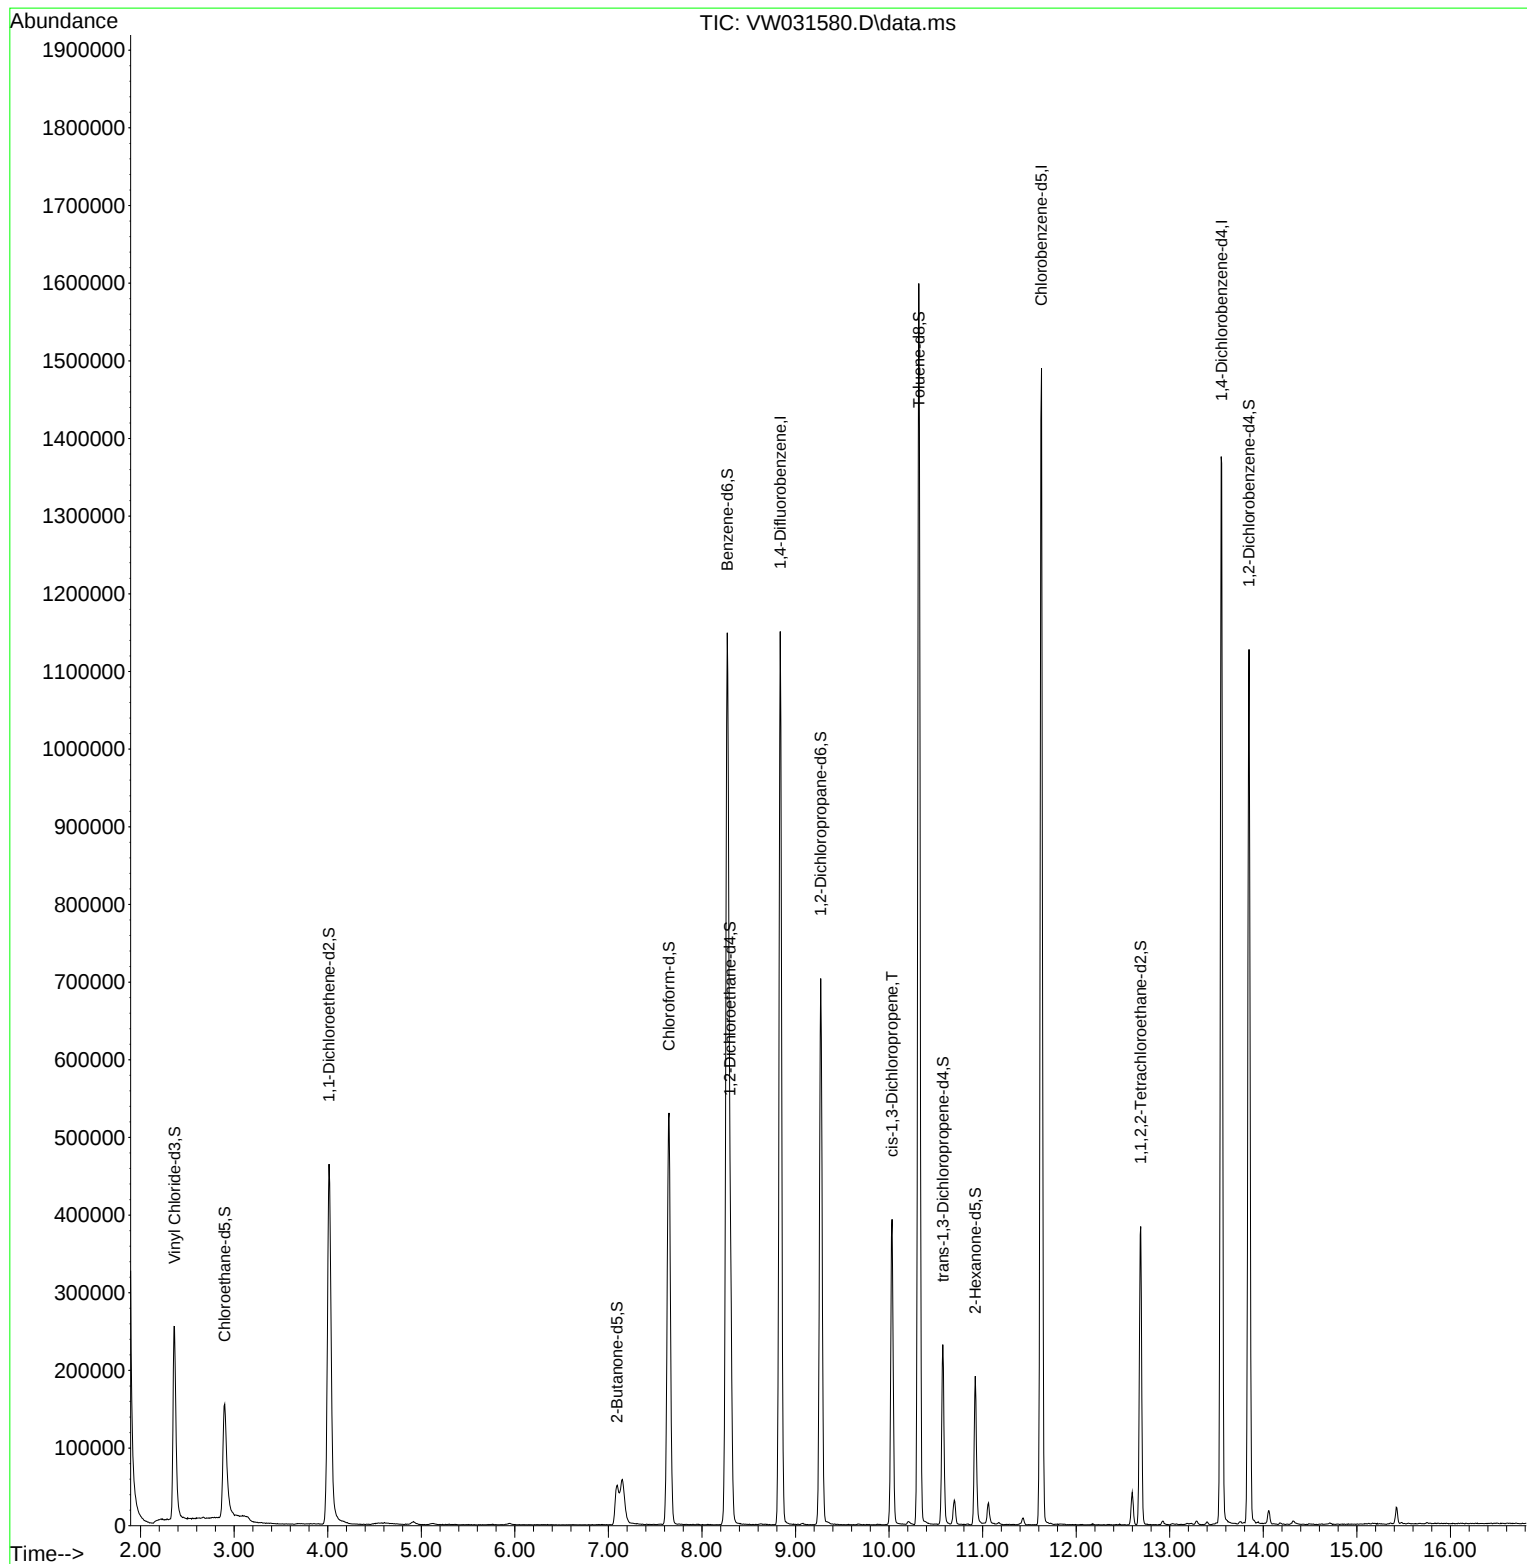

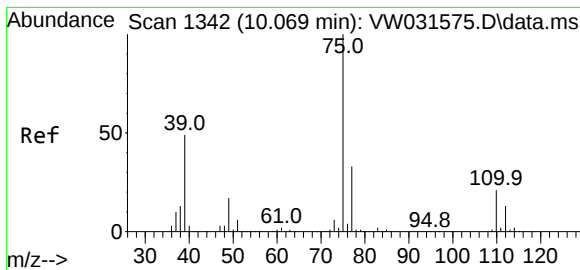

#39
 cis-1,3-Dichloropropene
 Concen: 0.426 ug/L
 RT: 10.032 min Scan# 11
 Delta R.T. -0.037 min
 Lab File: VW031580.D
 Acq: 20 Jan 2025 13:54

Instrument :
 MSVOA_W
 ClientSampleId :

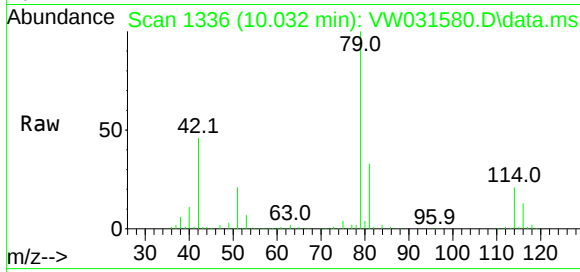

Tgt Ion: 75 Resp: 9308
 Ion Ratio Lower Upper
 75 100
 77 43.5 21.6 40.2#

