
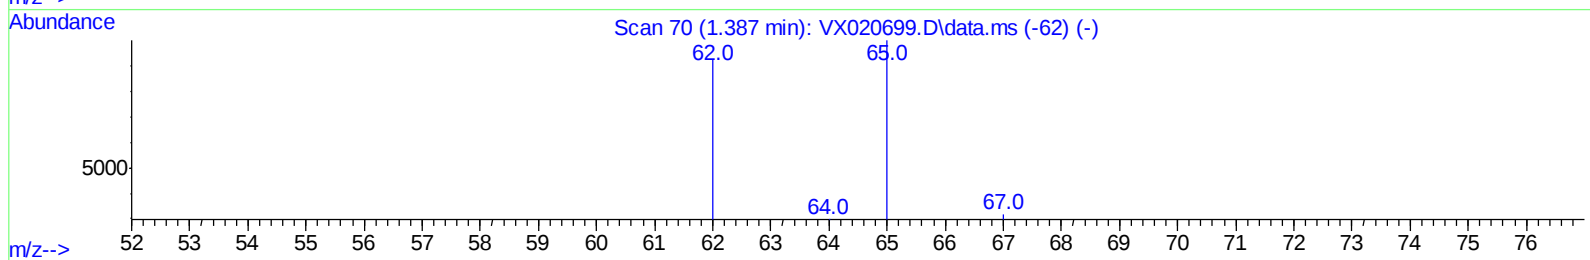
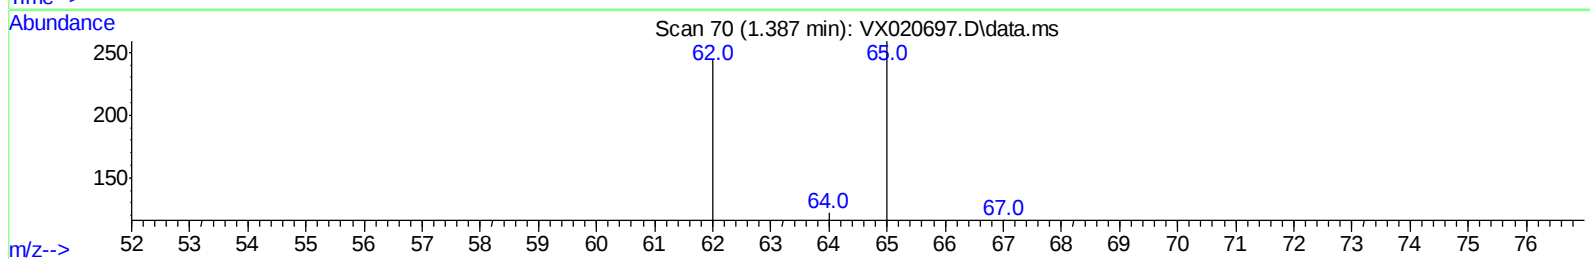


Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX012121\
Data File : VX020697.D
Acq On : 21 Jan 2021 14:47
Operator : JC/SP
Sample : VSTD0.0504
Misc : 25.0mL/MSVOA_X/WATER
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Jan 22 01:25:17 2021
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_X\METHOD\SFAMXSIM012121.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Fri Jan 22 01:23:42 2021
Response via : Initial Calibration

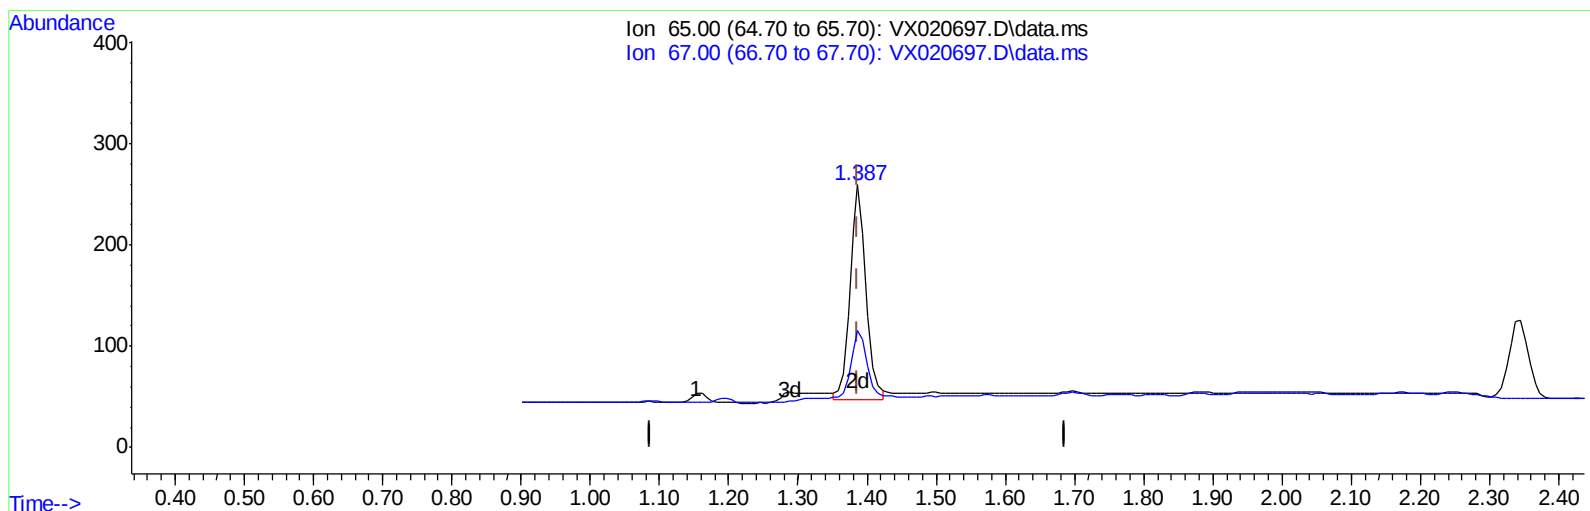

TIC: VX020697.D\data.ms

(2) Vinyl Chloride-d3 (S)

1.387min (-0.000) 0.04 ug/L m

response 339

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	33.20	1.47#
0.00	0.00	0.00
0.00	0.00	0.00