



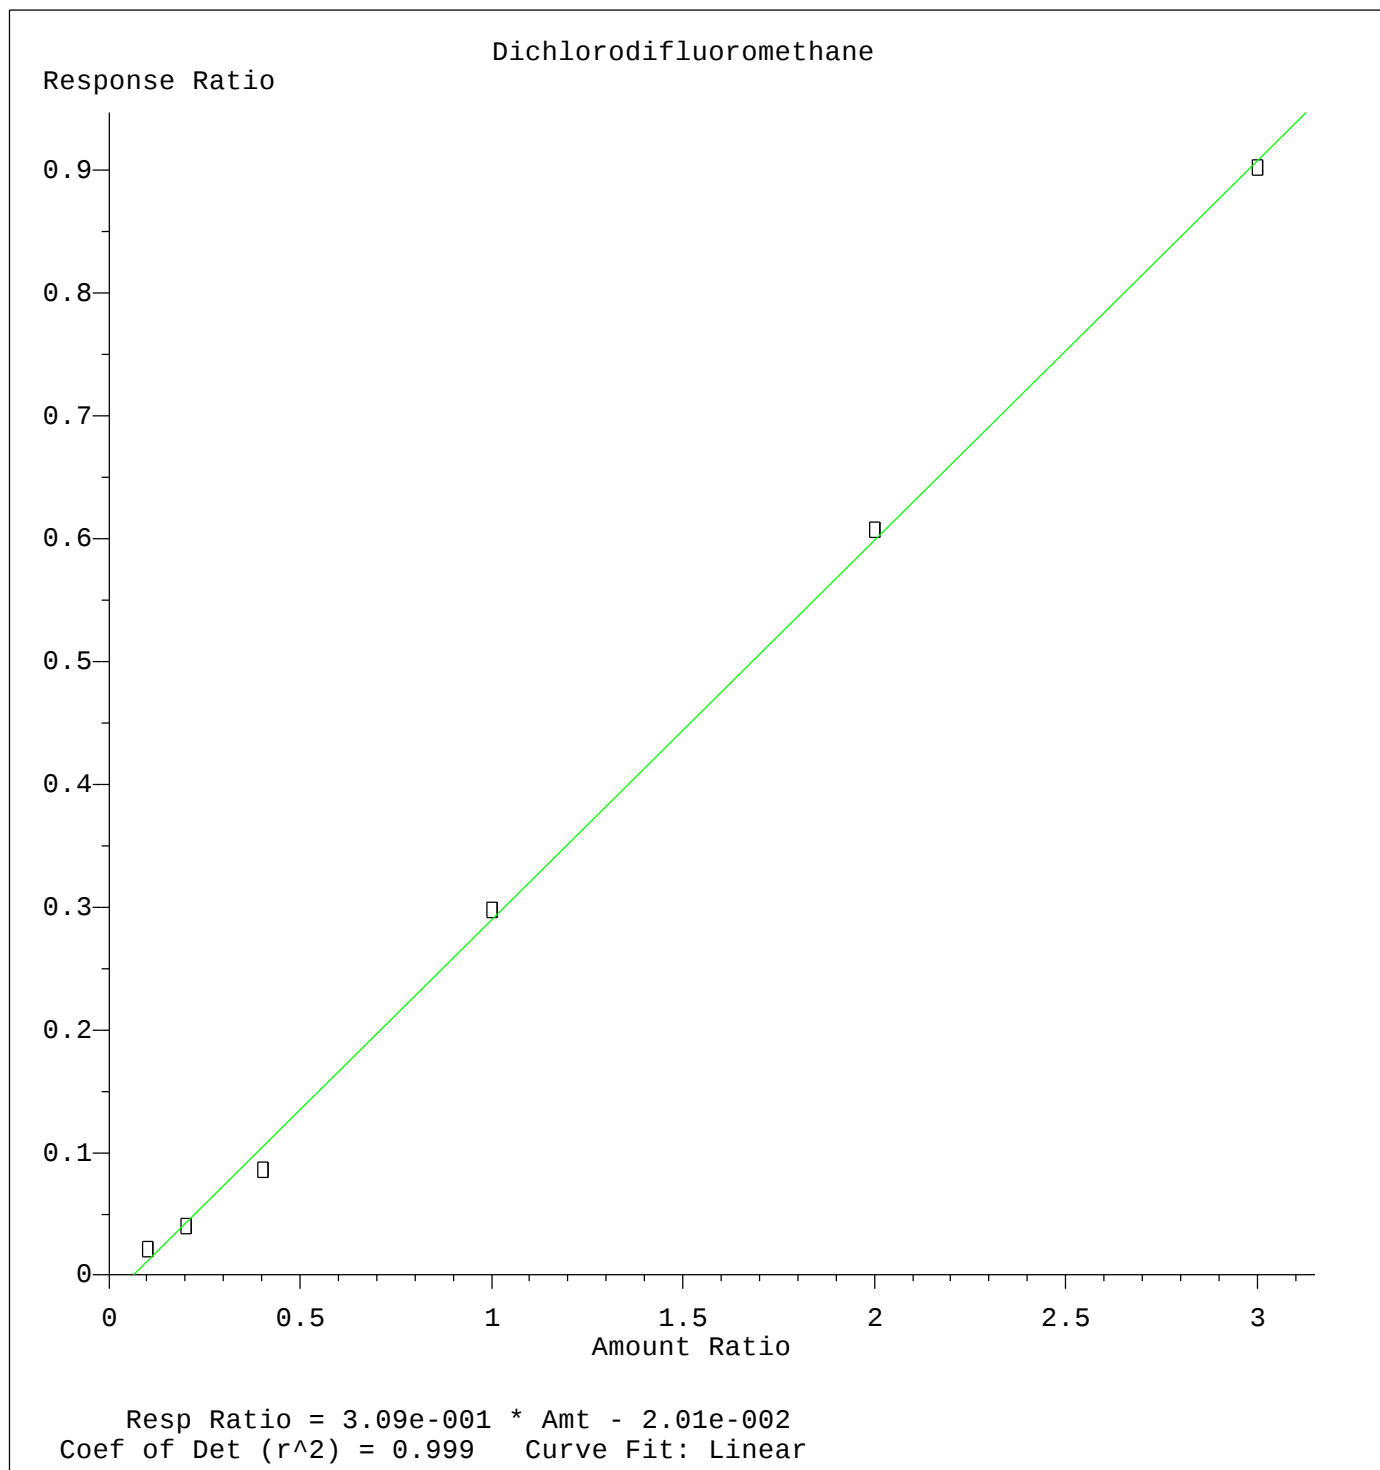

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W012419S.M
Calibration Table Last Updated: Fri Jan 25 11:07:41 2019


Trichlorofluoromethane

Response Ratio

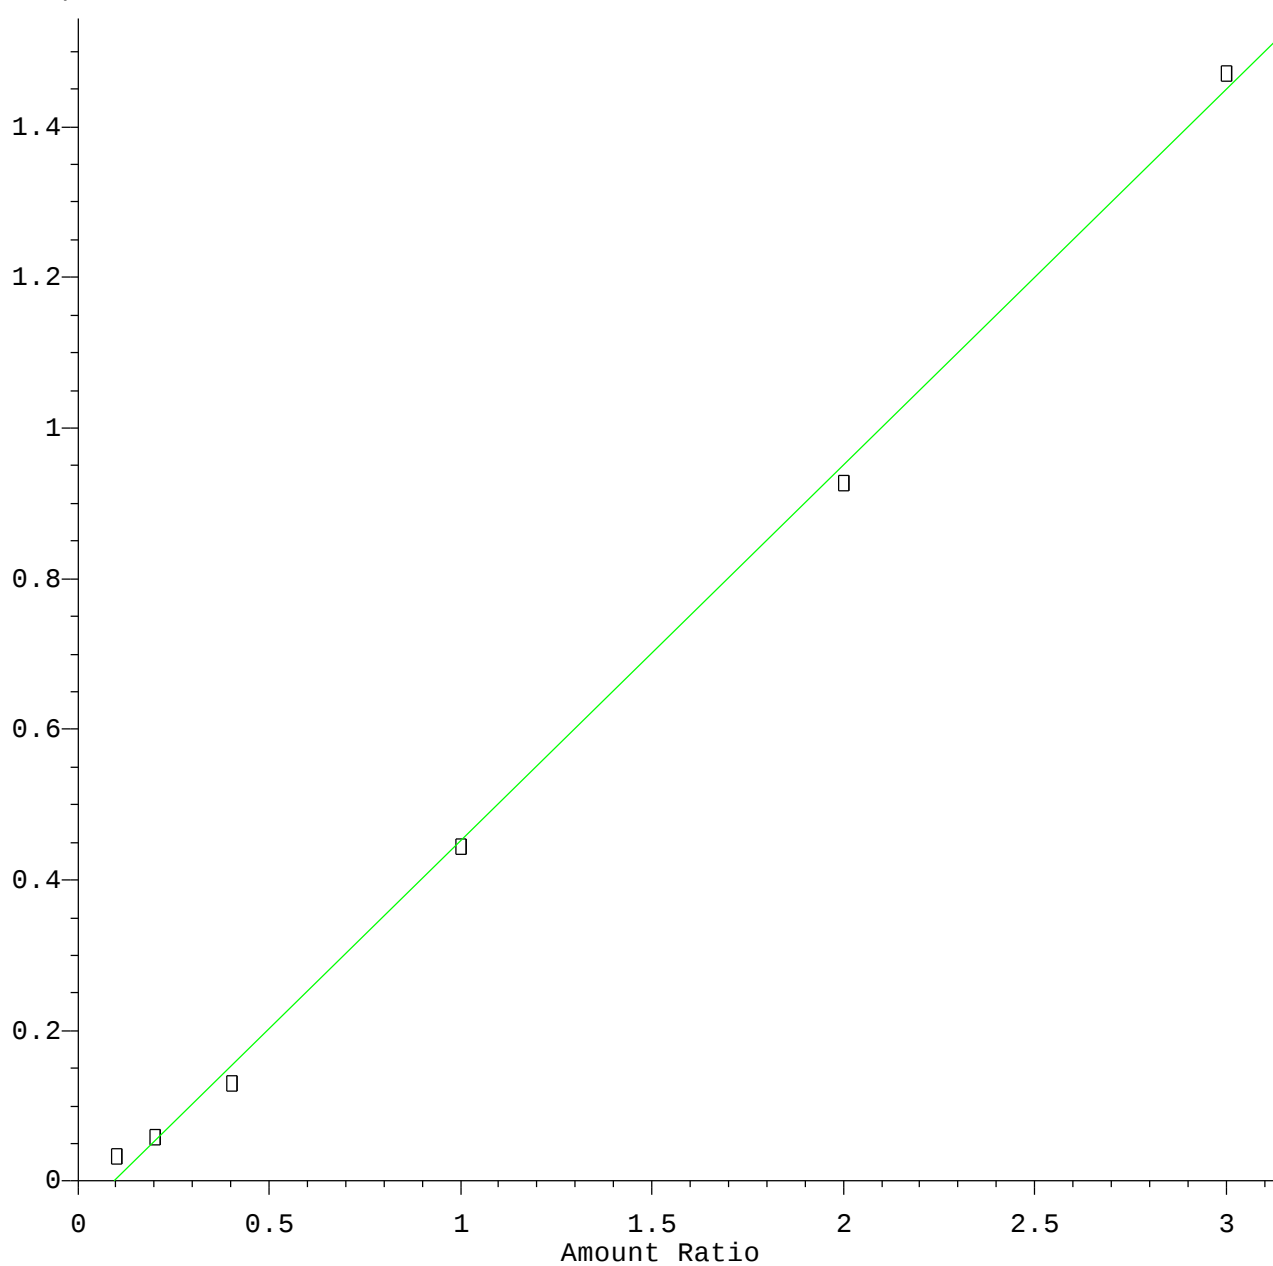

Resp Ratio = $4.99 \times 10^{-1} \times \text{Amt} - 4.72 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W012419S.M
Calibration Table Last Updated: Fri Jan 25 11:07:41 2019

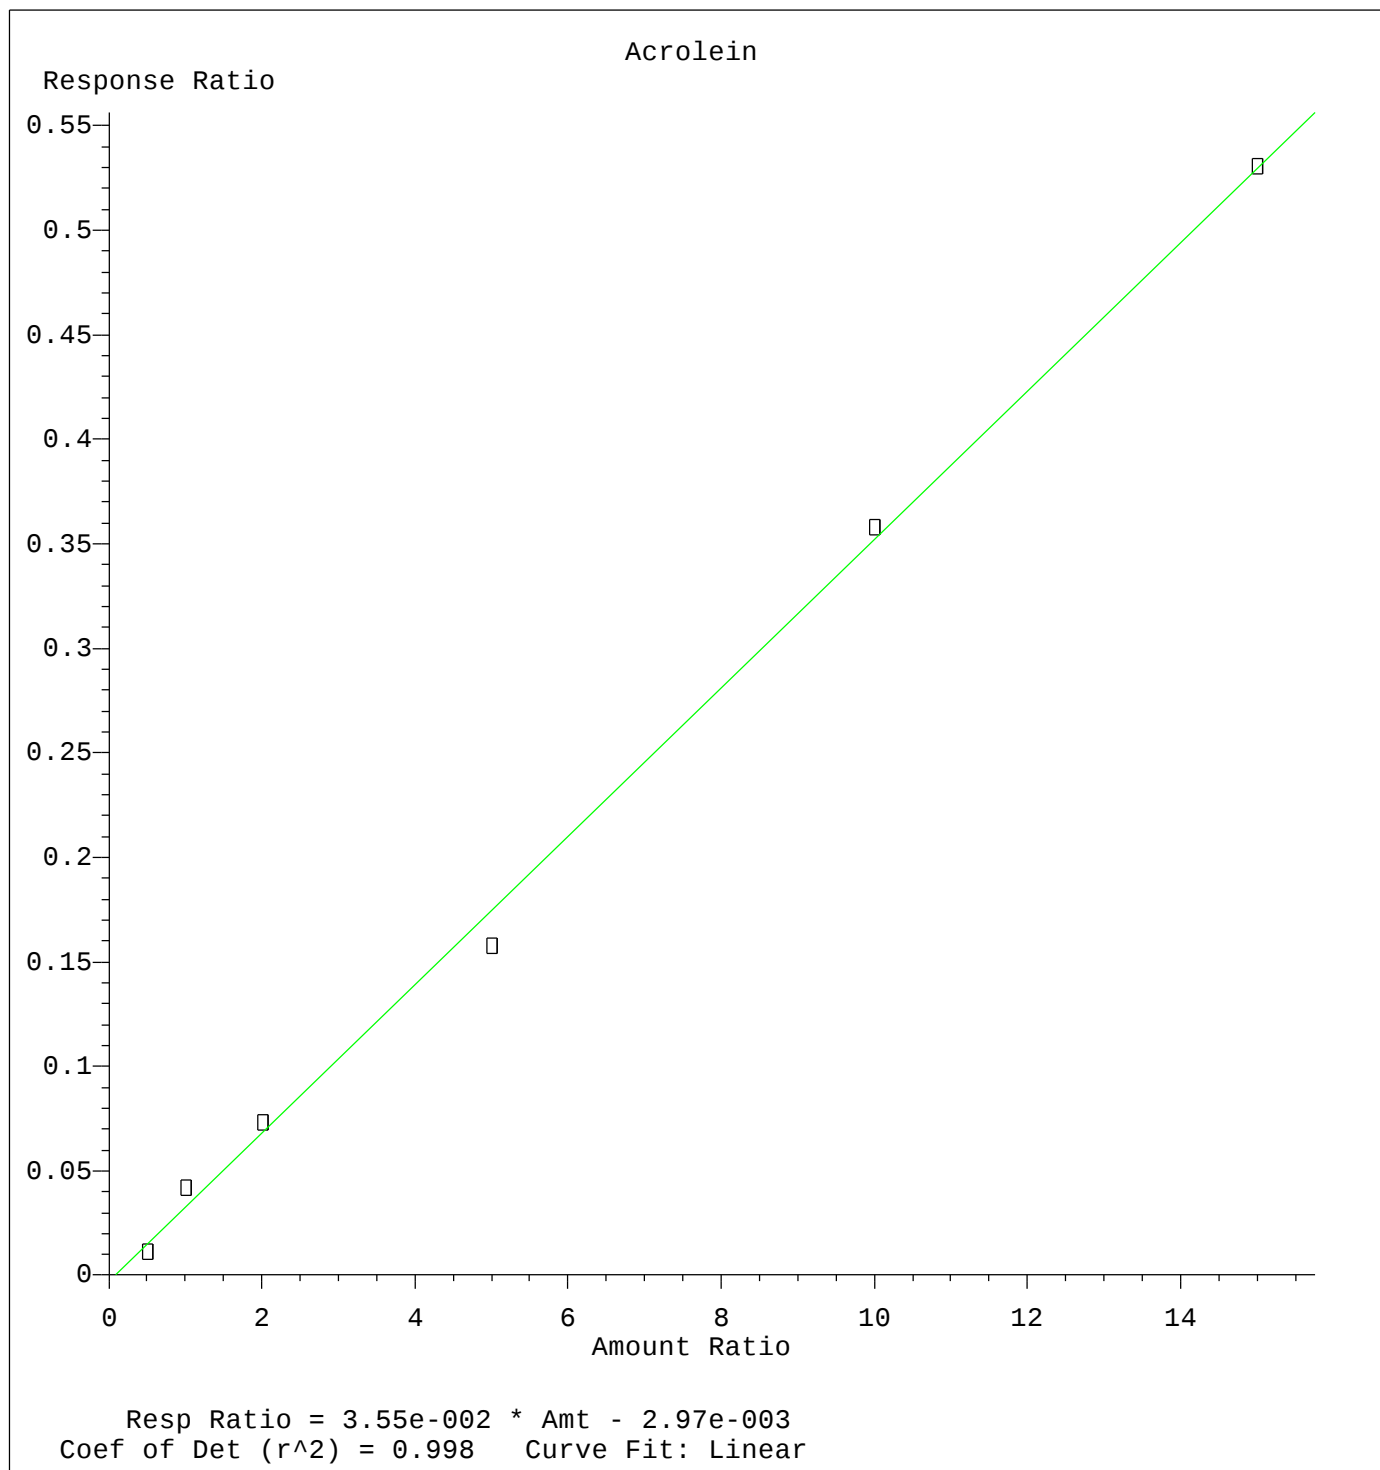

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W012419S.M
Calibration Table Last Updated: Fri Jan 25 11:07:41 2019