

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW012424\
 Data File : VW027849.D
 Acq On : 24 Jan 2024 10:39
 Operator : SY/MD
 Sample : VW0124SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jan 25 00:25:23 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jan 25 00:24:22 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	383724	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	351475	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	167162	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	101717	21.719	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	86.880%
7) Chloroethane-d5	2.899	69	71896	17.510	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.040%
11) 1,1-Dichloroethene-d2	4.021	65	45385	21.542	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	86.160%
21) 2-Butanone-d5	7.088	46	37812	48.824	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.640%
24) Chloroform-d	7.648	84	216806	23.366	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.480%
26) 1,2-Dichloroethane-d4	8.307	65	100689	23.952	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.800%
32) Benzene-d6	8.276	84	472957	23.709	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.840%
36) 1,2-Dichloropropane-d6	9.276	67	130677	23.678	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.720%
41) Toluene-d8	10.319	98	443401	23.776	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	95.120%
43) trans-1,3-Dichloroprop...	10.575	79	52143	24.307	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	97.240%
47) 2-Hexanone-d5	10.922	63	35190	48.577	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.160%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	94065	23.926	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.720%
66) 1,2-Dichlorobenzene-d4	13.849	152	149348	25.415	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	101.680%
Target Compounds						Qvalue
34) Trichloroethene	8.843	95	10272	1.937	ug/L #	3
39) cis-1,3-Dichloropropene	10.032	75	3364	0.467	ug/L #	67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW012424\
Data File : VW027849.D
Acq On : 24 Jan 2024 10:39
Operator : SY/MD
Sample : VW0124SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Jan 25 00:25:23 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010824SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jan 25 00:24:22 2024
Response via : Initial Calibration

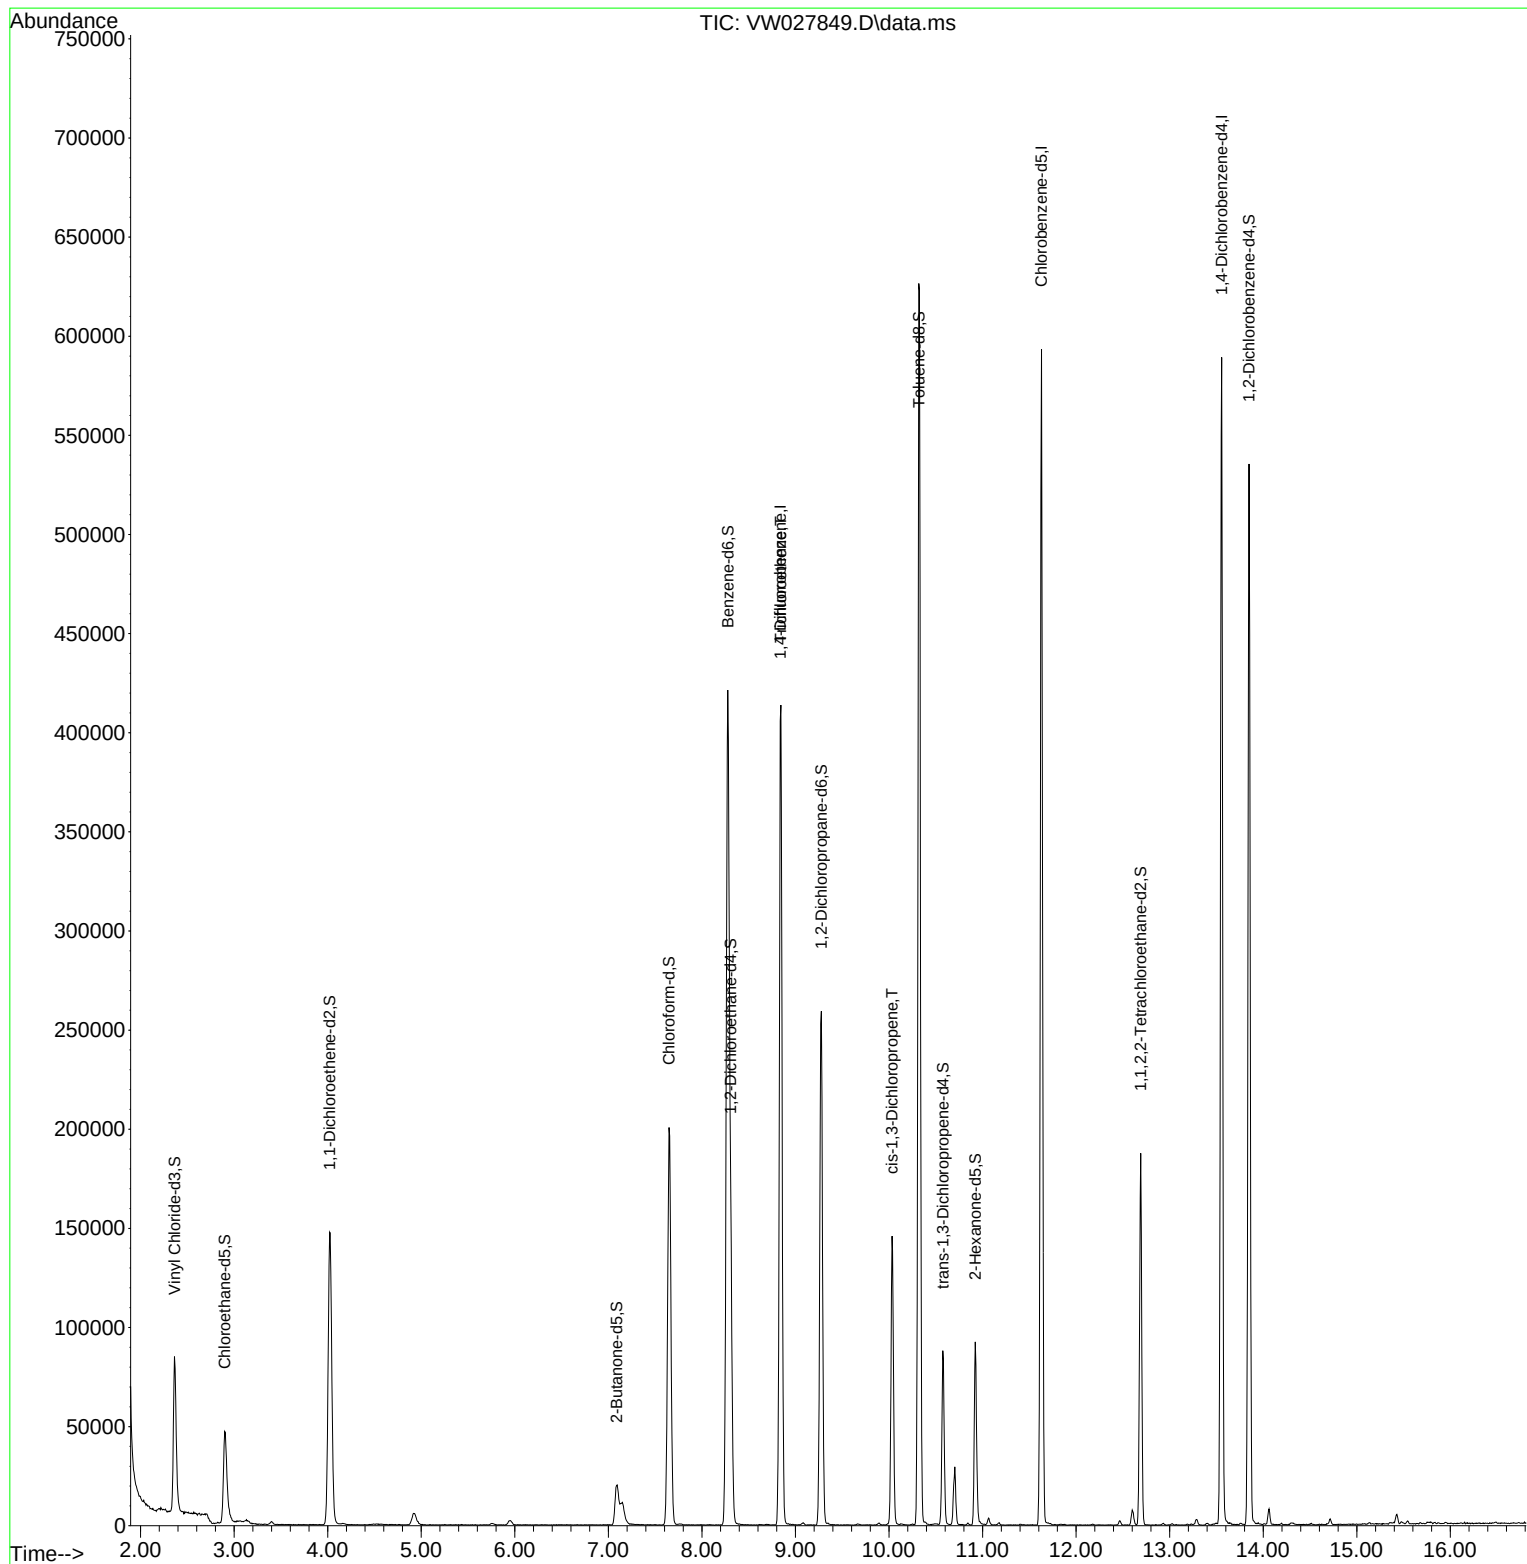



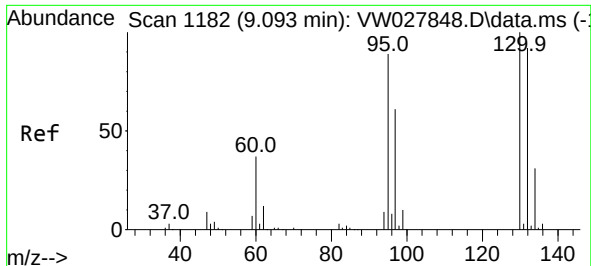


#34
 Trichloroethene
 Concen: 1.937 ug/L
 RT: 8.843 min Scan# 1182
 Delta R.T. -0.250 min
 Lab File: VW027849.D
 Acq: 24 Jan 2024 10:39

Instrument :
 MSVOA_W
 ClientSampleId :

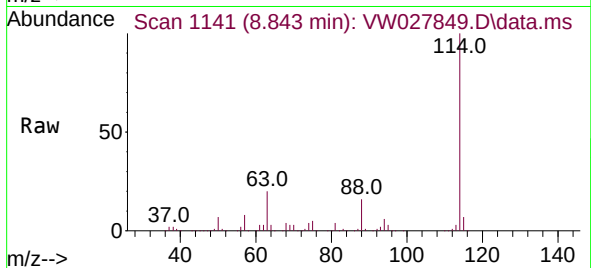

Tgt Ion: 95 Resp: 10272
 Ion Ratio Lower Upper
 95 100
 97 1.0 45.1 83.9#
 132 0.0 74.1 137.5#
 130 0.0 73.3 136.1#

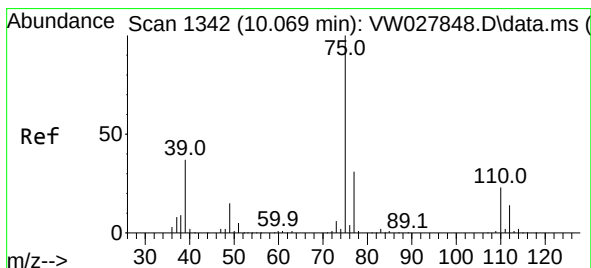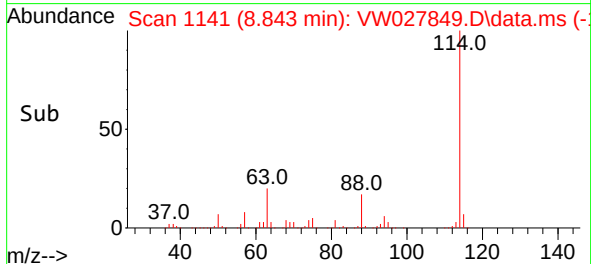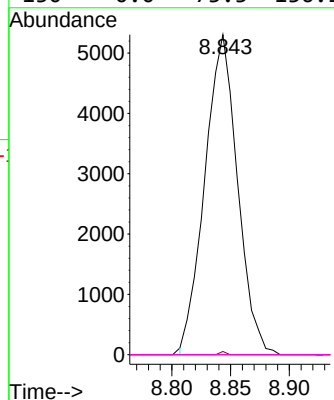

#39
 cis-1,3-Dichloropropene
 Concen: 0.467 ug/L
 RT: 10.032 min Scan# 1336
 Delta R.T. -0.036 min
 Lab File: VW027849.D
 Acq: 24 Jan 2024 10:39

Tgt Ion: 75 Resp: 3364
 Ion Ratio Lower Upper
 75 100
 77 49.4 21.7 40.3#

