
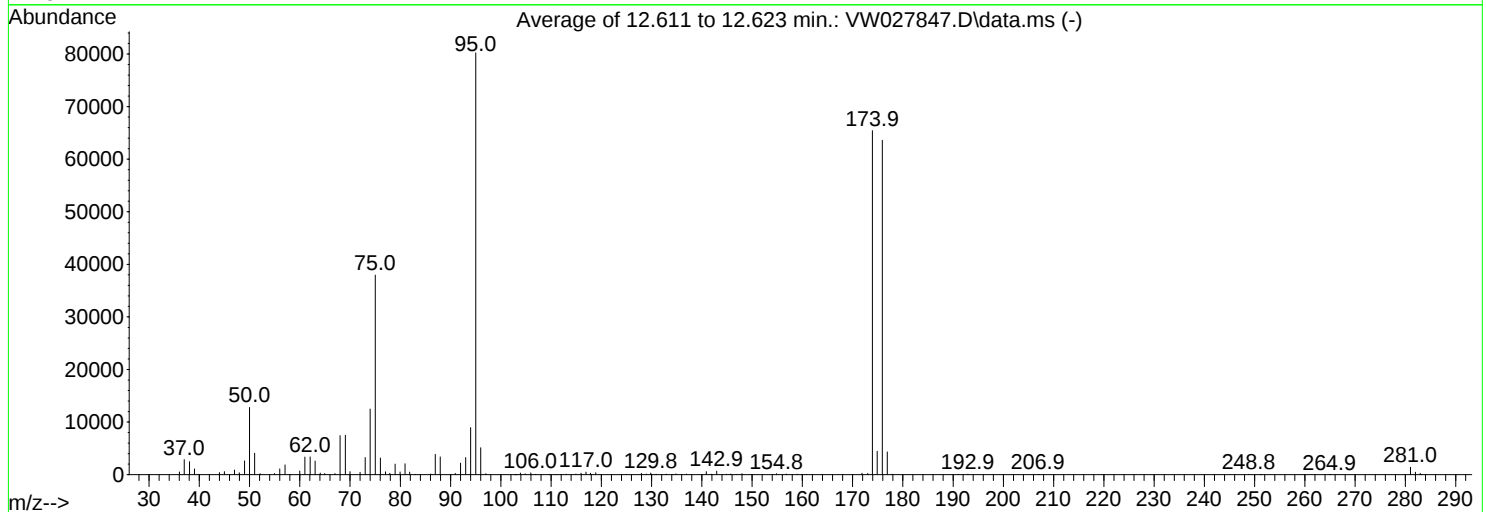


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW012424\
Data File : VW027847.D
Acq On : 24 Jan 2024 08:48
Operator : SY/MD
Sample : BFB426
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB426

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM010824SMA.M
Title : SFAM01.0
Last Update : Thu Jan 25 00:24:22 2024

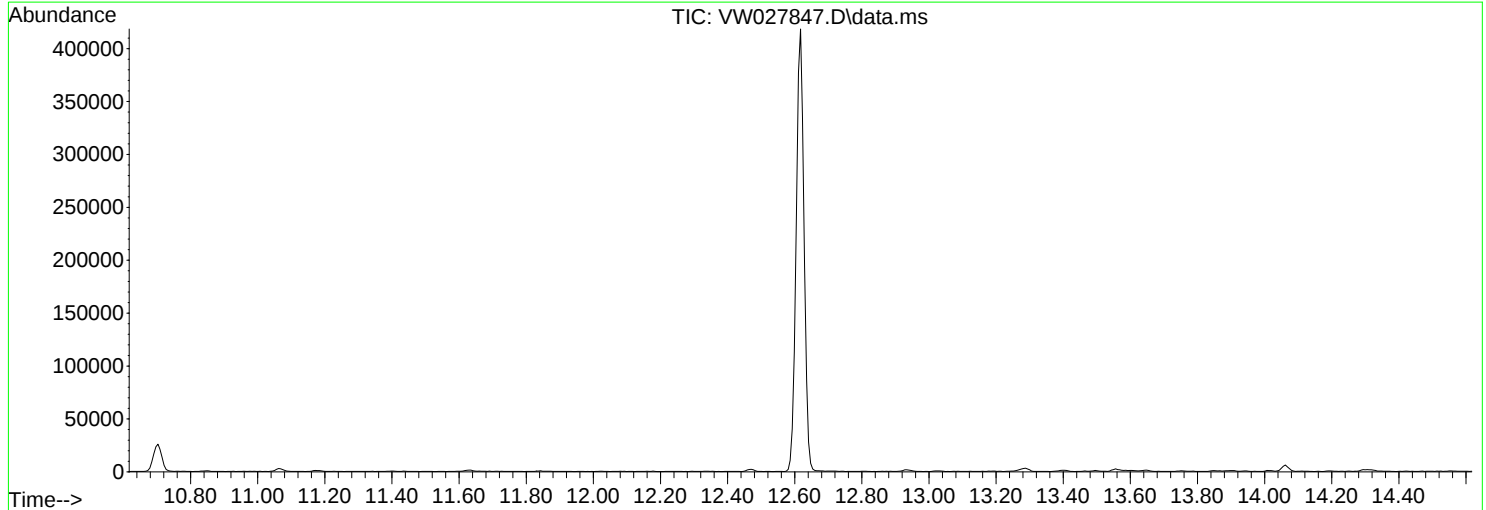

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.9	12793	PASS
75	95	30	80	47.3	37939	PASS
95	95	100	100	100.0	80221	PASS
96	95	5	9	6.4	5129	PASS
173	174	0.00	2	0.4	242	PASS
174	95	50	120	81.5	65413	PASS
175	174	5	9	6.8	4456	PASS
176	174	95	101	97.2	63605	PASS
177	176	5	9	6.8	4321	PASS

m/z	Abundance
39.90	362.0
43.90	122.0

Instrument :
MSVOA_W
ClientSampleId :
BFB426

m/z	Abundance
36.00	597.0
37.00	2874.0
38.10	2555.0
39.10	1253.0
40.10	339.0
44.10	531.0
45.00	617.0
47.00	884.0
48.10	308.0
49.00	2496.0
50.00	13342.0
51.00	4488.0
52.10	240.0
55.10	241.0
56.00	1149.0
57.00	1940.0
58.00	115.0
59.90	708.0
61.00	3545.0
62.00	3654.0
63.00	2653.0
64.00	307.0
64.90	181.0
67.00	199.0
68.00	7480.0
69.10	7477.0
70.00	638.0
72.00	466.0
73.00	3129.0
74.00	12903.0
75.00	39736.0
76.00	3523.0
77.10	509.0
77.90	291.0
78.90	2110.0
79.90	426.0
80.90	2169.0
81.90	431.0
86.00	131.0
87.00	3764.0
88.00	3444.0
90.90	236.0
92.00	2392.0
93.00	3197.0
94.00	8663.0
95.00	81272.0
96.00	5357.0
97.00	192.0
103.90	252.0
104.90	122.0
105.90	353.0
106.90	69.0
109.70	69.0
110.80	65.0
111.90	71.0
112.90	83.0
114.90	78.0
116.00	289.0
116.90	506.0
117.90	342.0
118.90	333.0
125.00	78.0
127.90	234.0
129.00	117.0
129.90	217.0
130.80	112.0
133.00	276.0
134.20	60.0
134.90	165.0
137.00	180.0
140.90	553.0
141.90	138.0
142.90	516.0
144.90	142.0
145.80	89.0
146.80	76.0
148.00	233.0
149.90	77.0
154.90	180.0
156.80	108.0
158.90	88.0
160.80	67.0
171.80	323.0
174.00	61392.0
174.90	3791.0
175.90	62152.0
176.90	3836.0
177.80	166.0
191.00	167.0
193.00	195.0
206.90	125.0
248.90	148.0

Instrument :
MSVOA_W
ClientSampleId :
BFB426

251.10	51.0
264.90	150.0
281.00	2407.0
282.00	753.0
283.00	408.0

Instrument :
MSVOA_W
ClientSampleId :
BFB426

m/z	Abundance
36.10	416.0
37.00	3306.0
38.00	2760.0
39.10	1201.0
40.10	342.0
44.00	651.0
45.00	579.0
47.00	977.0
47.90	501.0
49.00	2888.0
50.00	14637.0
51.00	4607.0
52.10	163.0
54.90	226.0
56.00	1325.0
57.10	2002.0
58.20	78.0
60.00	785.0
61.00	3568.0
62.00	3634.0
63.10	3063.0
64.00	365.0
65.00	212.0
67.00	190.0
68.00	8307.0
69.00	8523.0
70.00	594.0
72.00	472.0
73.00	3828.0
74.00	13800.0
75.00	41632.0
76.10	3427.0
77.10	607.0
77.90	275.0
78.90	2186.0
80.00	648.0
81.00	2396.0
81.90	530.0
83.10	85.0
86.00	116.0
86.90	4305.0
87.90	3602.0
91.00	281.0
92.00	2321.0
93.00	3758.0
94.00	9936.0
95.00	86888.0
96.00	5512.0
97.00	225.0
102.70	53.0
103.10	53.0
103.90	392.0
104.90	192.0
105.90	414.0
106.90	78.0
109.70	81.0
110.80	51.0
113.00	112.0
114.90	157.0
115.90	336.0
117.00	454.0
117.80	231.0
118.80	435.0
125.00	71.0
127.90	299.0
128.90	118.0
129.90	391.0
130.90	68.0
132.70	60.0
134.90	144.0
137.00	102.0
140.90	604.0
141.90	93.0
142.90	787.0
145.00	81.0
145.80	155.0
146.90	102.0
148.00	160.0
149.90	102.0
154.90	203.0
156.80	131.0
159.00	89.0
160.80	111.0
171.90	263.0
173.00	725.0
174.00	73672.0
174.90	5700.0
175.90	70976.0
176.90	4959.0
178.00	180.0
191.00	63.0
192.90	89.0

Instrument :
MSVOA_W
ClientSampleId :
BFB426

206.90	87.0
248.80	66.0
265.10	79.0
281.00	1335.0
282.00	451.0
283.00	258.0

Instrument :
MSVOA_W
ClientSampleId :
BFB426

m/z	Abundance
36.00	530.0
37.00	2418.0
38.10	2050.0
39.00	878.0
40.00	377.0
44.00	352.0
45.00	501.0
47.00	784.0
47.90	281.0
49.00	2473.0
50.00	10399.0
51.00	3106.0
52.00	115.0
54.80	148.0
56.00	797.0
57.00	1624.0
58.00	99.0
60.10	645.0
61.00	2966.0
62.10	2861.0
63.00	2087.0
64.10	247.0
65.00	238.0
67.00	228.0
68.00	6493.0
69.00	6433.0
70.00	478.0
72.00	409.0
73.00	2843.0
74.00	10782.0
75.00	32448.0
76.10	2528.0
77.00	565.0
77.90	265.0
79.00	1779.0
79.90	526.0
81.00	1635.0
81.80	474.0
83.00	67.0
86.10	96.0
87.00	3577.0
87.90	3072.0
91.00	218.0
92.00	1838.0
93.00	2837.0
94.00	8232.0
95.00	72504.0
96.00	4518.0
97.00	141.0
103.90	243.0
104.80	144.0
106.00	278.0
107.00	60.0
109.70	61.0
111.00	69.0
112.00	74.0
113.10	54.0
115.00	101.0
116.00	215.0
116.90	471.0
117.90	231.0
119.00	324.0
128.00	230.0
128.90	98.0
129.80	329.0
131.00	126.0
134.80	118.0
136.80	103.0
140.90	619.0
141.70	63.0
143.00	679.0
144.80	71.0
145.70	154.0
148.00	204.0
150.00	57.0
154.80	188.0
156.80	136.0
159.00	80.0
171.90	263.0
173.90	61176.0
174.90	3876.0
175.90	57688.0
176.90	4168.0
178.00	94.0
207.10	123.0
265.10	51.0
280.90	464.0
282.00	214.0
282.80	105.0
283.20	116.0

Instrument :
MSVOA_W
ClientSampleId :
BFB426