

Data File : VW014770.D
Acq On : 27 Jan 2020 17:28
Operator : SY/VA
Sample : L1193-14
Misc : 5.10G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK01

Quant Time: Jan 28 07:21:25 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM012720S.M
Quant Title : VOC Analysis
QLast Update : Tue Jan 28 07:18:57 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	935071	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	853925	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	367406	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	352692	23.81	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.24%
7) Chloroethane-d5	2.89	69	283528	22.53	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.12%
10) 1,1-Dichloroethene-d2	4.01	63	474764	17.72	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	70.88%
20) 2-Butanone-d5	7.07	46	220328	52.39	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	104.78%
24) Chloroform-d	7.65	84	617115	23.91	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.64%
26) 1,2-Dichloroethane-d4	8.30	65	349246	25.13	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	100.52%
29) Benzene-d6	8.27	84	1302197	24.23	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	96.92%
33) 1,2-Dichloropropane-d6	9.27	67	408217	24.44	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	97.76%
37) Toluene-d8	10.32	98	1146953	23.96	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	95.84%
38) trans-1,3-Dichloropropene-	10.57	79	159438	23.95	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	95.80%
39) 2-Hexanone-d5	10.92	63	170612	54.42	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	108.84%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	330934	25.24	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	100.96%
61) 1,2-Dichlorobenzene-d4	13.85	152	372639	25.88	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	103.52%


Target Compounds					Qvalue
59) 1,2,3-Trichloropropane	13.55	75	44539	4.862 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VW014770.D
Acq On : 27 Jan 2020 17:28
Operator : SY/VA
Sample : L1193-14
Misc : 5.10G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK01

Quant Time: Jan 28 07:21:25 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM012720S.M
Quant Title : VOC Analysis
QLast Update : Tue Jan 28 07:18:57 2020
Response via : Initial Calibration

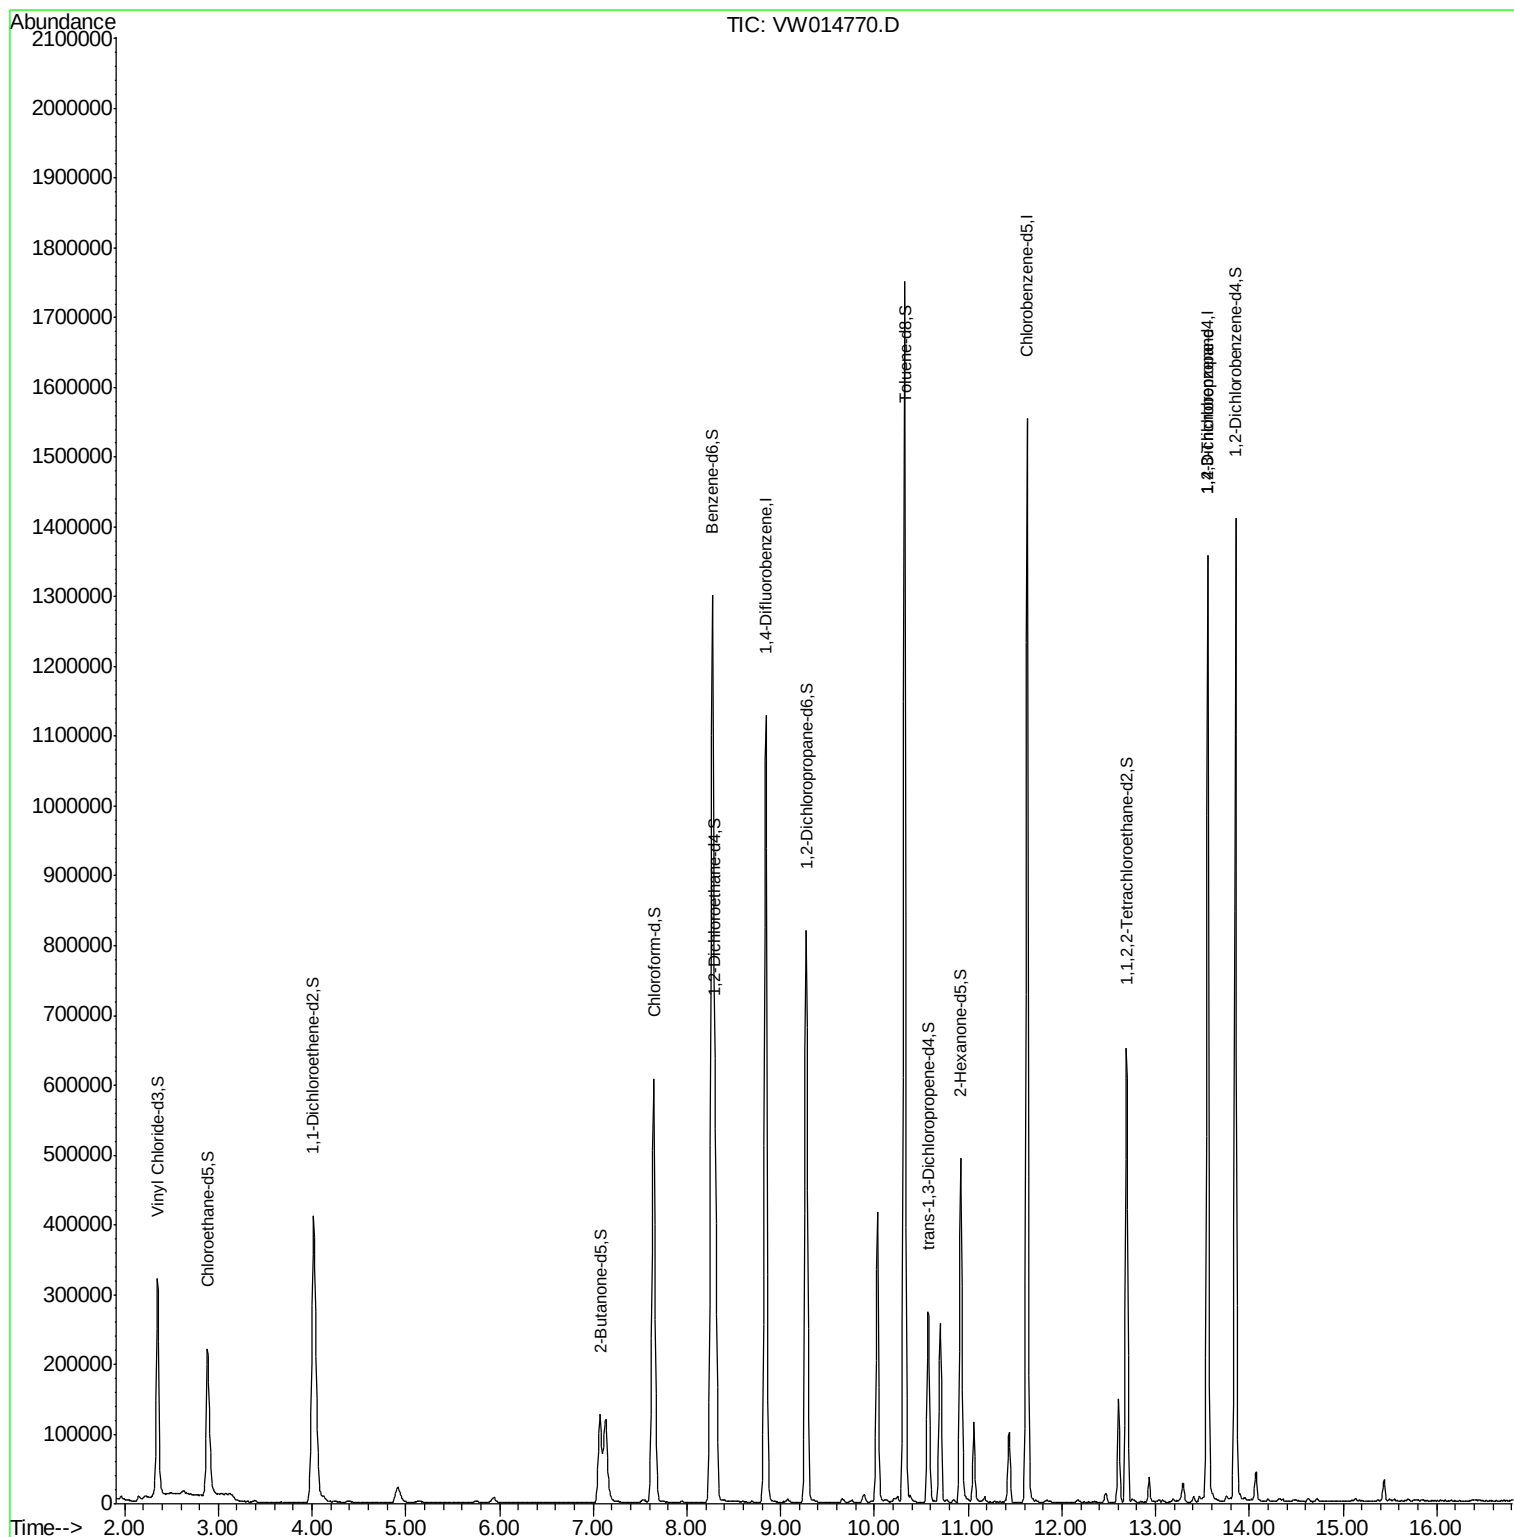

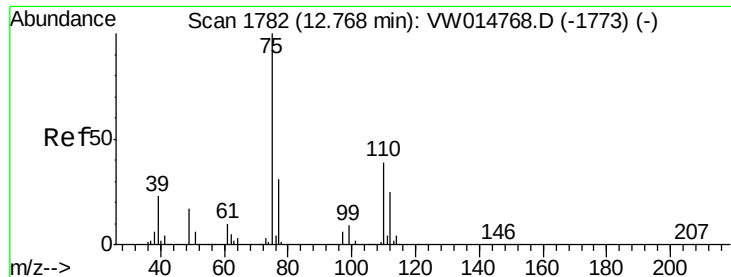

#59

1,2,3-Trichloropropane

Concen: 4.862 ug/L

RT: 13.55 min Scan# 1911

Delta R.T. 0.79 min

Lab File: VW014770.D

Acq: 27 Jan 2020 17:28

Instrument :

MSVOA_W

ClientSampleId :

VHBLK01

Tgt Ion: 75 Resp: 44539

Ion Ratio Lower Upper

75 100

77 35.6 25.8 38.8

