

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW012720\
Quantitation Report (Qedit)




Data File : VW014774.D
Acq On : 27 Jan 2020 19:13
Operator : SY/VA
Sample : L1271-12
Misc : 5.04G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GAT03

Manual Integrations
APPROVED

MMDadoda
1/28/2020 1:58:14 PM

Quant Time: Jan 28 07:21:47 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM012720S.M
Quant Title : VOC Analysis
QLast Update : Tue Jan 28 07:18:57 2020
Response via : Initial Calibration

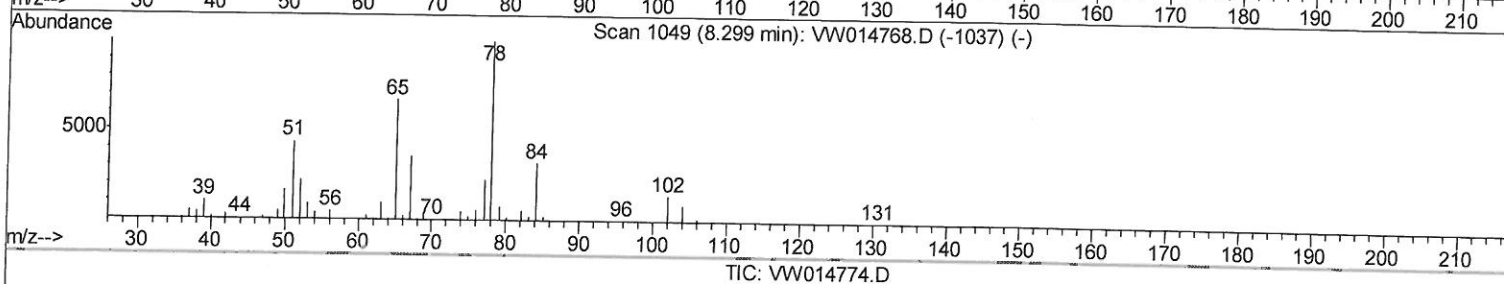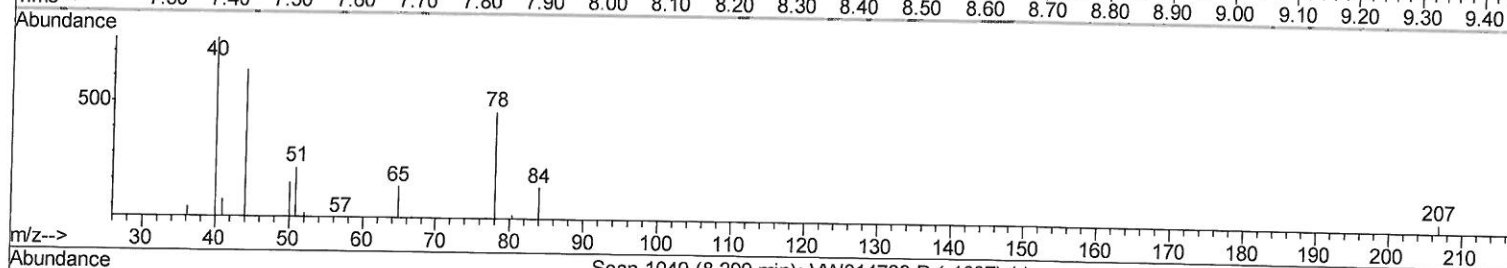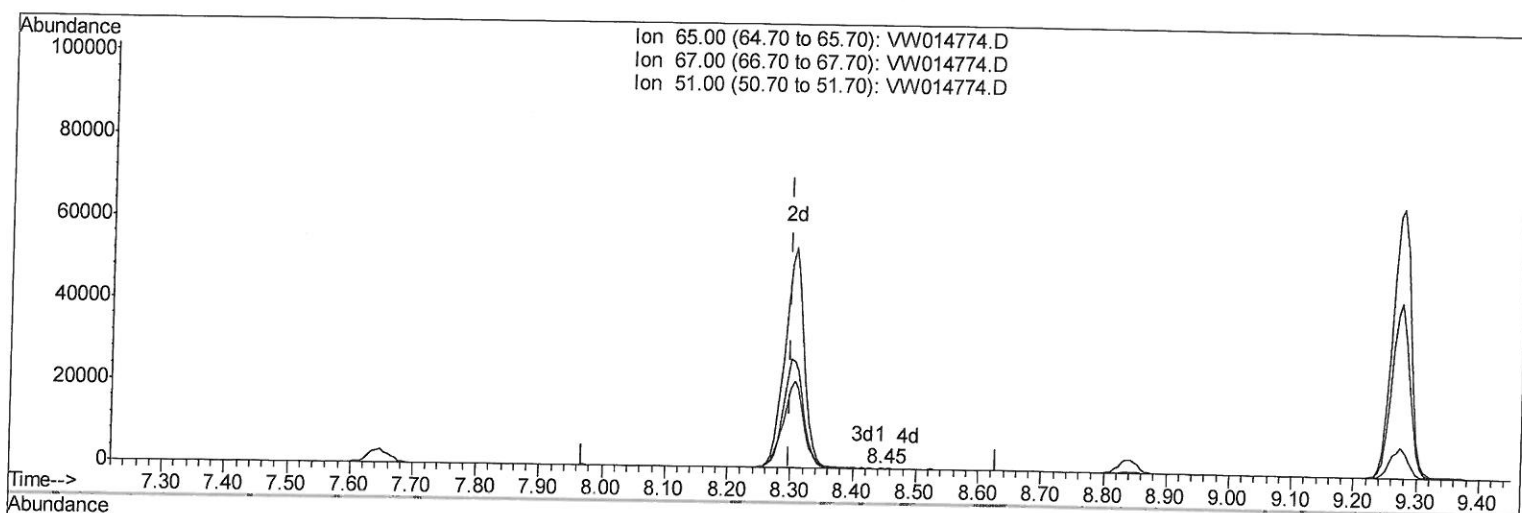

(26) 1,2-Dichloroethane-d4 (S)

8.445min (+0.146) 0.03ug/L

response 157

Ion	Exp%	Act%
65.00	100	100
67.00	53.40	61.15
51.00	102.70	113.38
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW012720\
Quantitation Report (Qedit)




Data File : VW014774.D
Acq On : 27 Jan 2020 19:13
Operator : SY/VA
Sample : L1271-12
Misc : 5.04G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GAT03

Manual Integrations
APPROVED

MMDadoda
1/28/2020 1:58:14 PM

Quant Time: Jan 28 07:21:47 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM012720S.M
Quant Title : VOC Analysis
QLast Update : Tue Jan 28 07:18:57 2020
Response via : Initial Calibration

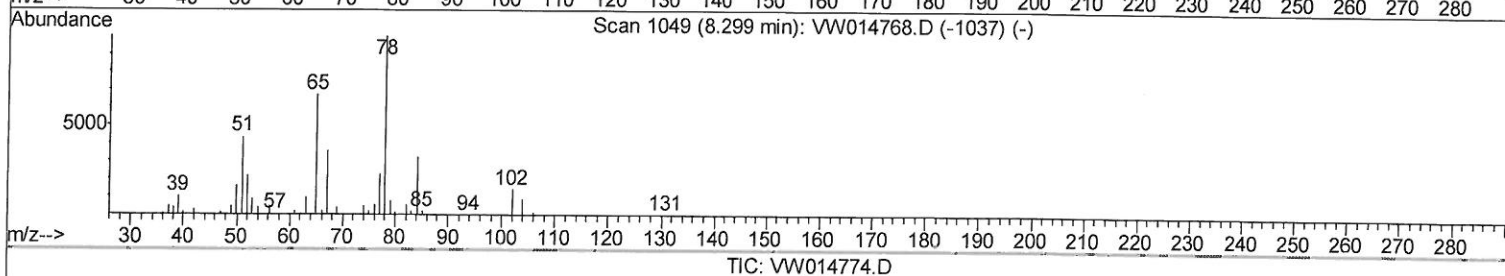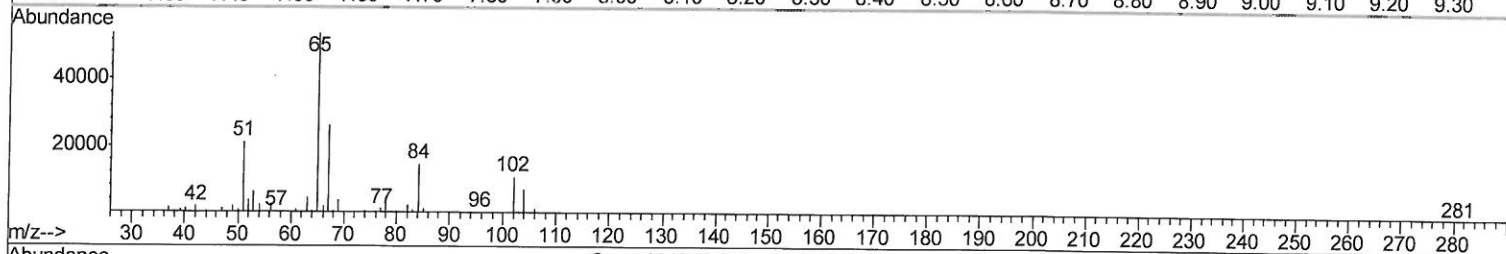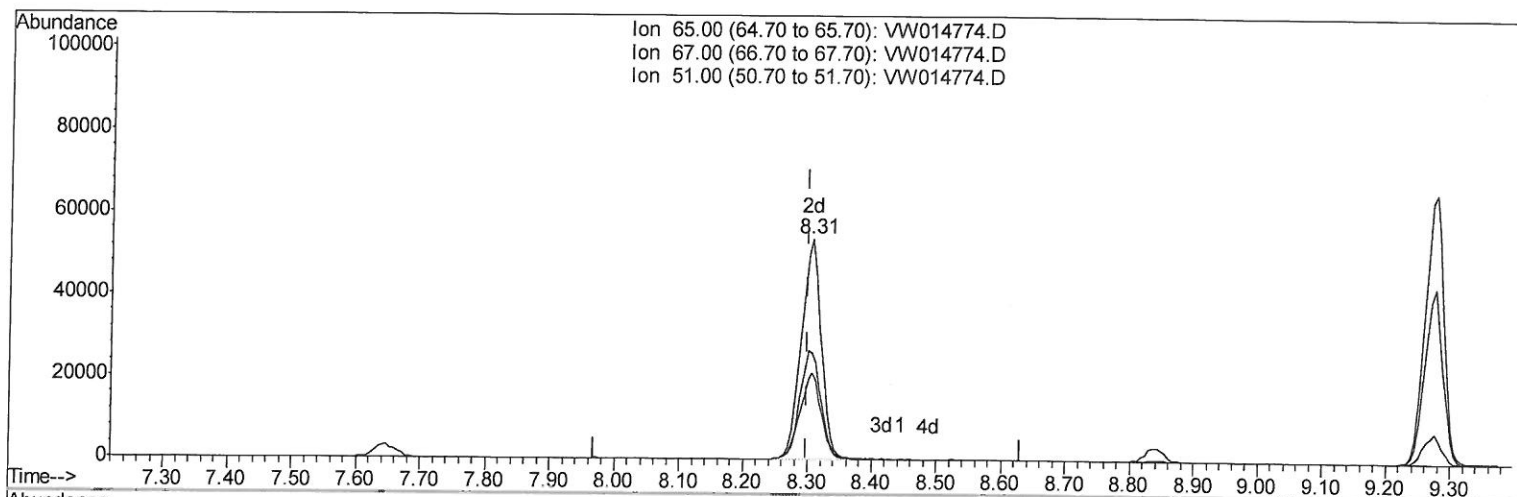

(26) 1,2-Dichloroethane-d4 (S)

8.305min (+0.006) 22.26ug/L m

response 115719

Ion	Exp%	Act%
65.00	100	100
67.00	53.40	0.08#
51.00	102.70	0.15#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW012720\

Quantitation Report (QT Reviewed)

Data File : VW014774.D

Acq On : 27 Jan 2020 19:13

Operator : SY/VA

Sample : L1271-12

Misc : 5.04G/10ML/MSVOA_W/SOIL

ALS Vial : 1 Sample Multiplier: 1

Instrument :

MSVOA_W

ClientSampleId :

GAT03

Manual Integrations
APPROVEDMMDadoda
1/28/2020 1:58:14 PM

Quant Time: Jan 28 07:49:02 2020

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM012720S.M

Quant Title : VOC Analysis

QLast Update : Tue Jan 28 07:18:57 2020

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	349720	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	312306	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	123937	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	131608	23.76	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.04%
7) Chloroethane-d5	2.89	69	100824	21.42	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.68%
10) 1,1-Dichloroethene-d2	4.01	63	161570	16.12	ug/L	-0.01
Spiked Amount	25.000	Range	45 - 110	Recovery	=	64.48%
20) 2-Butanone-d5	7.08	46	63856	40.60	ug/L	0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	81.20%
24) Chloroform-d	7.65	84	204160	21.15	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	84.60%
26) 1,2-Dichloroethane-d4	8.31	65	115719m	22.26	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	89.04%
29) Benzene-d6	8.27	84	409717	20.84	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	83.36%
33) 1,2-Dichloropropane-d6	9.27	67	131987	21.60	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	86.40%
37) Toluene-d8	10.32	98	336704	19.23	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	76.92%
38) trans-1,3-Dichloropropene-	10.57	79	47725	19.60	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	78.40%
39) 2-Hexanone-d5	10.92	63	42836	37.36	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	74.72%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	104056	21.70	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	86.80%
61) 1,2-Dichlorobenzene-d4	13.85	152	106203	21.87	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	87.48%

Target Compounds

					Qvalue
13) Acetone	4.13	43	8954	5.315	ug/L 83
16) Methylene chloride	4.91	84	10993	1.860	ug/L 97
34) Benzene	8.32	78	17482	0.874	ug/L 100
44) Toluene	10.38	91	47518	2.338	ug/L 98
54) m,p-Xylene	11.83	106	28565	3.441	ug/L 86
55) o-xylene	12.16	106	18031	2.315	ug/L 98

(#)=qualifier out of range (m)=manual integration (+)=signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW012720\
Quantitation Report (QT Reviewed)
Data File : VW014774.D
Acq On : 27 Jan 2020 19:13
Operator : SY/VA
Sample : L1271-12
Misc : 5.04G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
GAT03

Manual Integrations
APPROVED

MMDadoda
1/28/2020 1:58:14 PM

Quant Time: Jan 28 07:49:02 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM012720S.M
Quant Title : VOC Analysis
QLast Update : Tue Jan 28 07:18:57 2020
Response via : Initial Calibration

