

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW012720\
 Data File : VW014778.D
 Acq On : 27 Jan 2020 20:58
 Operator : SY/VA
 Sample : L1271-16
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 GAT07

Manual Integrations
 APPROVED

MMDadoda
 1/28/2020 1:59:00 PM

Quant Time: Jan 28 08:22:14 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM012720S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jan 28 07:18:57 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	1009477	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	925928	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	420640	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	360015	22.52	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.08%
7) Chloroethane-d5	2.89	69	290391	21.38	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	85.52%
10) 1,1-Dichloroethene-d2	4.01	63	463792	16.03	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	64.12%
20) 2-Butanone-d5	7.07	46	257216	56.65	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	113.30%
24) Chloroform-d	7.64	84	634504	22.77	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	91.08%
26) 1,2-Dichloroethane-d4	8.30	65	379859	25.31	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	101.24%
29) Benzene-d6	8.27	84	1339473	22.98	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	91.92%
33) 1,2-Dichloropropane-d6	9.27	67	428724	23.67	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	94.68%
37) Toluene-d8	10.32	98	1174374	22.62	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.48%
38) trans-1,3-Dichloropropene-	10.57	79	177924	24.65	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	98.60%
39) 2-Hexanone-d5	10.92	63	193269	56.85	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	113.70%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	364182	25.62	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	102.48%
61) 1,2-Dichlorobenzene-d4	13.85	152	398339	24.16	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.64%

Target Compounds				Ovalue
13) Acetone	4.12	43	16794m	3.454 ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW012720\
Data File : VW014778.D
Acq On : 27 Jan 2020 20:58
Operator : SY/VA
Sample : L1271-16
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
GAT07

Manual Integrations
APPROVED

MMDadoda
1/28/2020 1:59:00 PM

Quant Time: Jan 28 08:22:14 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM012720S.M
Quant Title : VOC Analysis
QLast Update : Tue Jan 28 07:18:57 2020
Response via : Initial Calibration

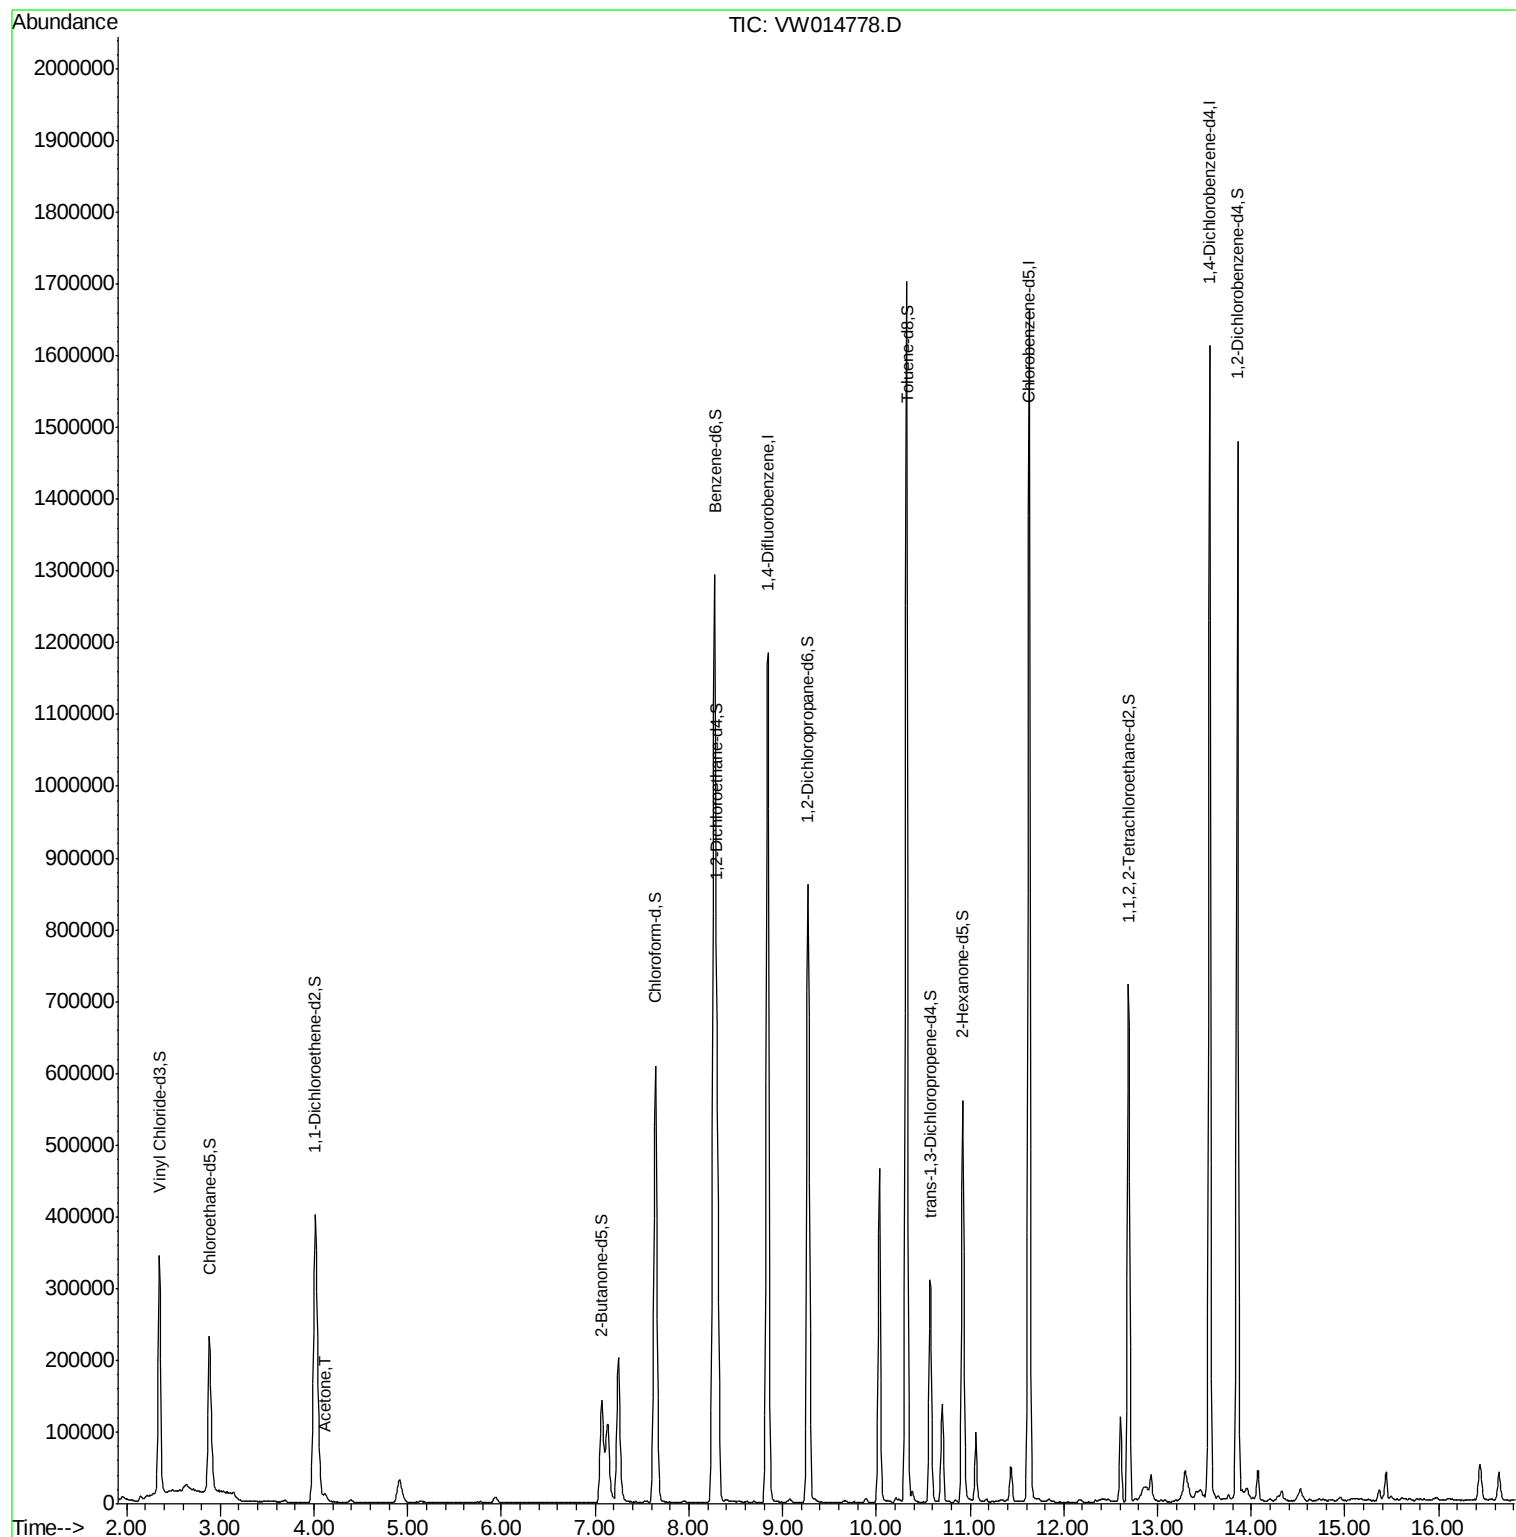

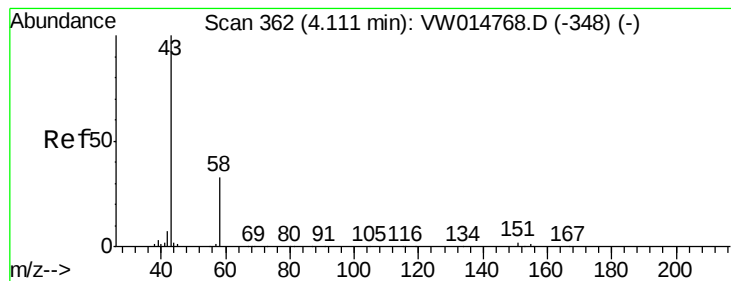

#13

Acetone

Concen: 3.454 ug/L m

RT: 4.12 min Scan# 363

Delta R.T. 0.01 min

Lab File: VW014778.D

Acq: 27 Jan 2020 20:58

Instrument :

MSVOA_W

ClientSampleId :

GAT07

Tot Ion: 43 Resp: 16794

Ion Ratio Lower Upper

43 100

58 29.1 0.0 64.6

Manual Integrations

APPROVED

MMDadoda

1/28/2020 1:59:00 PM

