

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW012920\
 Data File : VW014795.D
 Acq On : 29 Jan 2020 15:25
 Operator : SY/VA
 Sample : L1303-05
 Misc : 5.94G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AF0

Manual Integrations
 APPROVED

MMDadoda
 1/30/2020 5:33:21 PM

Quant Time: Jan 30 07:33:13 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM012720S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jan 30 07:05:48 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	1204527	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	1068248	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	441315	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	395292	20.72	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.88%
7) Chloroethane-d5	2.89	69	324011	19.99	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.96%
10) 1,1-Dichloroethene-d2	4.02	63	576661	16.70	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.80%
20) 2-Butanone-d5	7.07	46	152800	28.21	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	56.42%
24) Chloroform-d	7.65	84	662539	19.93	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	79.72%
26) 1,2-Dichloroethane-d4	8.31	65	318079	17.76	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	71.04%
29) Benzene-d6	8.27	84	1338644	19.91	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	79.64%
33) 1,2-Dichloropropane-d6	9.27	67	406622	19.46	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	77.84%
37) Toluene-d8	10.32	98	1210713	20.21	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	80.84%
38) trans-1,3-Dichloropropene-	10.57	79	155576	18.68	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	74.72%
39) 2-Hexanone-d5	10.92	63	112230	28.62	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	57.24%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	246136	15.01	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	60.04%
61) 1,2-Dichlorobenzene-d4	13.85	152	340612	19.69	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	78.76%

Target Compounds

					Ovalue
13) Acetone	4.12	43	32954	5.680 ug/L	97
16) Methylene chloride	4.92	84	45524	2.236 ug/L	94
18) trans-1,2-Dichloroethene	5.43	96	8764m	0.516 ug/L	
22) cis-1,2-Dichloroethene	7.17	96	397782	22.364 ug/L	99
35) Trichloroethene	9.09	95	11809	0.679 ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW012920\
Data File : VW014795.D
Acq On : 29 Jan 2020 15:25
Operator : SY/VA
Sample : L1303-05
Misc : 5.94G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
C0AF0

Manual Integrations
APPROVED

MMDadoda
1/30/2020 5:33:21 PM

Quant Time: Jan 30 07:33:13 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM012720S.M
Quant Title : VOC Analysis
QLast Update : Thu Jan 30 07:05:48 2020
Response via : Initial Calibration

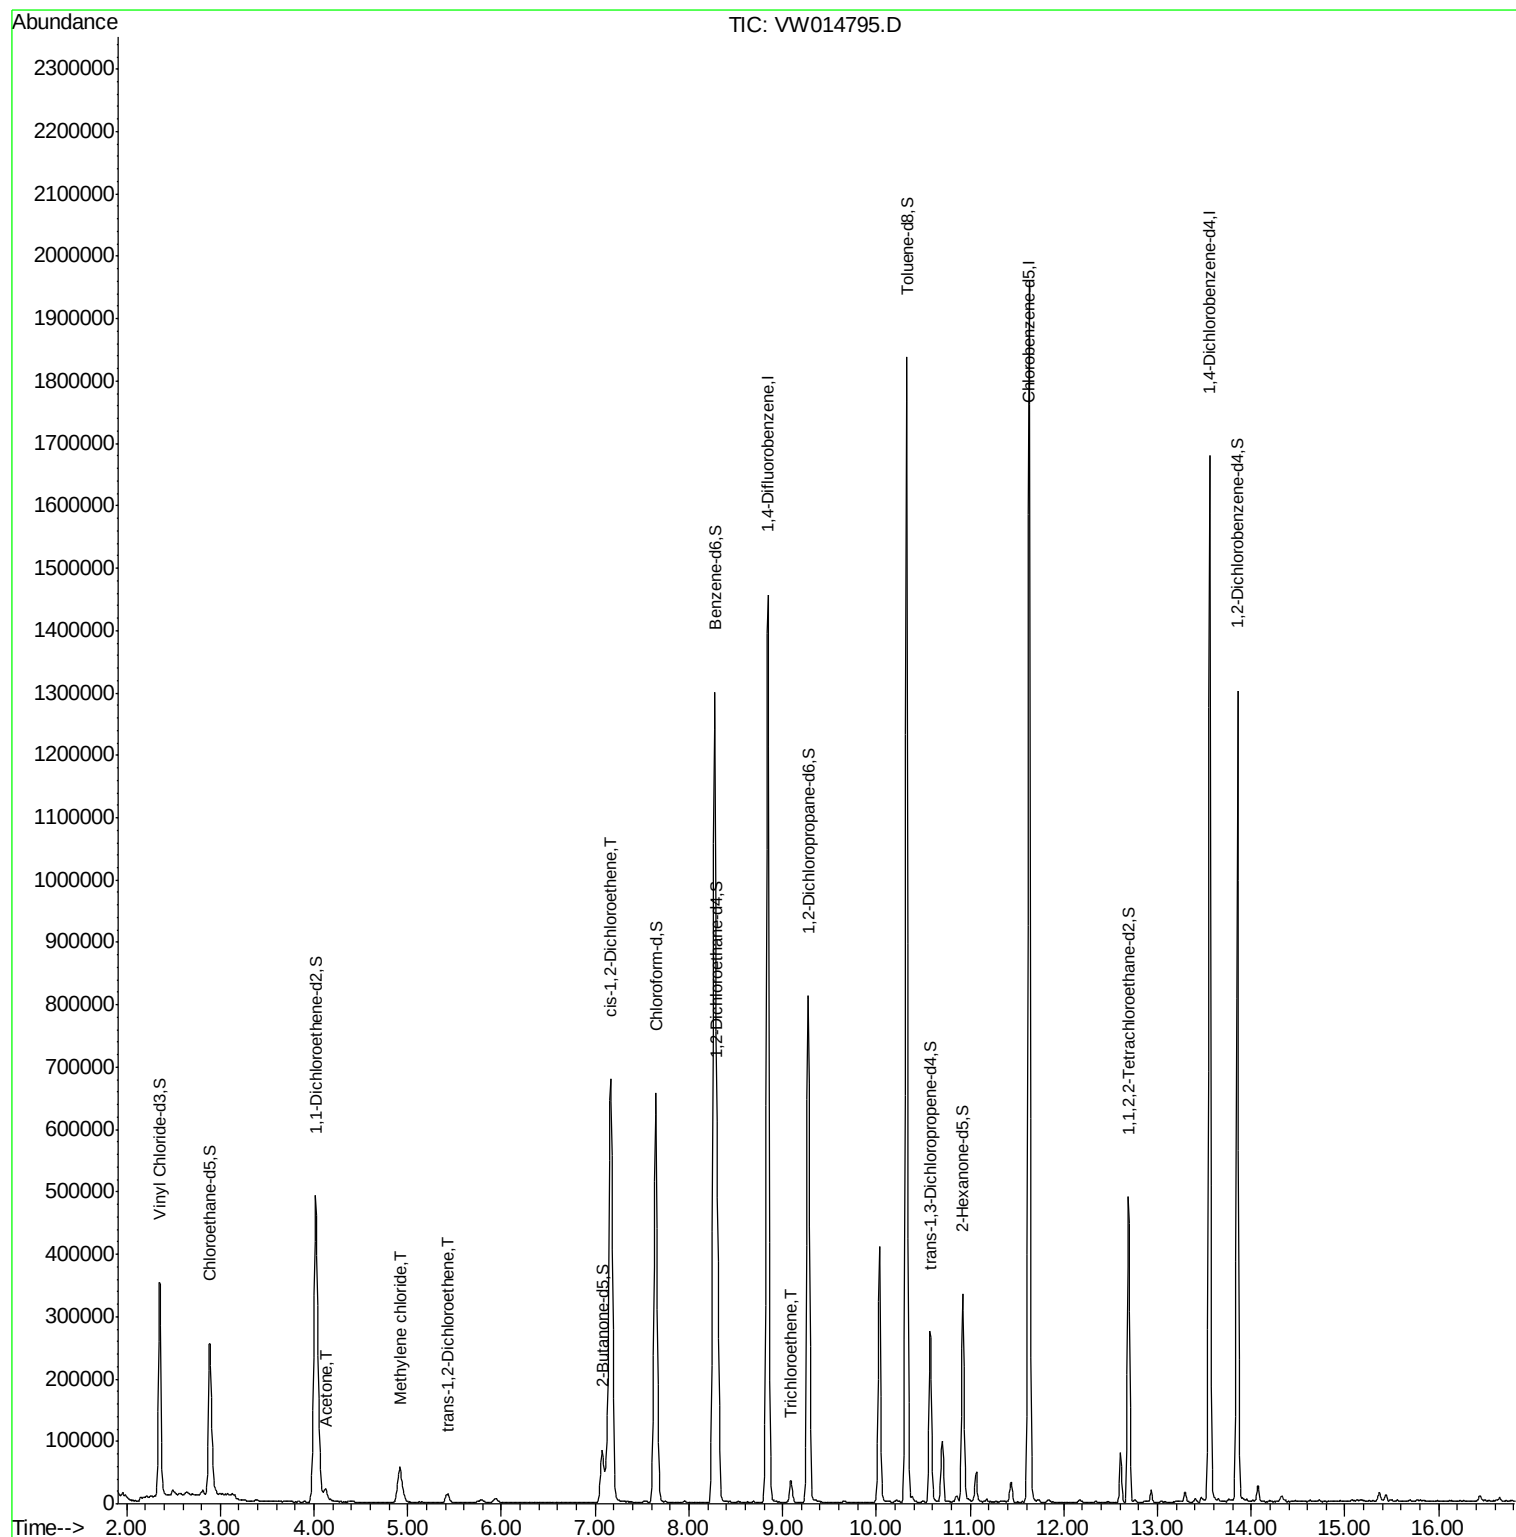

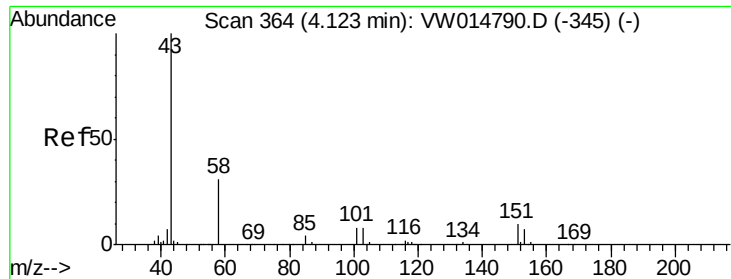





#13
Acetone
Concen: 5.680 ug/L
RT: 4.12 min Scan# 364
Delta R.T. -0.00 min
Lab File: VW014795.D
Acq: 29 Jan 2020 15:25

Instrument :
MSVOA_W
ClientSampled :
C0AF0

Tot Ion	43	Resp	32954
Ion Ratio	100	Lower	Upper
43	100	0.0	64.6
58	30.7		




Manual Integrations
APPROVED


MMDadoda
1/30/2020 5:33:21 PM

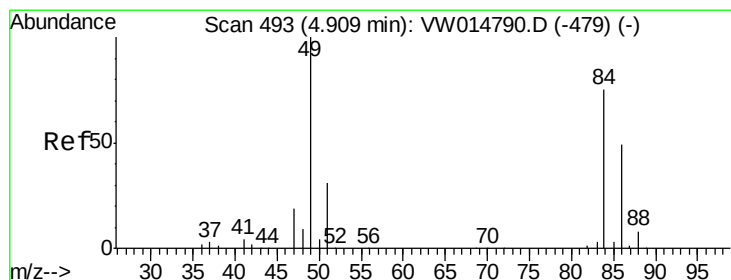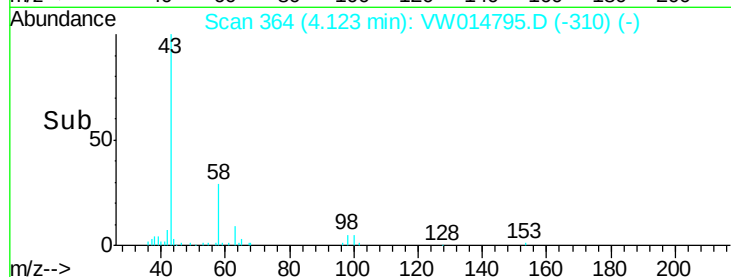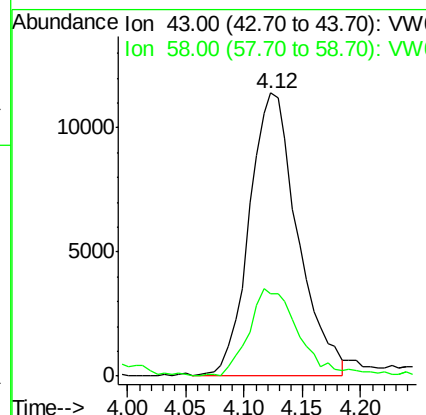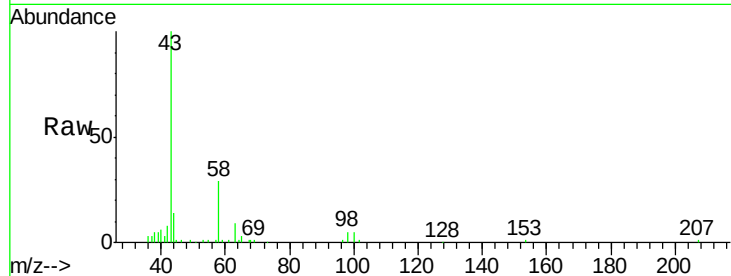

#16
Methylene chloride
Concen: 2.236 ug/L
RT: 4.92 min Scan# 494
Delta R.T. 0.01 min
Lab File: VW014795.D
Acq: 29 Jan 2020 15:25

Tgt Ion	84	Resp	45524
Ion Ratio	100	Lower	Upper
84	100	90.9	168.7
49	140.6	43.5	80.7
86	61.7		

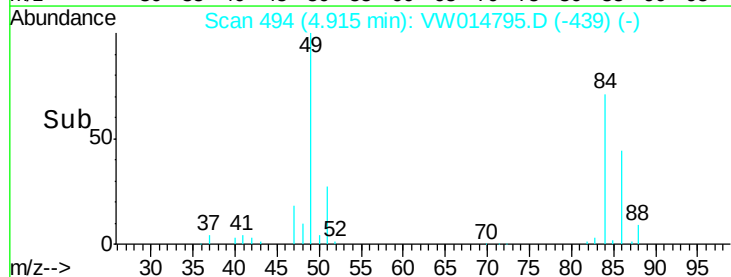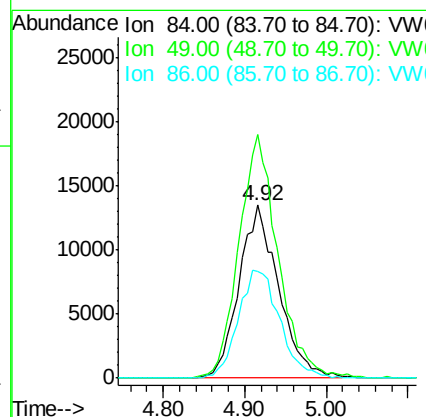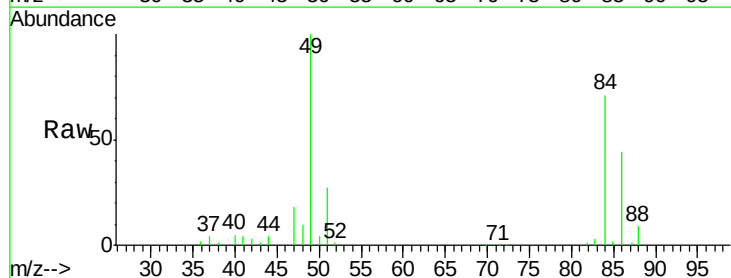

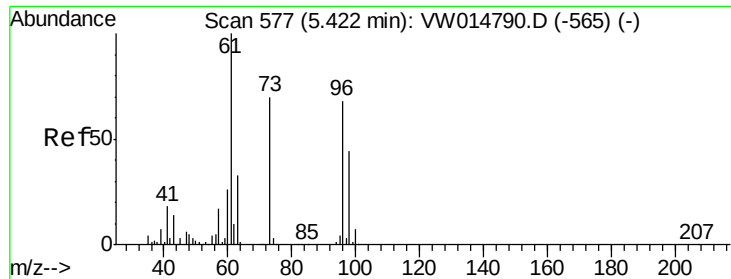

#18

trans-1,2-Dichloroethene

Concen: 0.516 ug/L m

RT: 5.43 min Scan# 578

Delta R.T. 0.01 min

Lab File: VW014795.D

Acq: 29 Jan 2020 15:25

Instrument :

MSVOA_W





ClientSampled :

C0AF0

Tot Ion:	96	Resp:	8764
Ion	Ratio	Lower	Upper
96	100		
61	129.6	100.2	186.0
98	55.0	43.1	80.1

Manual Integrations
APPROVED

MMDadoda
1/30/2020 5:33:21 PM

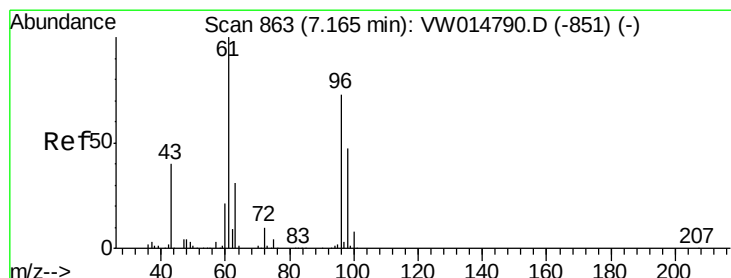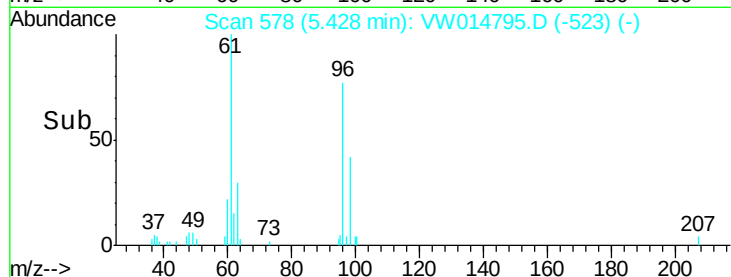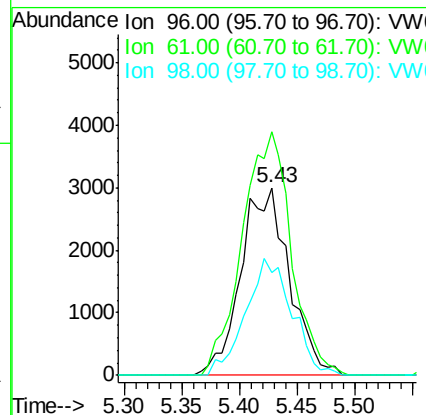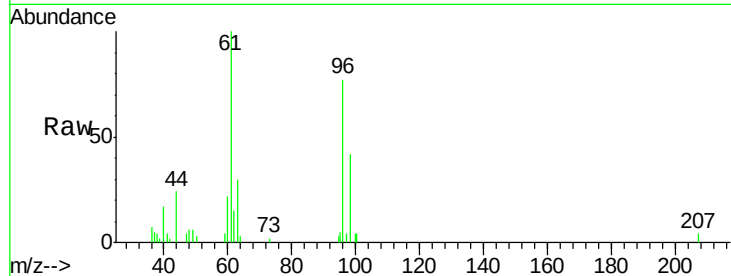

#22

cis-1,2-Dichloroethene

Concen: 22.364 ug/L




RT: 7.17 min Scan# 863




Delta R.T. -0.00 min

Lab File: VW014795.D

Acq: 29 Jan 2020 15:25

Tgt Ion:	96	Resp:	397782
Ion	Ratio	Lower	Upper
96	100		
61	136.2	94.1	174.7
98	63.2	44.9	83.3

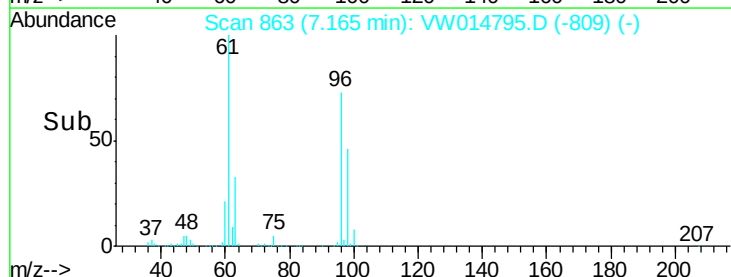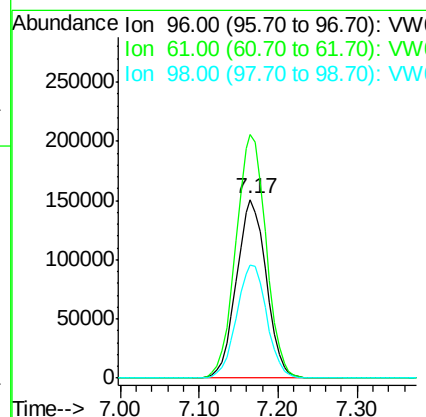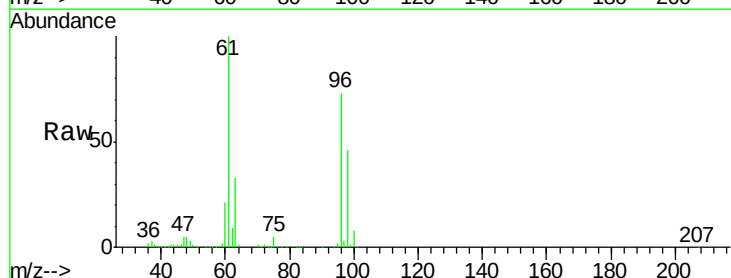

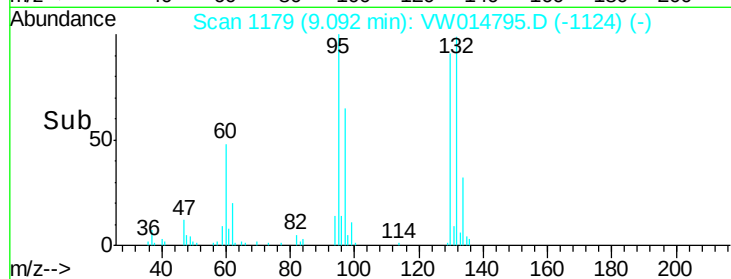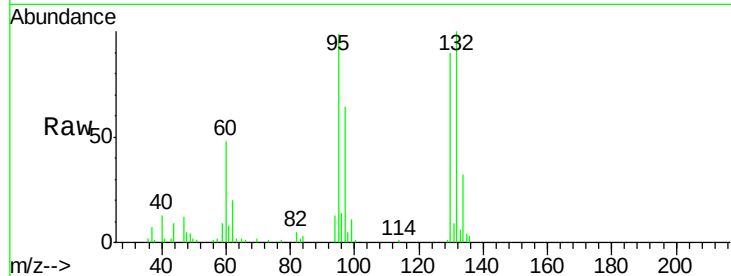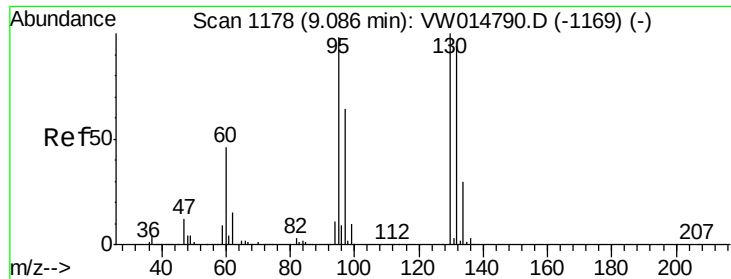

#35

Trichloroethene

Concen: 0.679 ug/L

RT: 9.09 min Scan# 1179

Delta R.T. 0.01 min

Lab File: VW014795.D

Acq: 29 Jan 2020 15:25

Tot Ion	Ratio	Resp	Lower	Upper
95	100	11809		
97	66.8		44.3	82.3
132	98.6		67.1	124.7
130	97.3		69.9	129.7

Instrument :
MSVOA_W
ClientSampleId :
C0AF0

Manual Integrations
APPROVED

MMDadoda
1/30/2020 5:33:21 PM

