
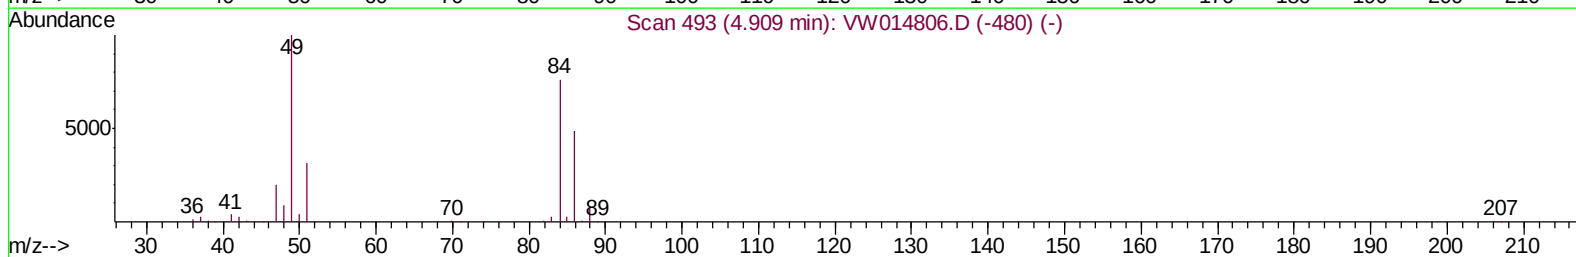
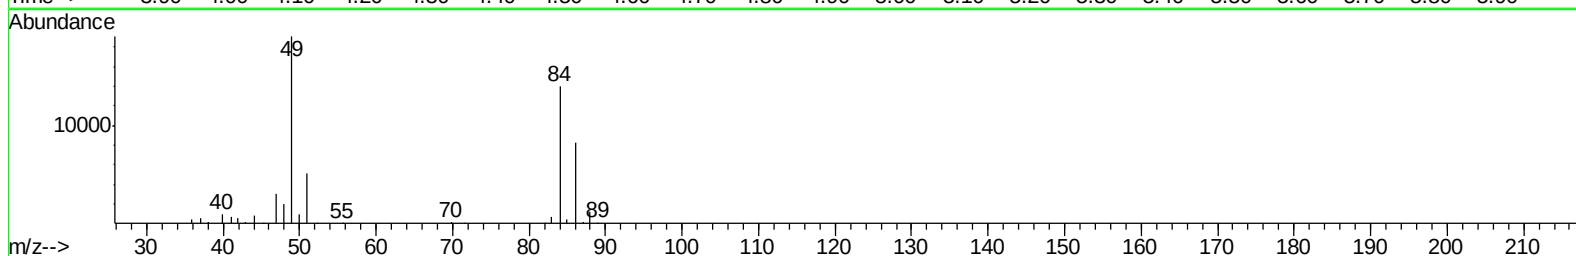


Data File : VW014816.D
Acq On : 30 Jan 2020 19:03
Operator : SY/VA
Sample : L1323-01
Misc : 5.07G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 31 01:12:18 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM012720S.M
Quant Title : VOC Analysis
QLast Update : Fri Jan 31 01:08:17 2020
Response via : Initial Calibration

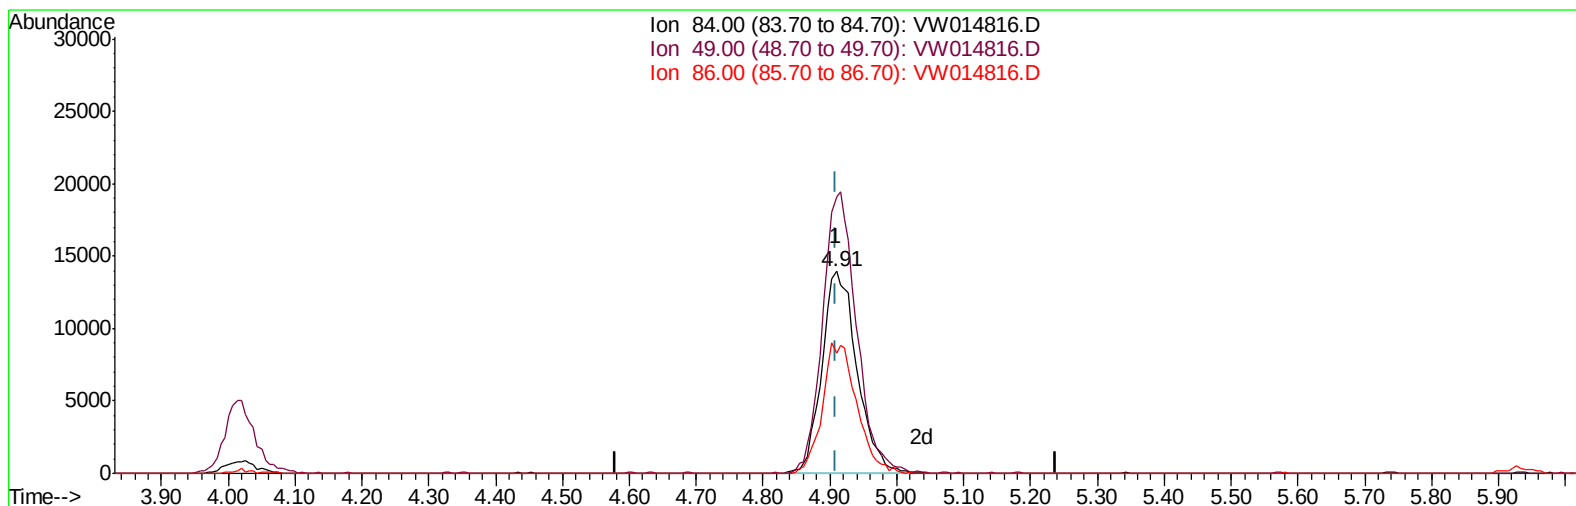

TIC: VW014816.D

(16) Methylene chloride (T)

4.909min (+0.000) 2.10ug/L m

response 50754

Ion	Exp%	Act%
84.00	100	100
49.00	129.80	136.65
86.00	62.10	59.35
0.00	0.00	0.00